

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091321\
 Data File : PD065698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2021 19:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 02:19:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	19754084	160.2E6	20.157	21.855
28)	SA Decachlor...	8.236	9.086	17528035	55373269	10.167	10.377
Target Compounds							
15)	B Endosulfa...	0.000	6.939	0	614517	N.D.	0.096 #
23)	Chlordane-1	4.393f	0.000	1053043	0	25.467	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091321\
Data File : PD065698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2021 19:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 02:19:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

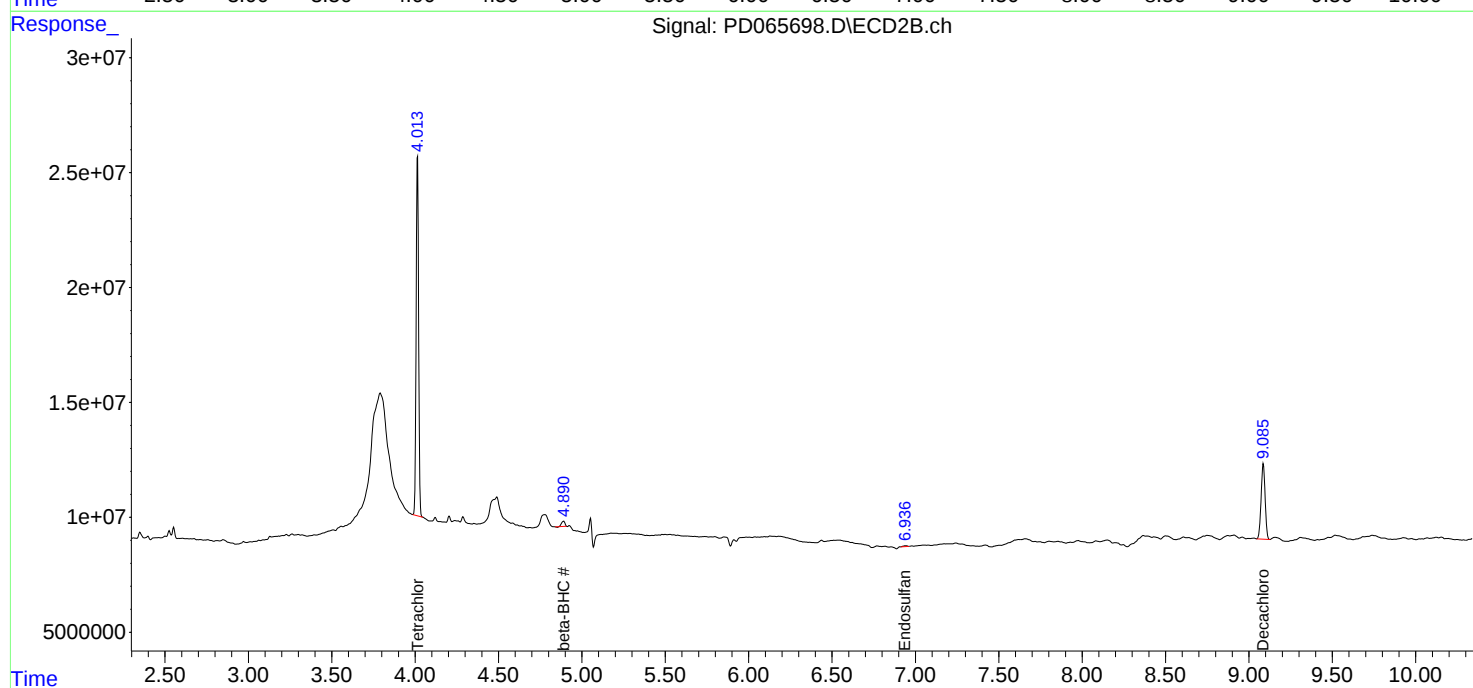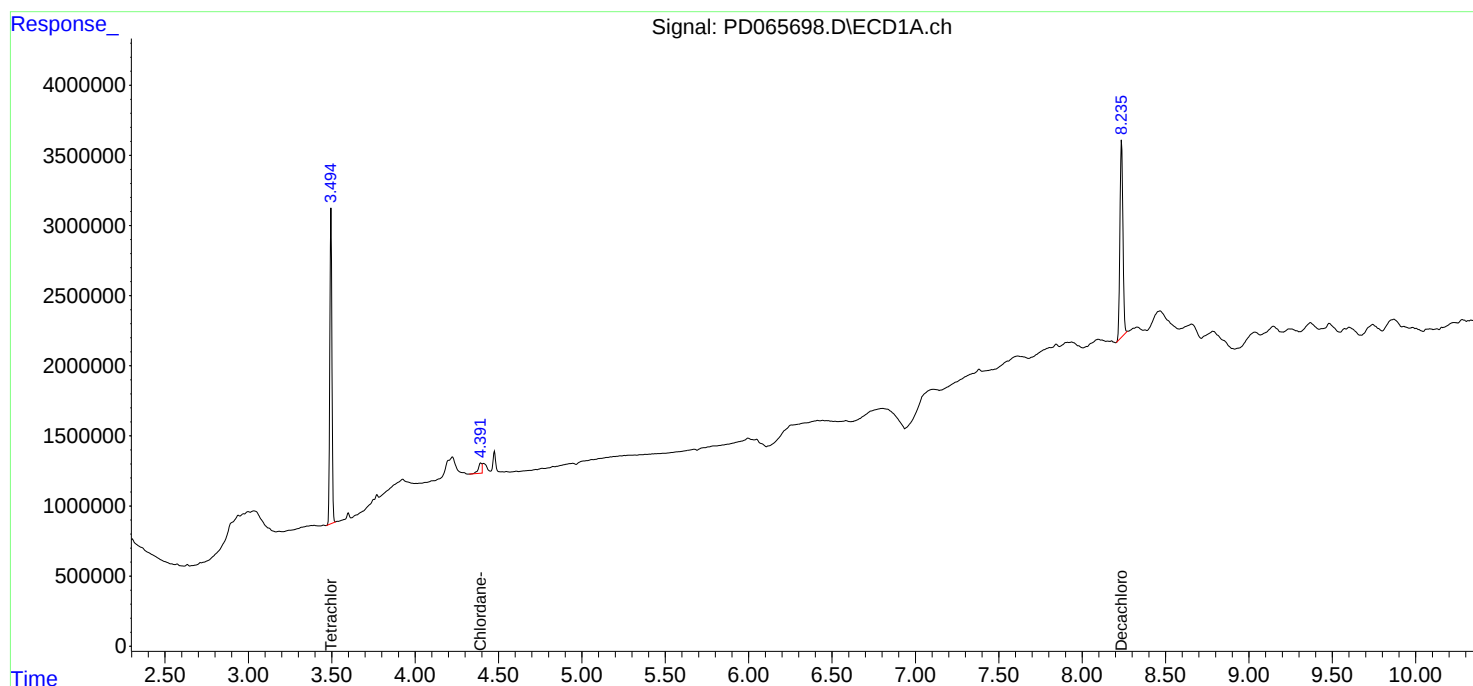


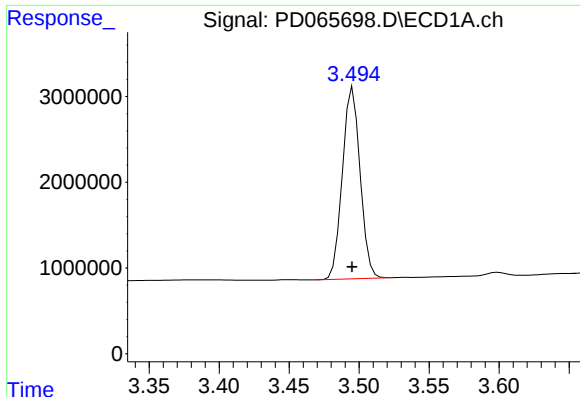

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 19754084
Conc: 20.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

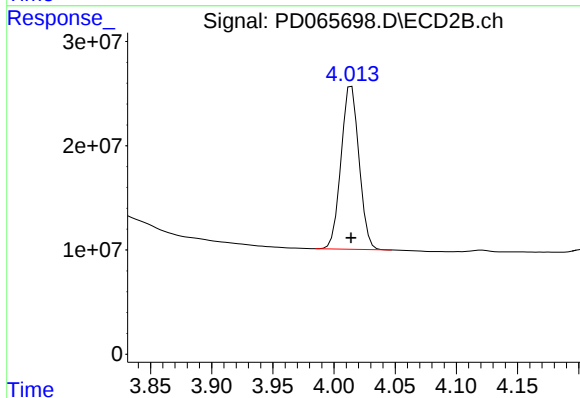


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 160182074
Conc: 21.85 ng/ml

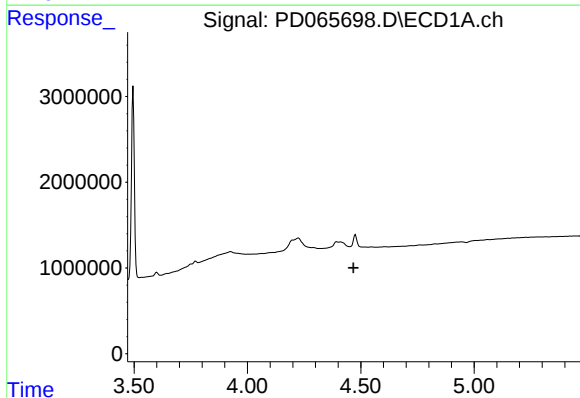


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.008 min
Response: 1662386
Conc: N.D.

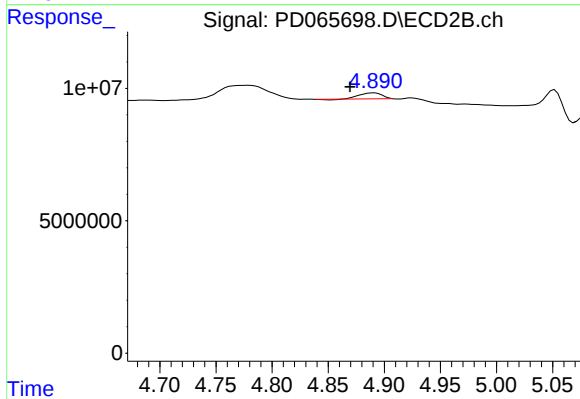

#6 beta-BHC


R.T.: 4.891 min
Delta R.T.: 0.021 min
Response: 3140058
Conc: 0.67 ng/ml

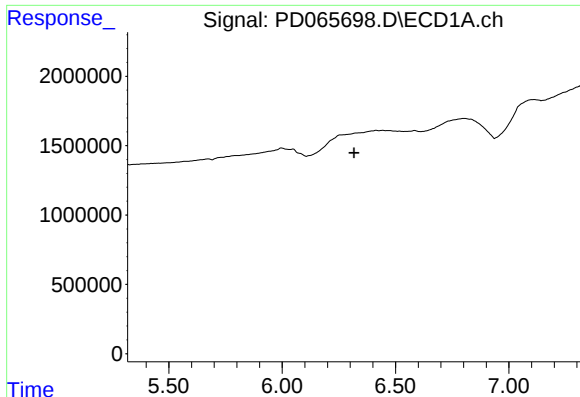

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

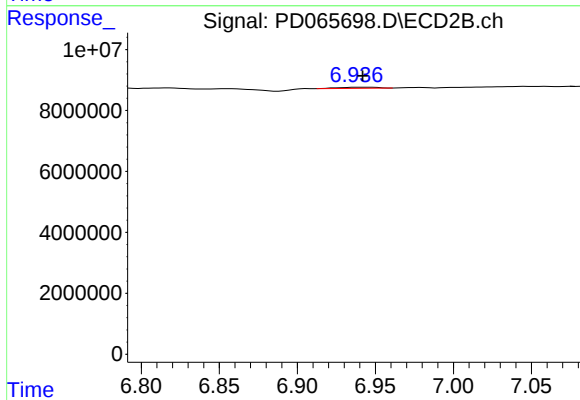


#15 Endosulfan II

R.T.: 6.939 min
Delta R.T.: -0.003 min
Response: 614517
Conc: 0.10 ng/ml

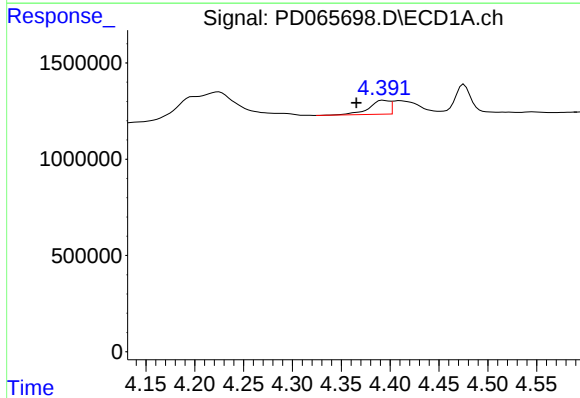


#23 Chlordane-1

R.T.: 4.393 min
Delta R.T.: 0.028 min
Response: 1053043
Conc: 25.47 ng/ml

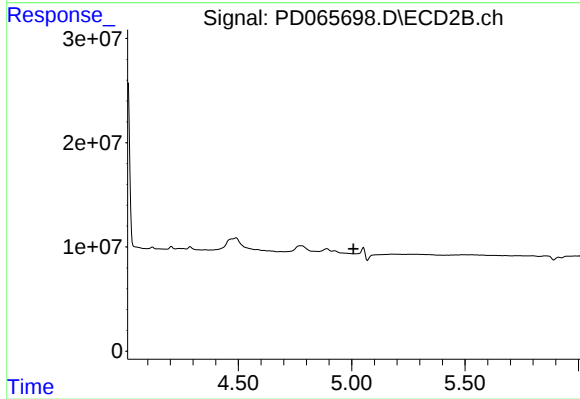

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

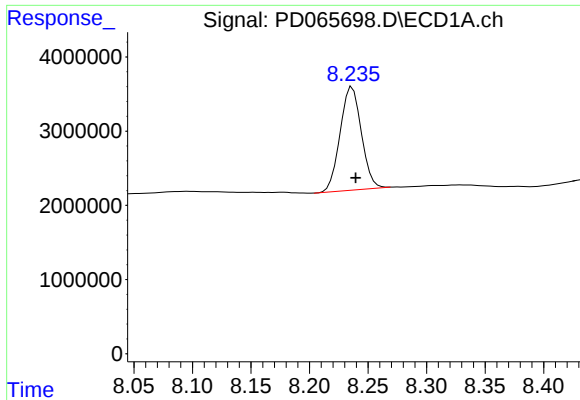

#28 Decachlorobiphenyl


R.T.: 8.236 min

Delta R.T.: -0.003 min

Response: 17528035

Conc: 10.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

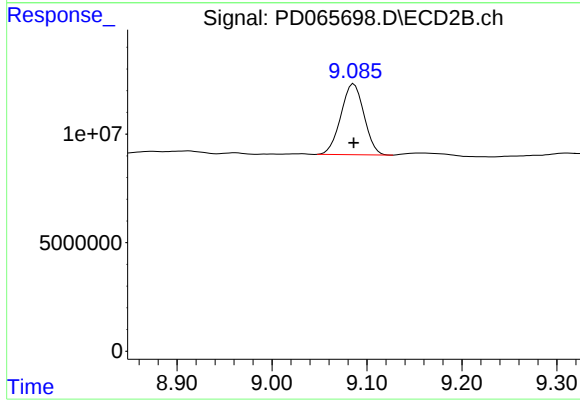

#28 Decachlorobiphenyl

R.T.: 9.086 min

Delta R.T.: 0.000 min

Response: 55373269

Conc: 10.38 ng/ml