

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091321\
 Data File : PD065685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2021 13:02
 Operator : AR\AJ
 Sample : M3719-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-04-091021

Manual Integrations
 APPROVED

mohammad
 9/14/2021 11:29:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 02:15:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.011	12553124	91240698	12.809	12.449m
28)	SA Decachlor...	8.236	9.084	20405267	60478689	11.835	11.334
Target Compounds							
17)	MA 4,4'-DDT	6.404	7.145	910209	5014631	0.661m	0.823m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091321\
Data File : PD065685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2021 13:02
Operator : AR\AJ
Sample : M3719-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
SU-04-091021


Manual Integrations
APPROVED

mohammad
9/14/2021 11:29:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 02:15:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

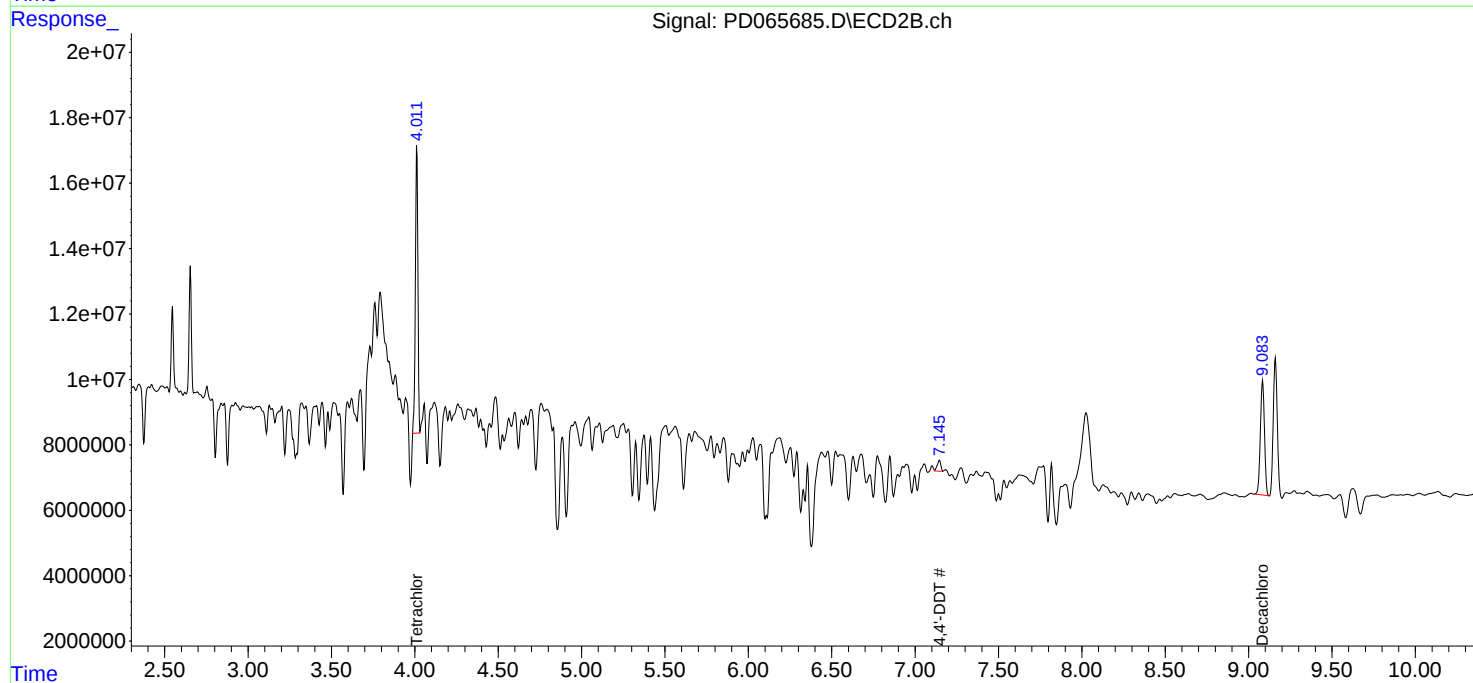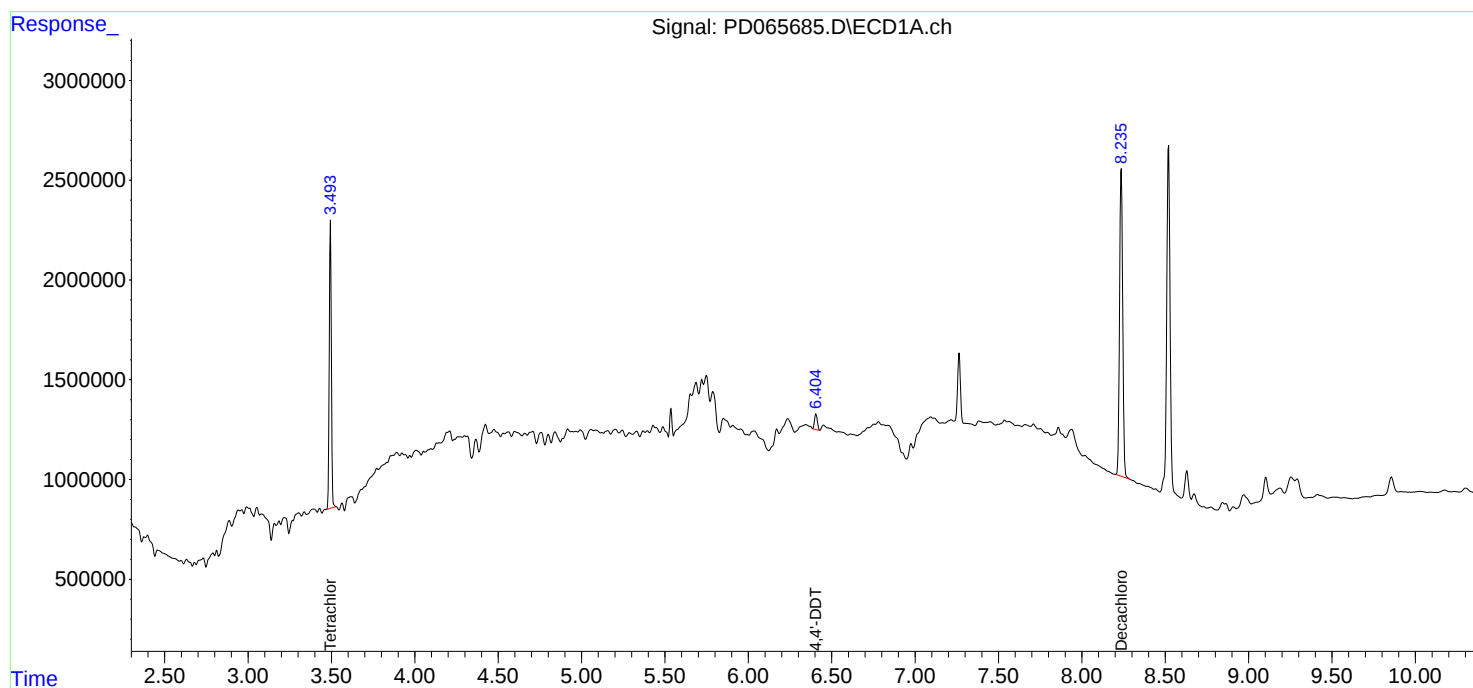

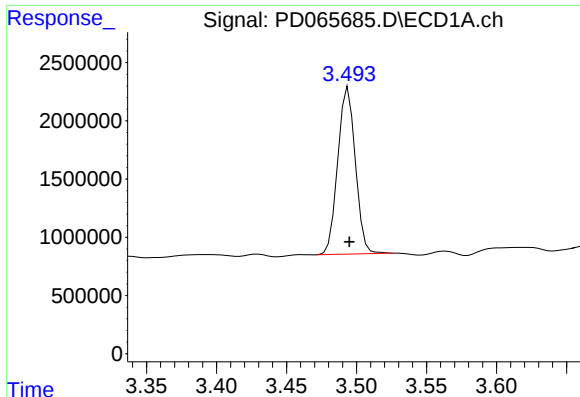


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 12553124
Conc: 12.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-04-091021


Manual Integrations
APPROVED

mohammad
9/14/2021 11:29:30 AM

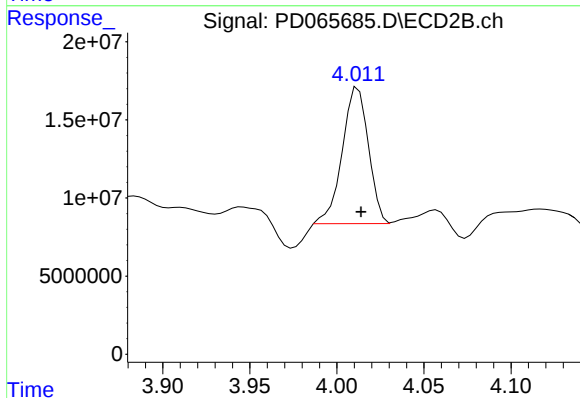


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.003 min
Response: 91240698
Conc: 12.45 ng/ml m

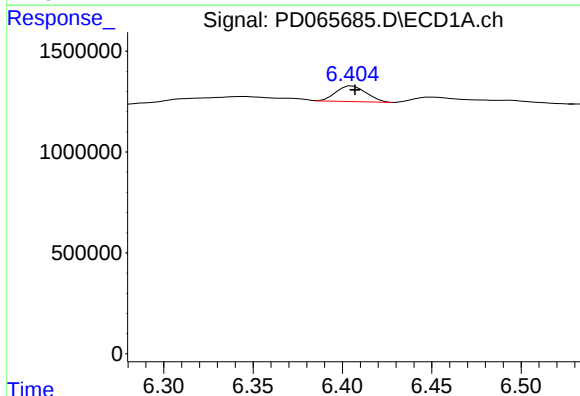


#17 4,4'-DDT

R.T.: 6.404 min
Delta R.T.: -0.003 min
Response: 910209
Conc: 0.66 ng/ml m

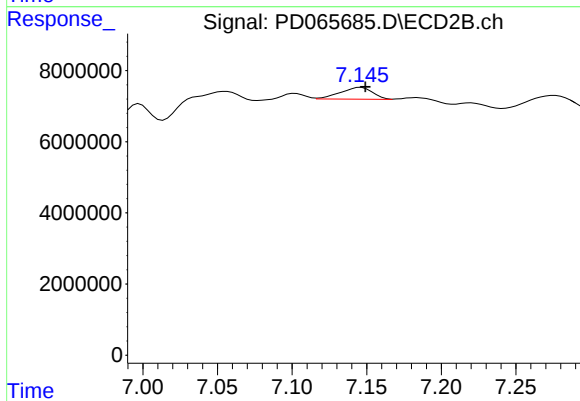

#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.004 min
Response: 5014631
Conc: 0.82 ng/ml m

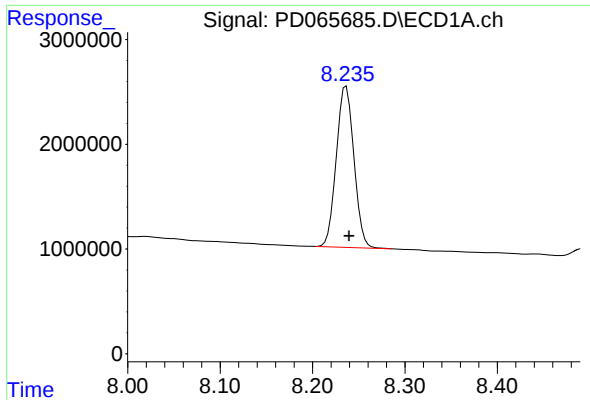


#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: -0.003 min
Response: 20405267
Conc: 11.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-04-091021

Manual Integrations
APPROVED

mohammad
9/14/2021 11:29:30 AM

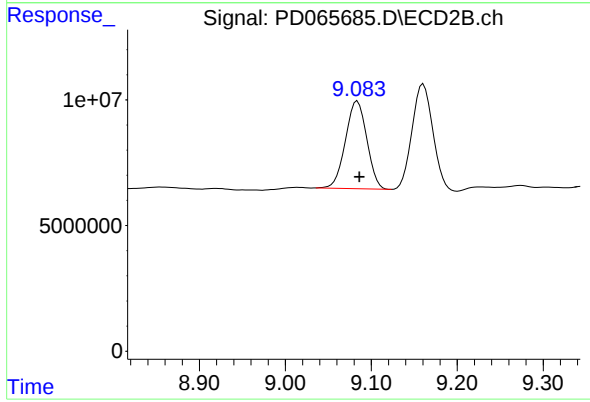

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 60478689
Conc: 11.33 ng/ml