

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091322\
 Data File : PD071857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 05:43
 Operator : AR\AJ
 Sample : N4572-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSC-124035

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/14/2022
 Supervised By : Ankita Jodhani 09/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 07:09:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.804	3.561	44208237	350.5E6	18.079	12.213m#
2) SA Decachlor...	7.994	9.088	29470957	108.2E6	11.698	11.634

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091322\
Data File : PD071857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 05:43
Operator : AR\AJ
Sample : N4572-07
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PSC-124035


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/14/2022
Supervised By : Ankita Jodhani 09/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 07:09:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

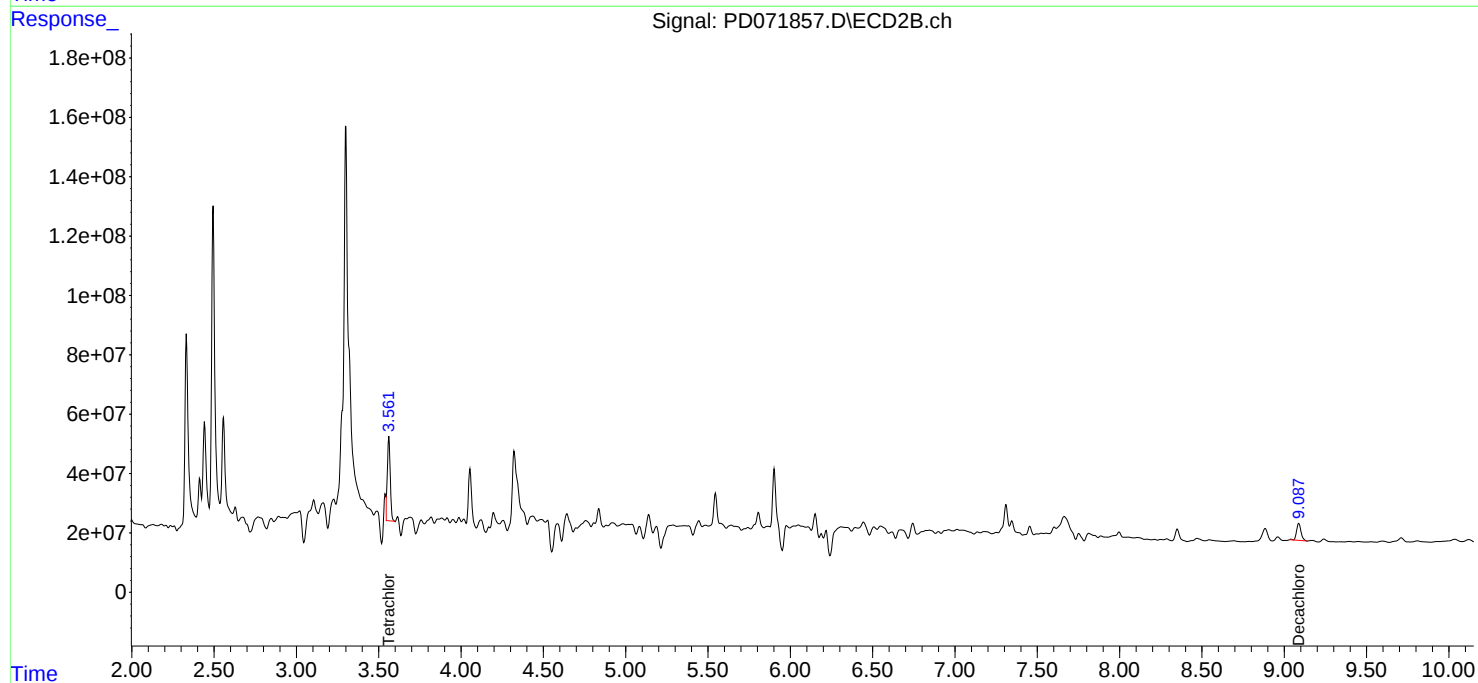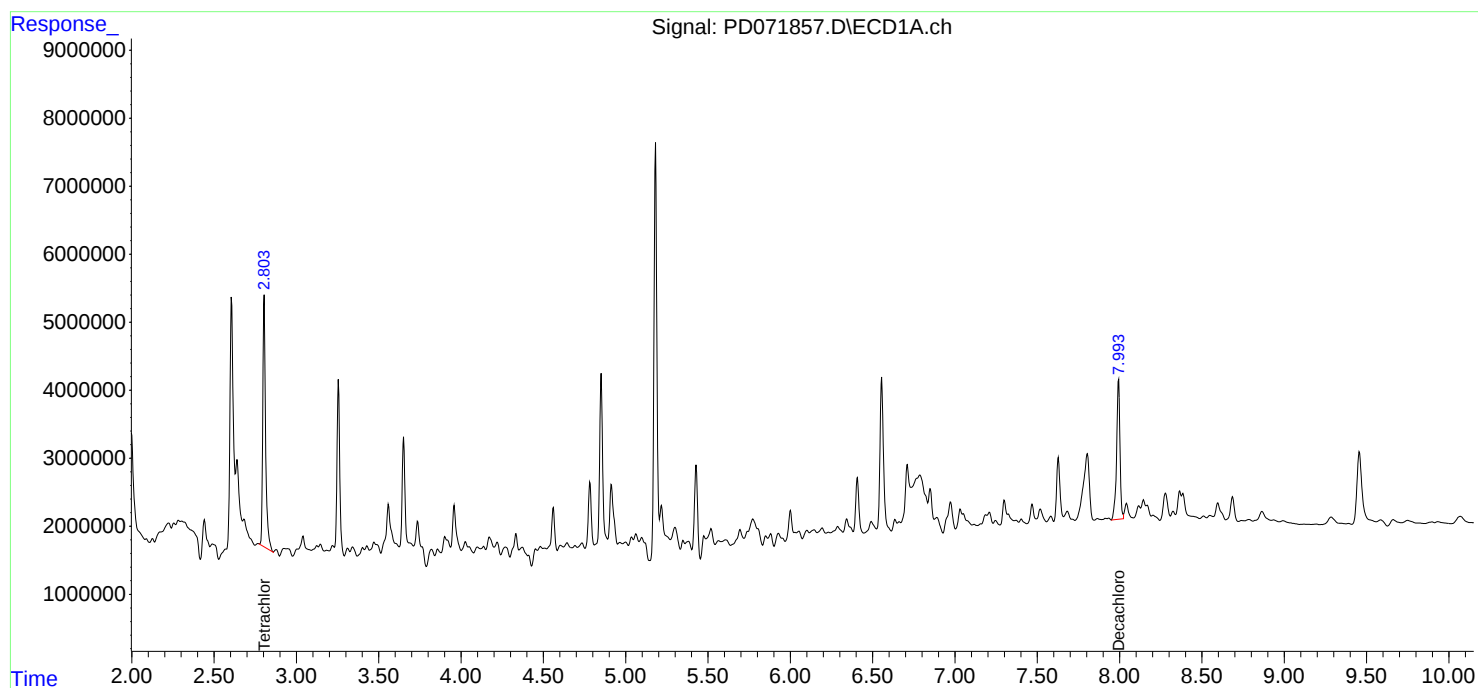

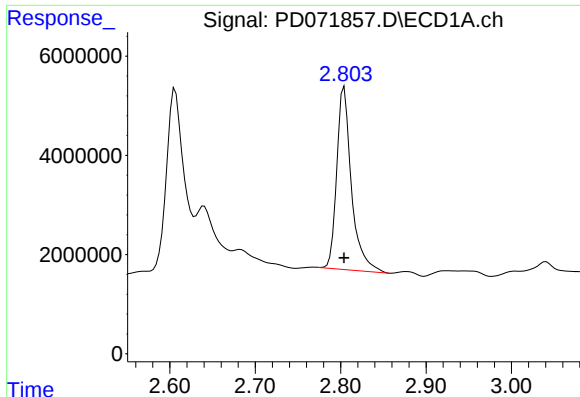


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 44208237
Conc: 18.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSC-124035


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/14/2022
Supervised By :Ankita Jodhani 09/14/2022

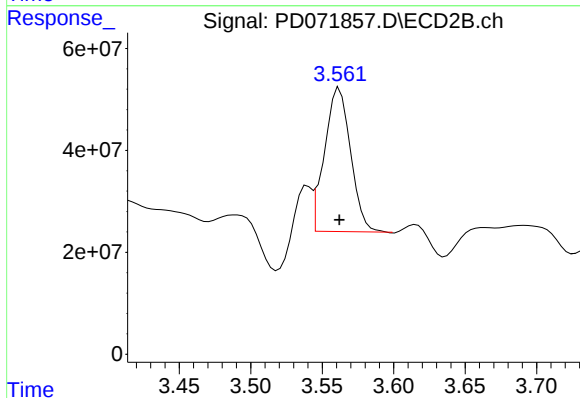


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.001 min
Response: 350472988
Conc: 12.21 ng/ml m

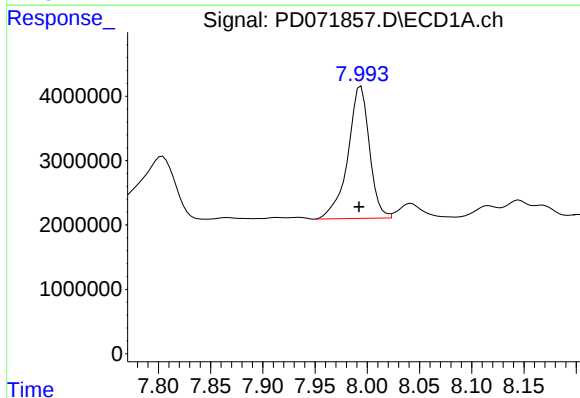

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: 0.002 min
Response: 29470957
Conc: 11.70 ng/ml

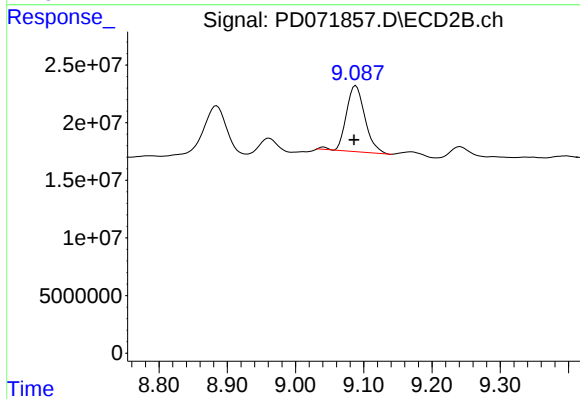

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.002 min
Response: 108160864
Conc: 11.63 ng/ml