

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091323\
 Data File : PD077908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 14:13
 Operator : AR\AJ
 Sample : PB155487BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 22:09:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.760	50176969	30826343	19.773	20.858
2)	SA Decachlor...	9.095	7.903	74016690	39362571	23.694	24.305
Target Compounds							
3)	MA gamma-BHC...	0.000	3.603	0	352886	N.D.	0.163
4)	MA Heptachlor	0.000	3.923	0	36579	N.D.	<MDL
6)	B beta-BHC	0.000	3.893	0	99375	N.D.	0.101


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091323\
Data File : PD077908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 14:13
Operator : AR\AJ
Sample : PB155487BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 22:09:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

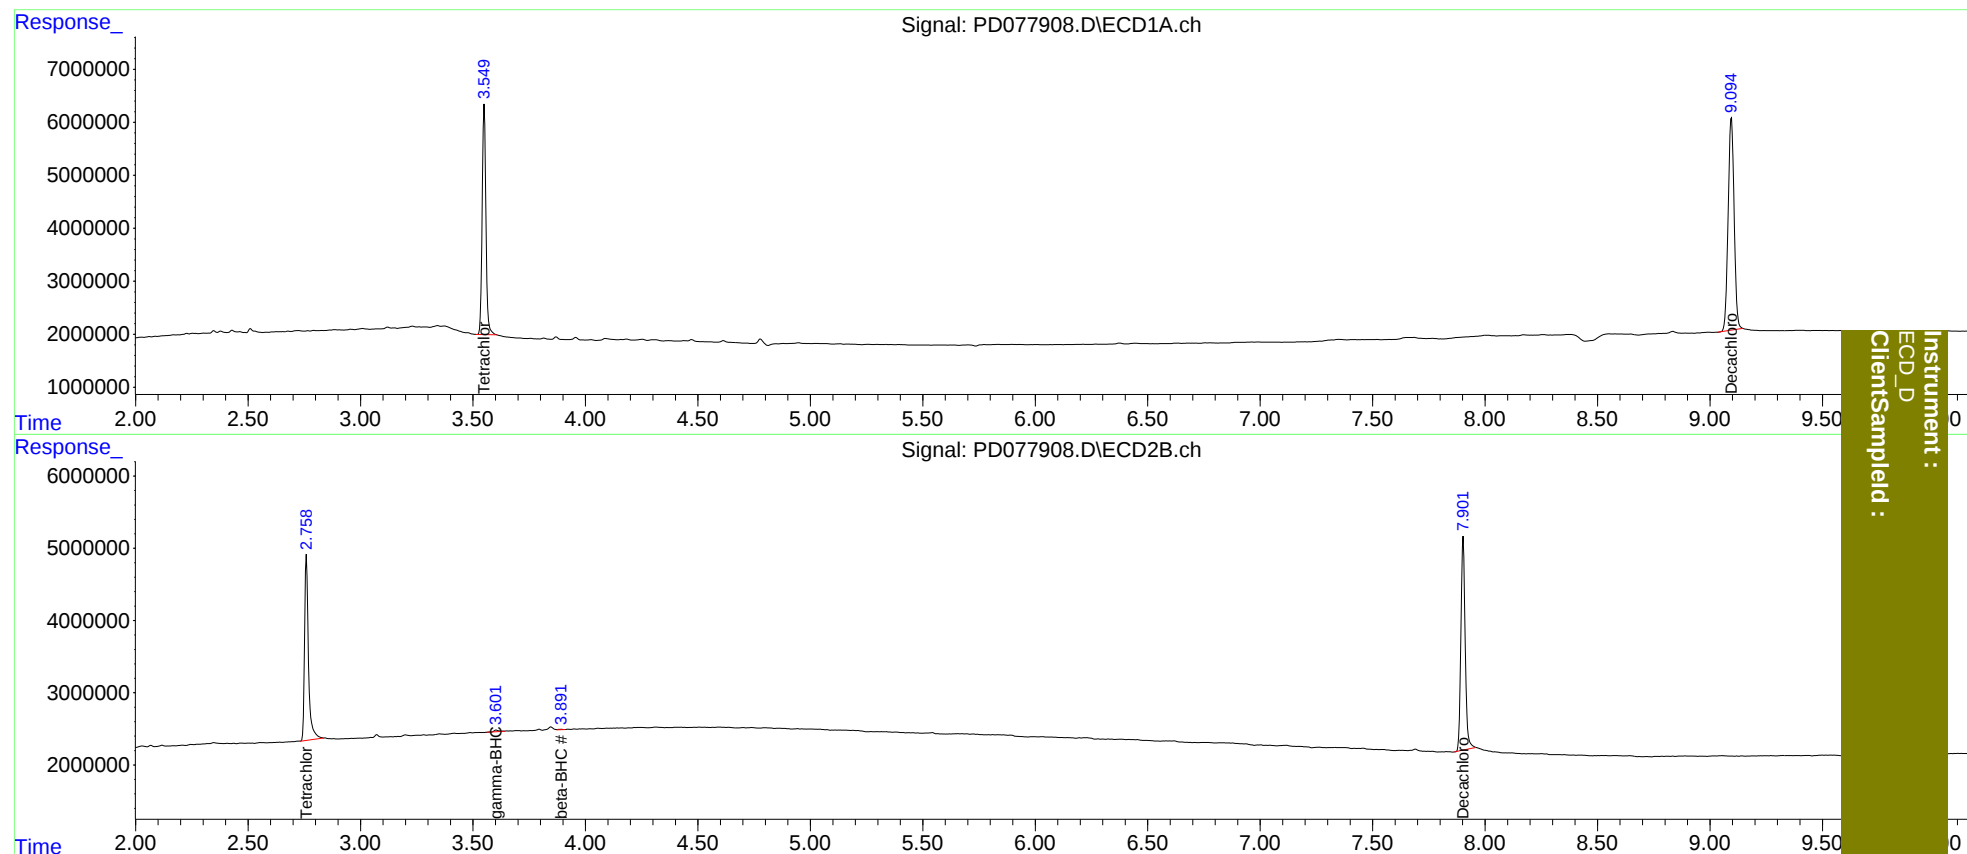


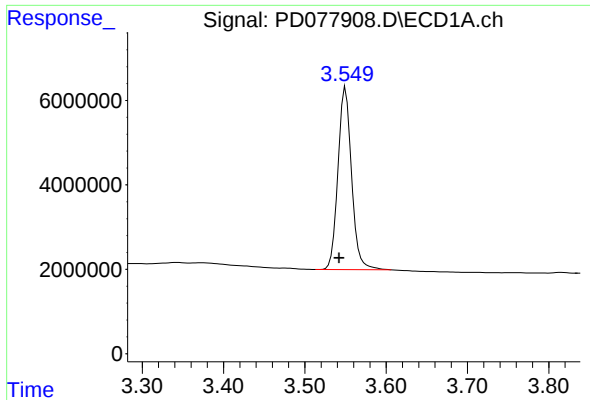

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.008 min
Response: 50176969
Conc: 19.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

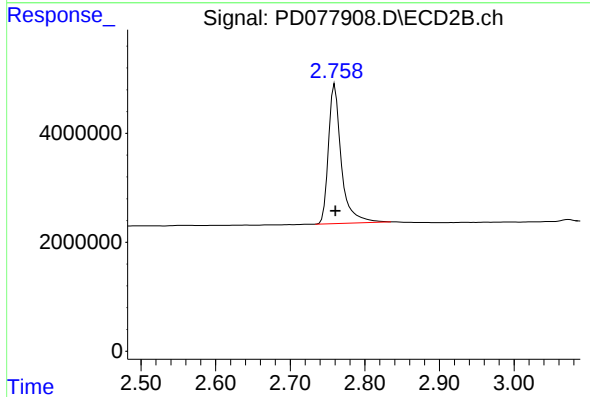


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 30826343
Conc: 20.86 ng/ml

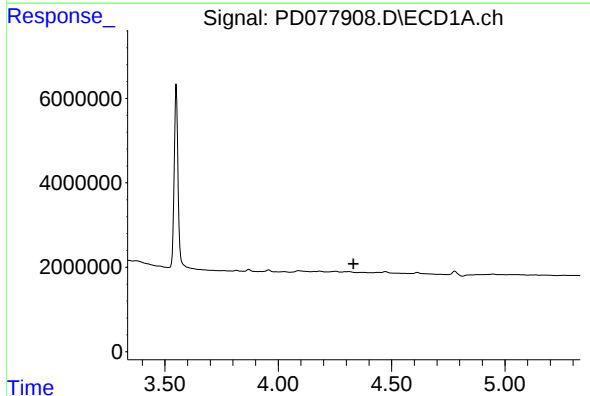

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.332 min
Response: 0
Conc: N.D.

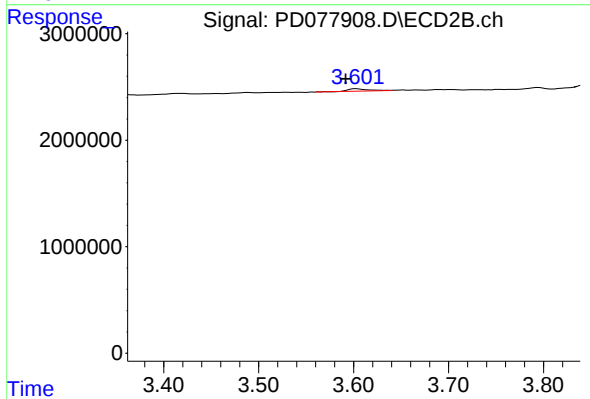

#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.011 min
Response: 352886
Conc: 0.16 ng/ml

