

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091323\
 Data File : PD077917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 16:16
 Operator : AR\AJ
 Sample : 04378-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 22:11:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	52209888	32734070	20.574	22.149
27)	SA Decachlor...	9.081	7.898	69293552	36367413	22.182	22.456
Target Compounds							
3)	MA gamma-BHC...	0.000	3.602	0	56400	N.D.	<MDL
6)	B beta-BHC	0.000	3.843f	0	605852	N.D.	0.613
7)	B delta-BHC	0.000	4.082f	0	71400	N.D.	<MDL
8)	B Heptachlo...	5.710	0.000	6769601	0	1.752	N.D. #
9)	A Endosulfan I	0.000	5.054	0	5386697	N.D.	3.001
10)	B trans-Chl...	0.000	4.944	0	224742	N.D.	0.113
11)	B cis-Chlor...	0.000	5.054	0	5386697	N.D.	2.634
14)	MA Endrin	0.000	5.688f	0	146855	N.D.	<MDL
22)	Toxaphene-1	0.000	4.981	0	381705	N.D.	36.570
23)	Toxaphene-2	0.000	5.688	0	146855	N.D.	12.178


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091323\
Data File : PD077917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 16:16
Operator : AR\AJ
Sample : 04378-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 22:11:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

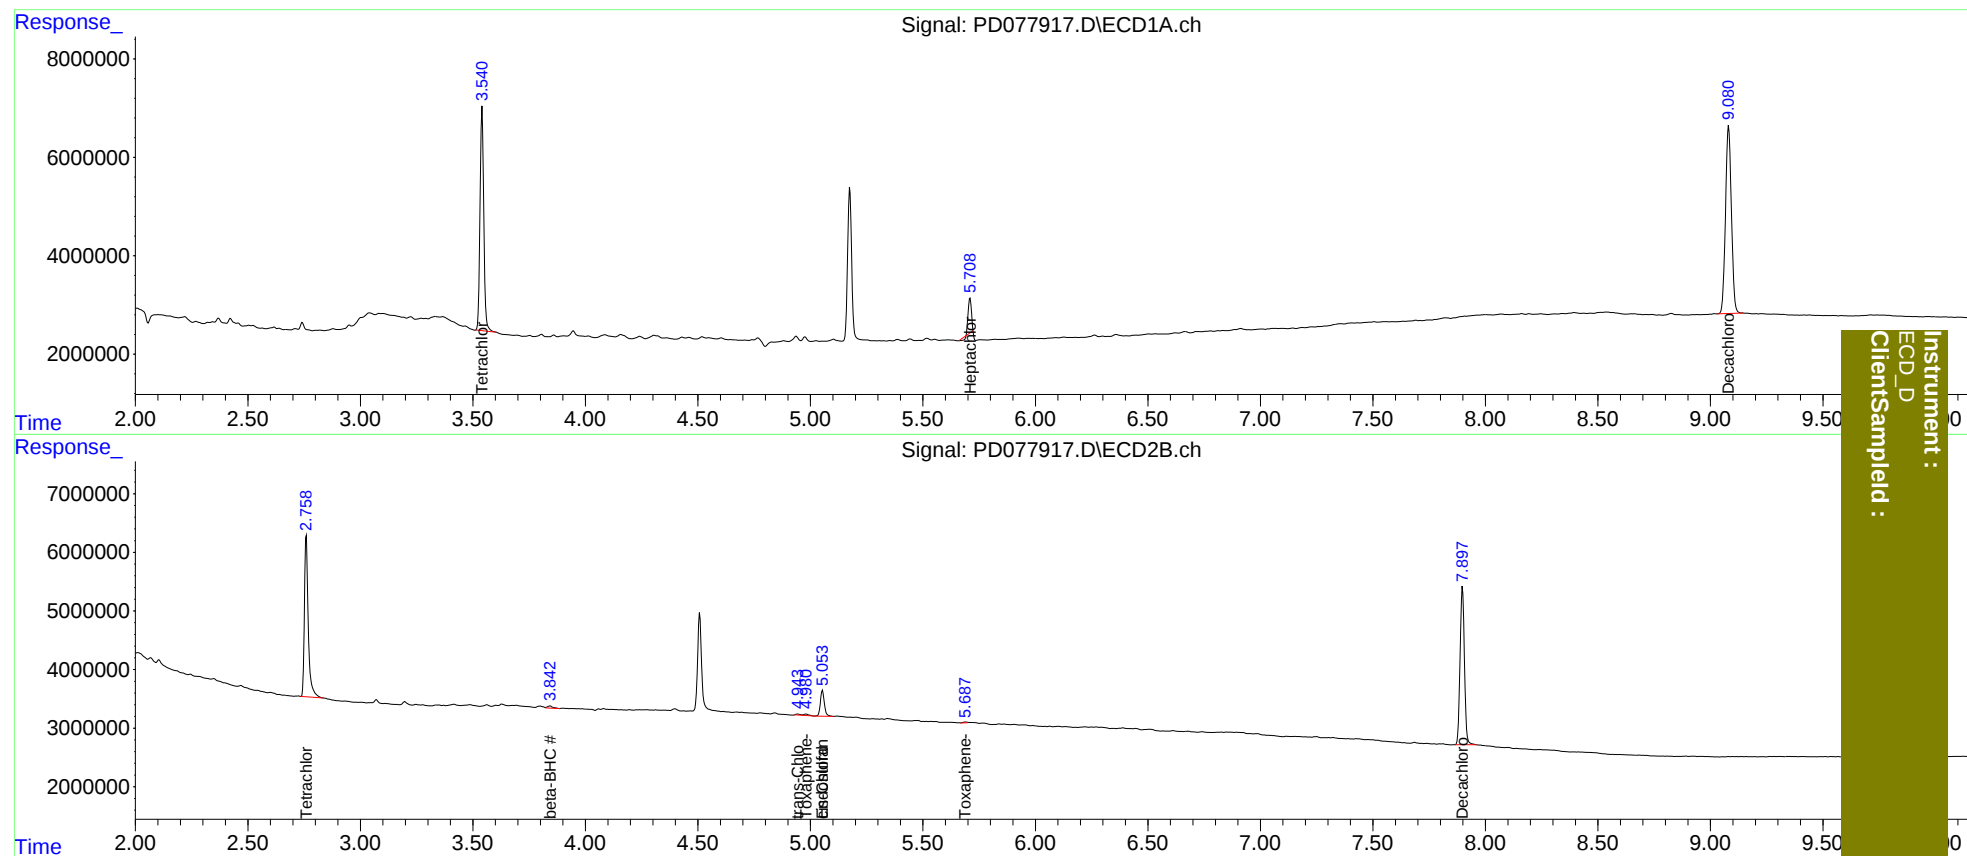


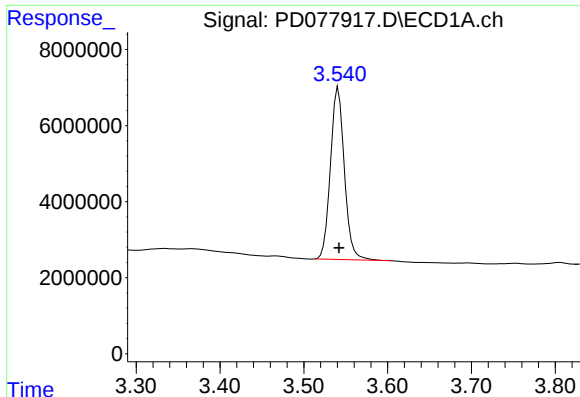

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 52209888
Conc: 20.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

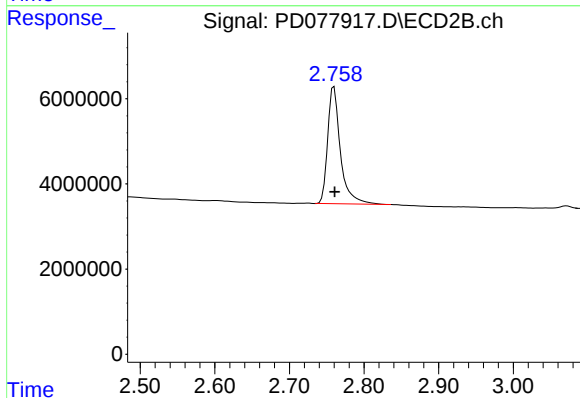


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 32734070
Conc: 22.15 ng/ml

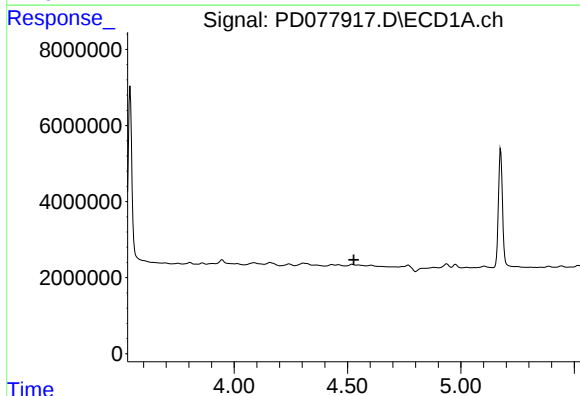


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

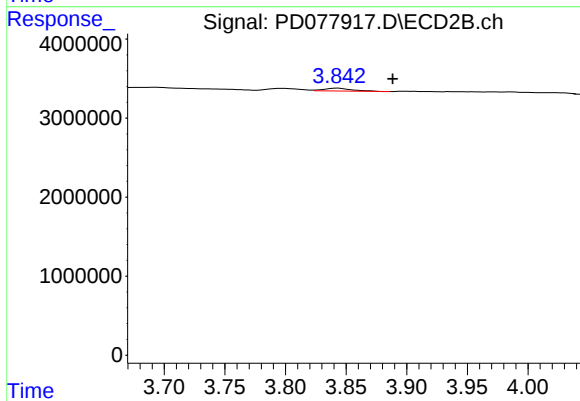

#6 beta-BHC


R.T.: 3.843 min
Delta R.T.: -0.045 min
Response: 605852
Conc: 0.61 ng/ml

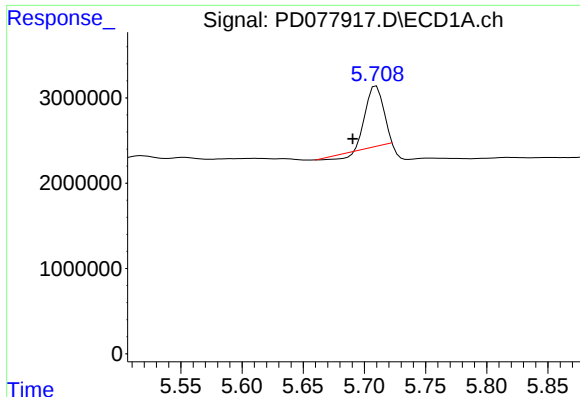

#8 Heptachlor epoxide


R.T.: 5.710 min
Delta R.T.: 0.019 min
Response: 6769601
Conc: 1.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

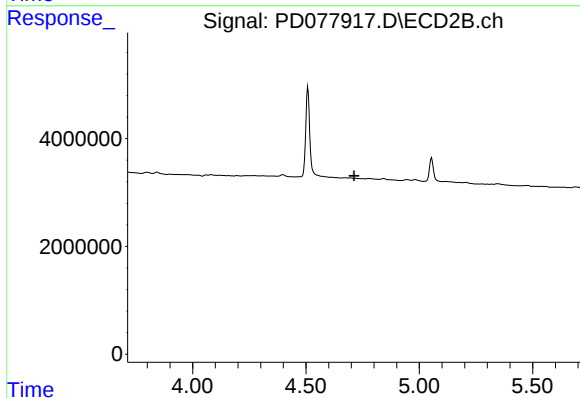


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.712 min
Response: 0
Conc: N.D.

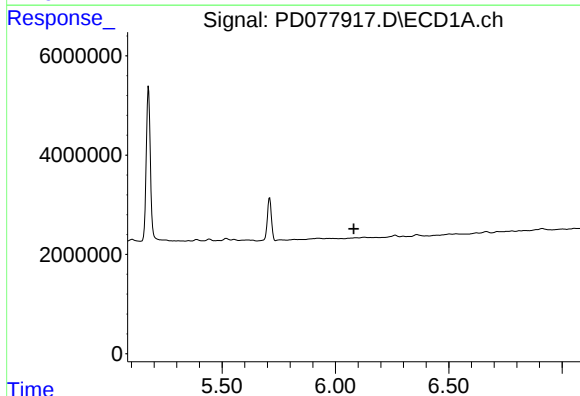


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

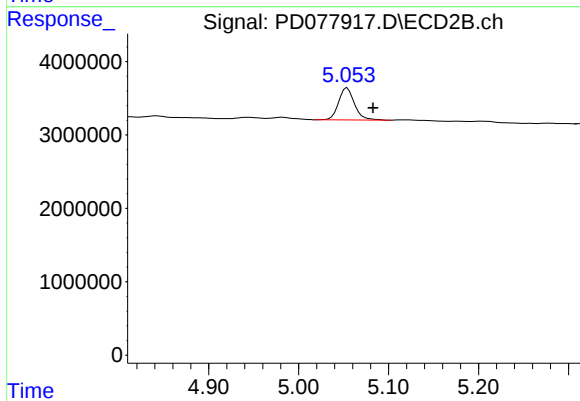

#9 Endosulfan I


R.T.: 5.054 min
Delta R.T.: -0.029 min
Response: 5386697
Conc: 3.00 ng/ml

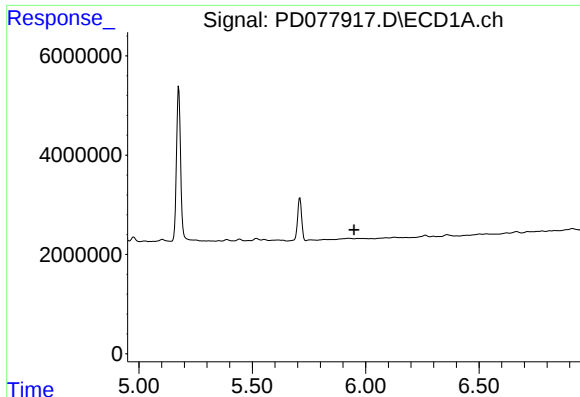

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

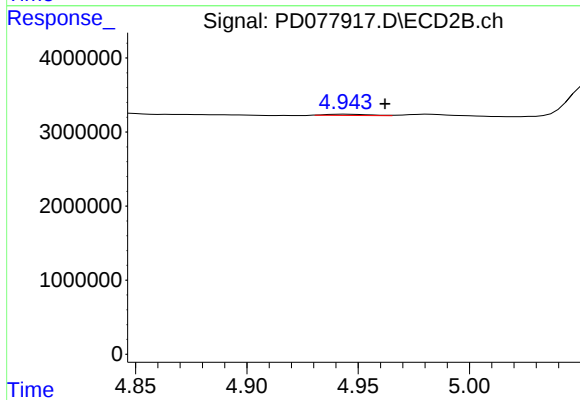


#10 trans-Chlordane

R.T.: 4.944 min
Delta R.T.: -0.018 min
Response: 224742
Conc: 0.11 ng/ml

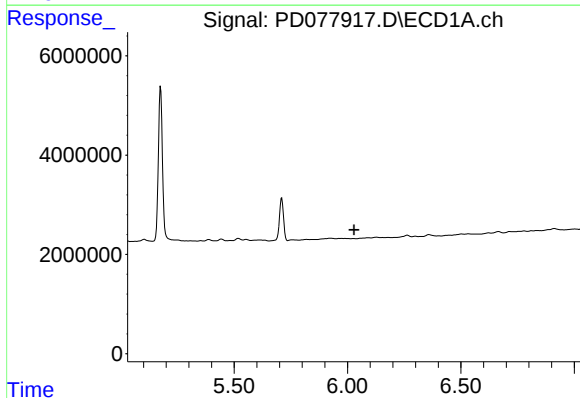


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.029 min
Response: 0
Conc: N.D.

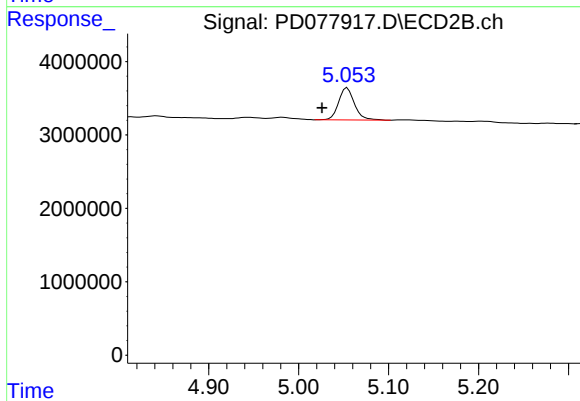

#11 cis-Chlordane


R.T.: 5.054 min
Delta R.T.: 0.028 min
Response: 5386697
Conc: 2.63 ng/ml

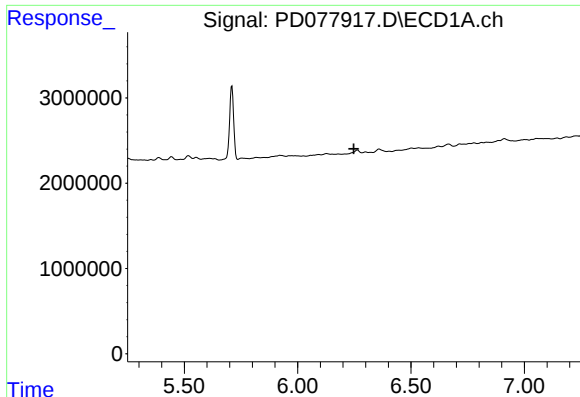

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 6.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

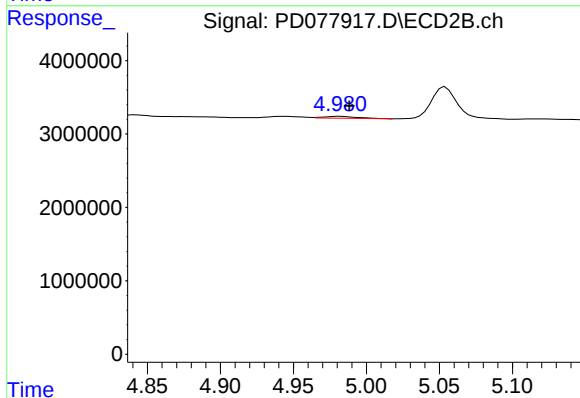


#22 Toxaphene-1

R.T.: 4.981 min
Delta R.T.: -0.007 min
Response: 381705
Conc: 36.57 ng/ml

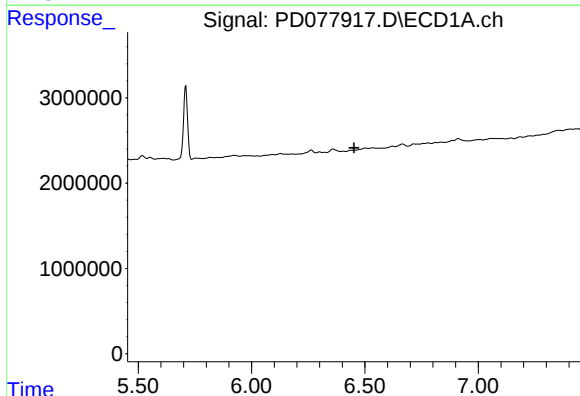


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.452 min
Response: 0
Conc: N.D.

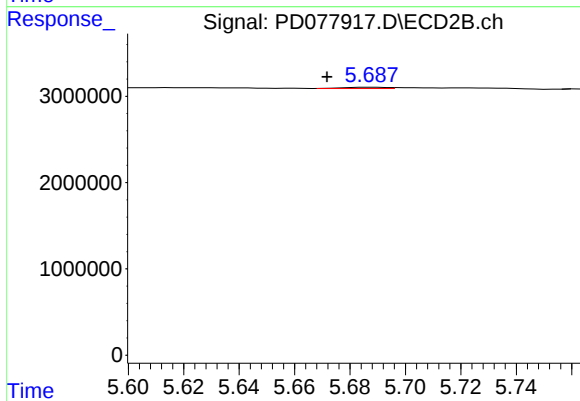

#23 Toxaphene-2


R.T.: 5.688 min
Delta R.T.: 0.016 min
Response: 146855
Conc: 12.18 ng/ml

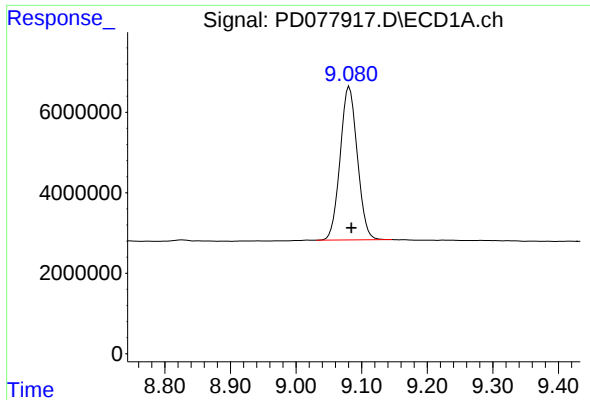

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.003 min
Response: 69293552
Conc: 22.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

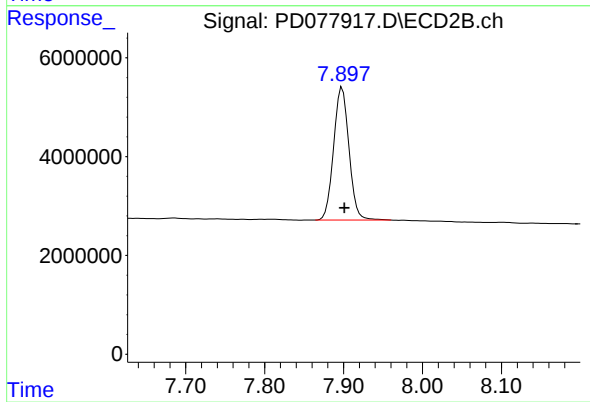

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 36367413
Conc: 22.46 ng/ml