

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091324\
 Data File : PD085087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2024 16:59
 Operator : AR\AJ
 Sample : P3877-16RXRE
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVZ5RXRE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/15/2024
 Supervised By : Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 00:50:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.915	21514711	277.6E6	21.272m	78.451m#
2) SA Decachlor...	9.035	8.104	25098726	59821966	19.218	17.204
Target Compounds						
2) A alpha-BHC	3.982	3.414	6396358	20329559	3.762	4.010
9) A Endosulfan I	6.061	5.278	5284266	10748074	3.841m	2.804 #
10) B trans-Chl...	5.910	5.144	1777182	11003759	1.260m	2.675m#
13) MA Dieldrin	6.326	5.544	1557713	6760900	1.056m	1.574m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091324\
Data File : PD085087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2024 16:59
Operator : AR\AJ
Sample : P3877-16RXRE
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 00:50:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

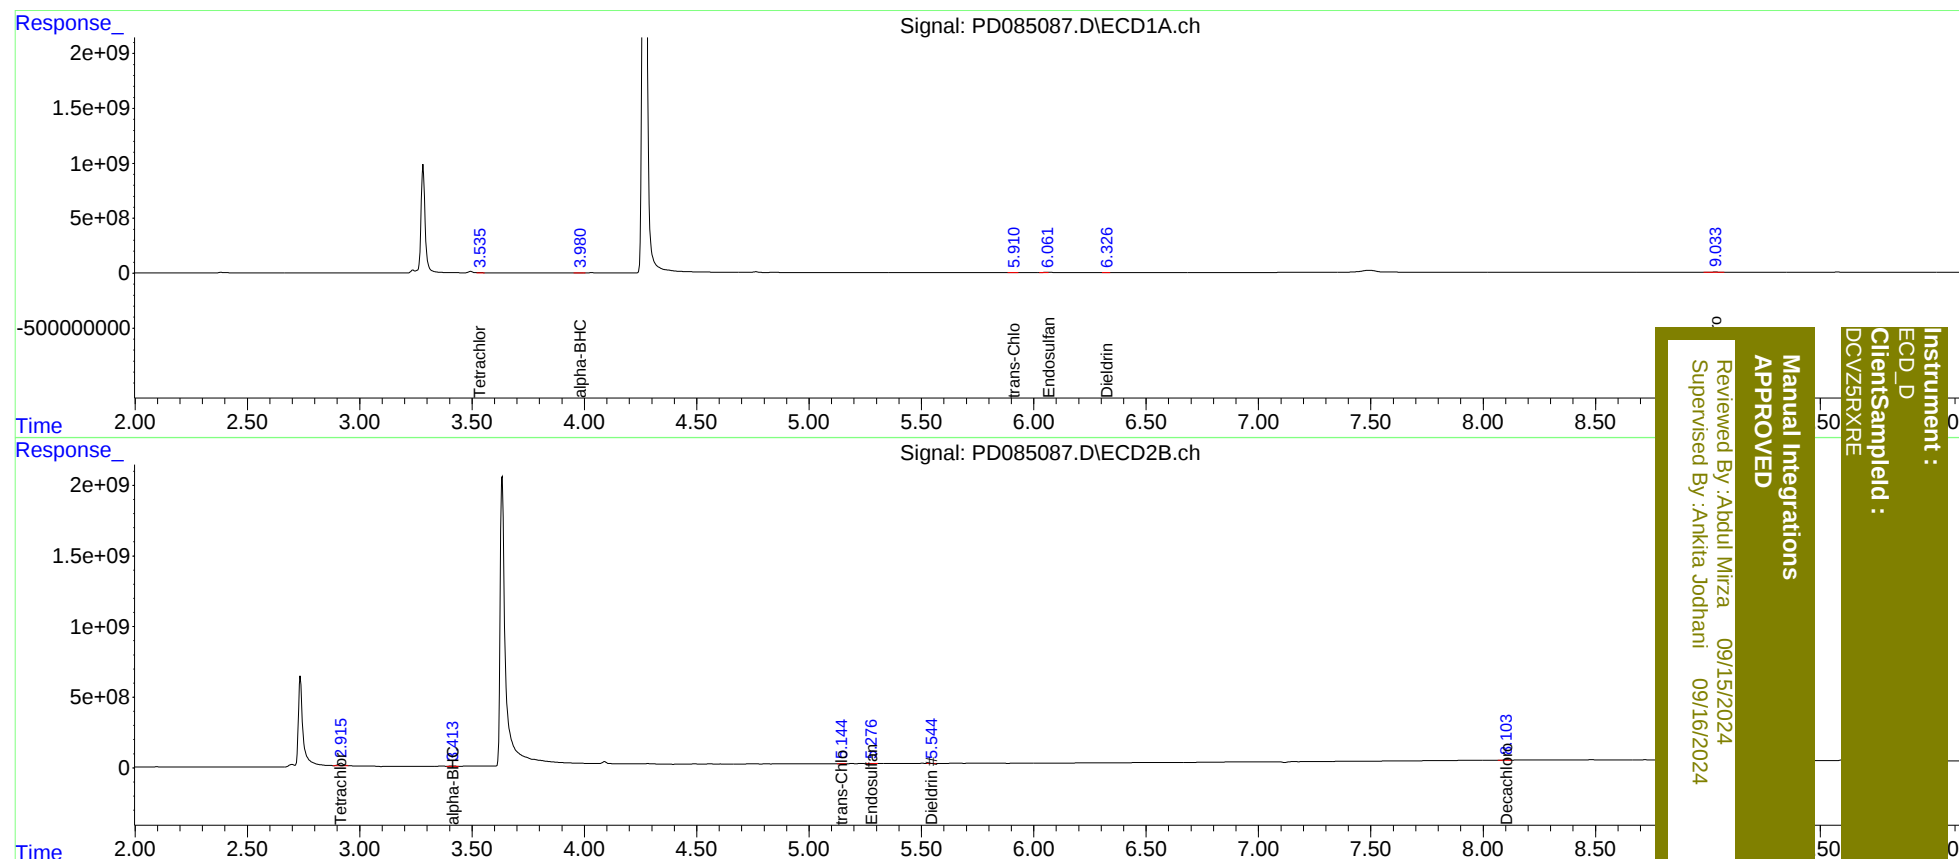

Reviewed By: Abdul Mirza 09/15/2024
Supervised By: Ankita Jodhani 09/16/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DCVZ5RXRE