

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE



## Manual IntegrationsAPPROVED

Reviewed By :Abdul  
Mirza  
09/15/2024

Supervised By :Ankita  
Jodhani  
09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

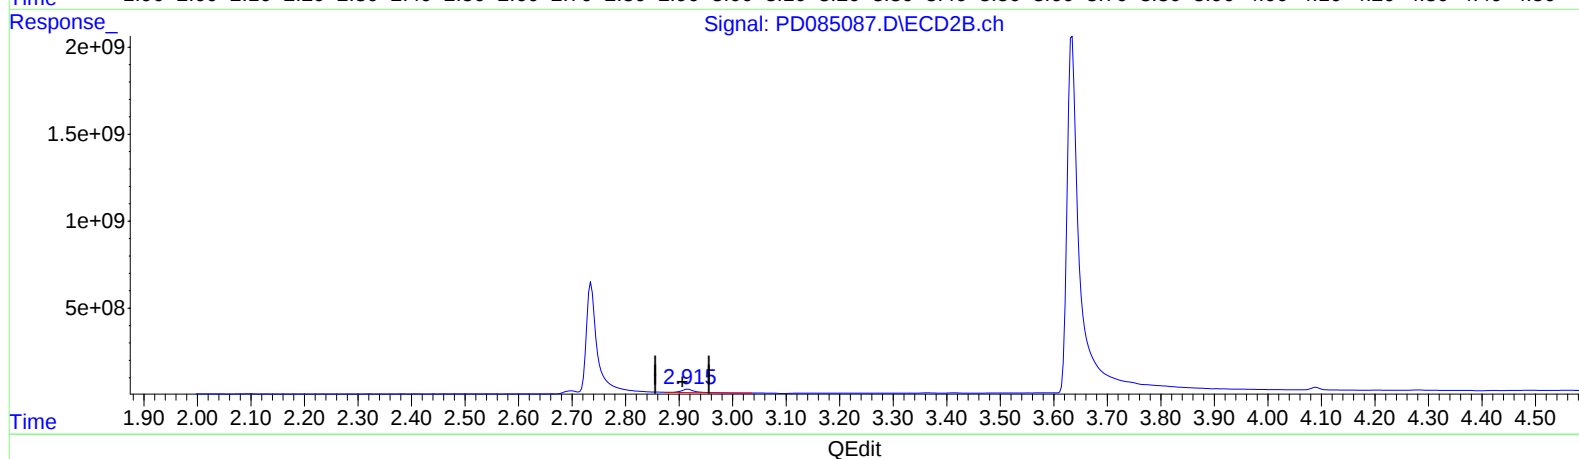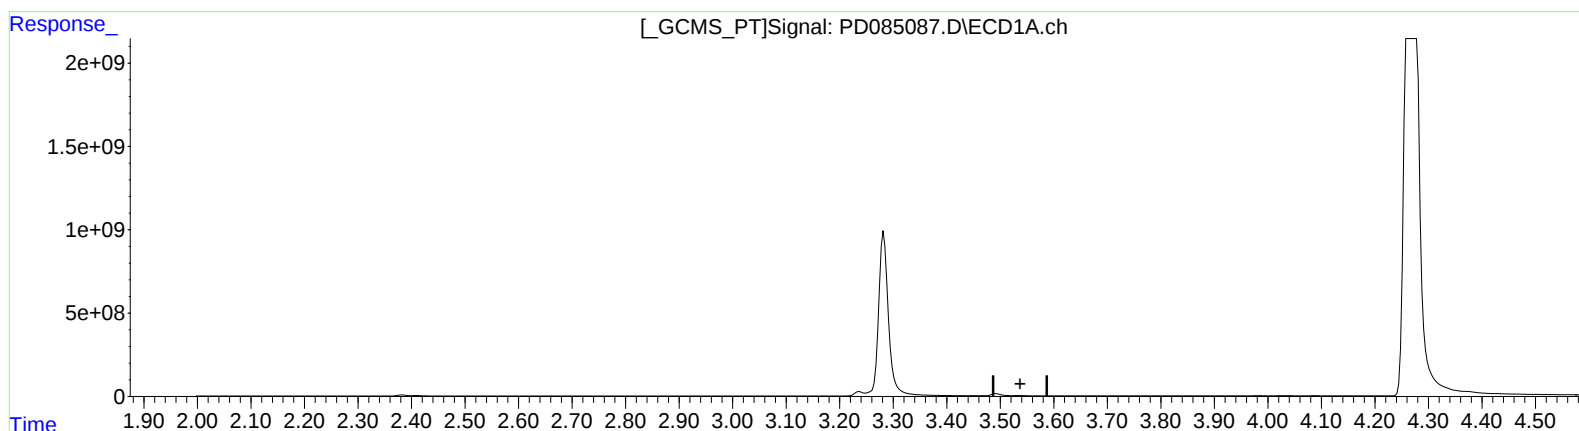

(1) Tetrachloro-m-xylene (SA)

3.536min -136.929 ng/ml

response -138490350

(1) Tetrachloro-m-xylene #2 (SA)

2.916min 92.503 ng/ml

response 327348961

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE

## Manual IntegrationsAPPROVED

Reviewed By :Abdul

Mirza

09/15/2024


Supervised By :Ankita

Jodhani

09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

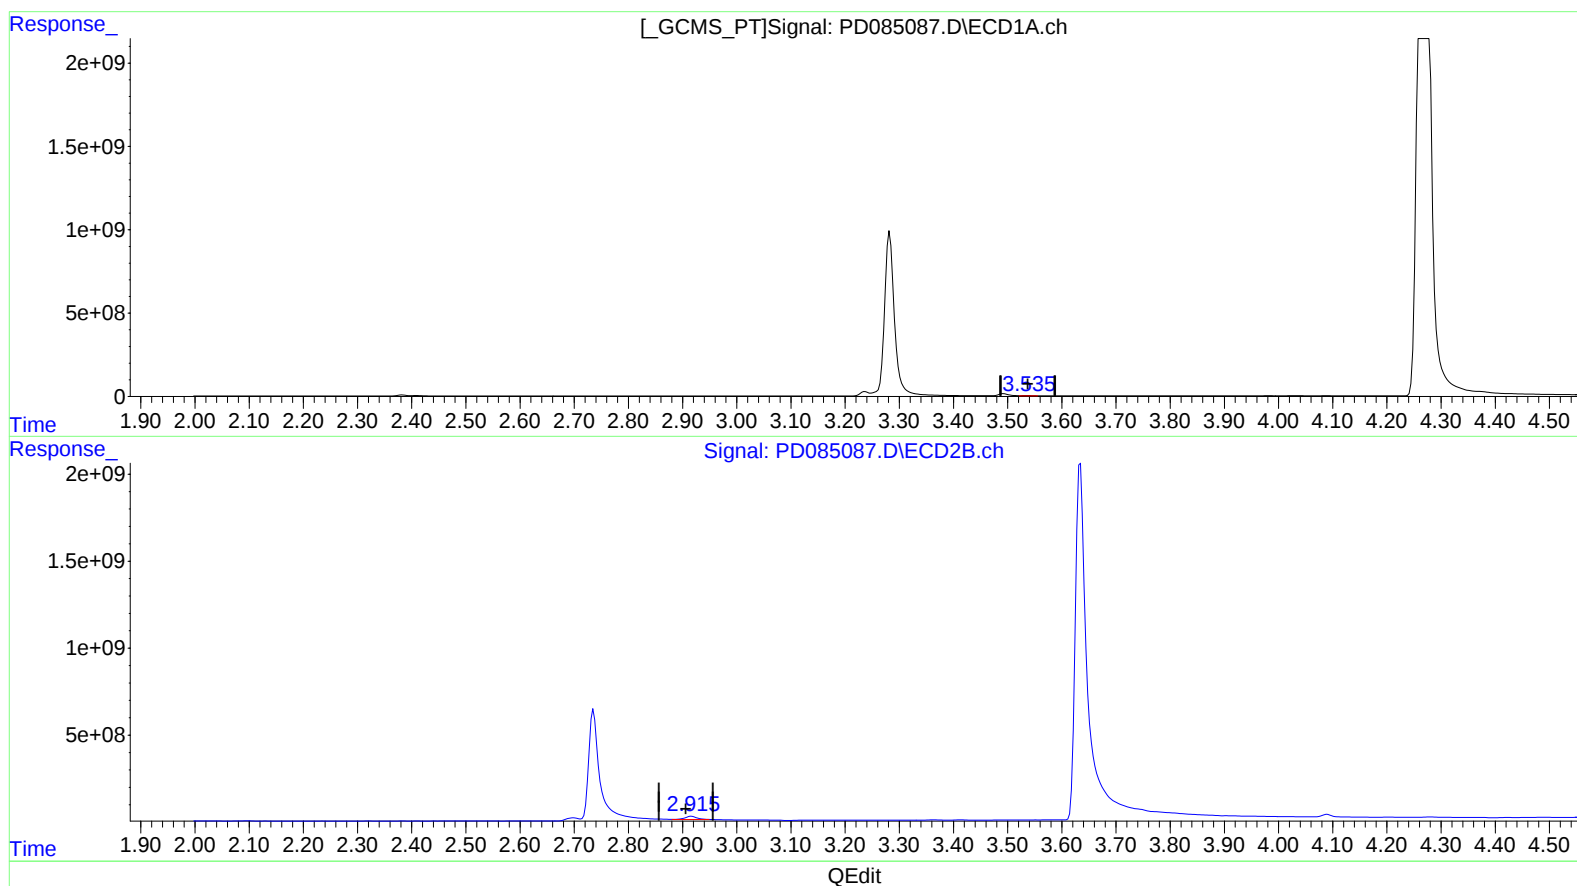

(1) Tetrachloro-m-xylene (SA)

3.535min 21.272 ng/ml m

response 21514711

(1) Tetrachloro-m-xylene #2 (SA)

2.915min 78.451 ng/ml m

response 277621604

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE

## Manual IntegrationsAPPROVED

Reviewed By :Abdul

Mirza

09/15/2024


Supervised By :Ankita

Jodhani

09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

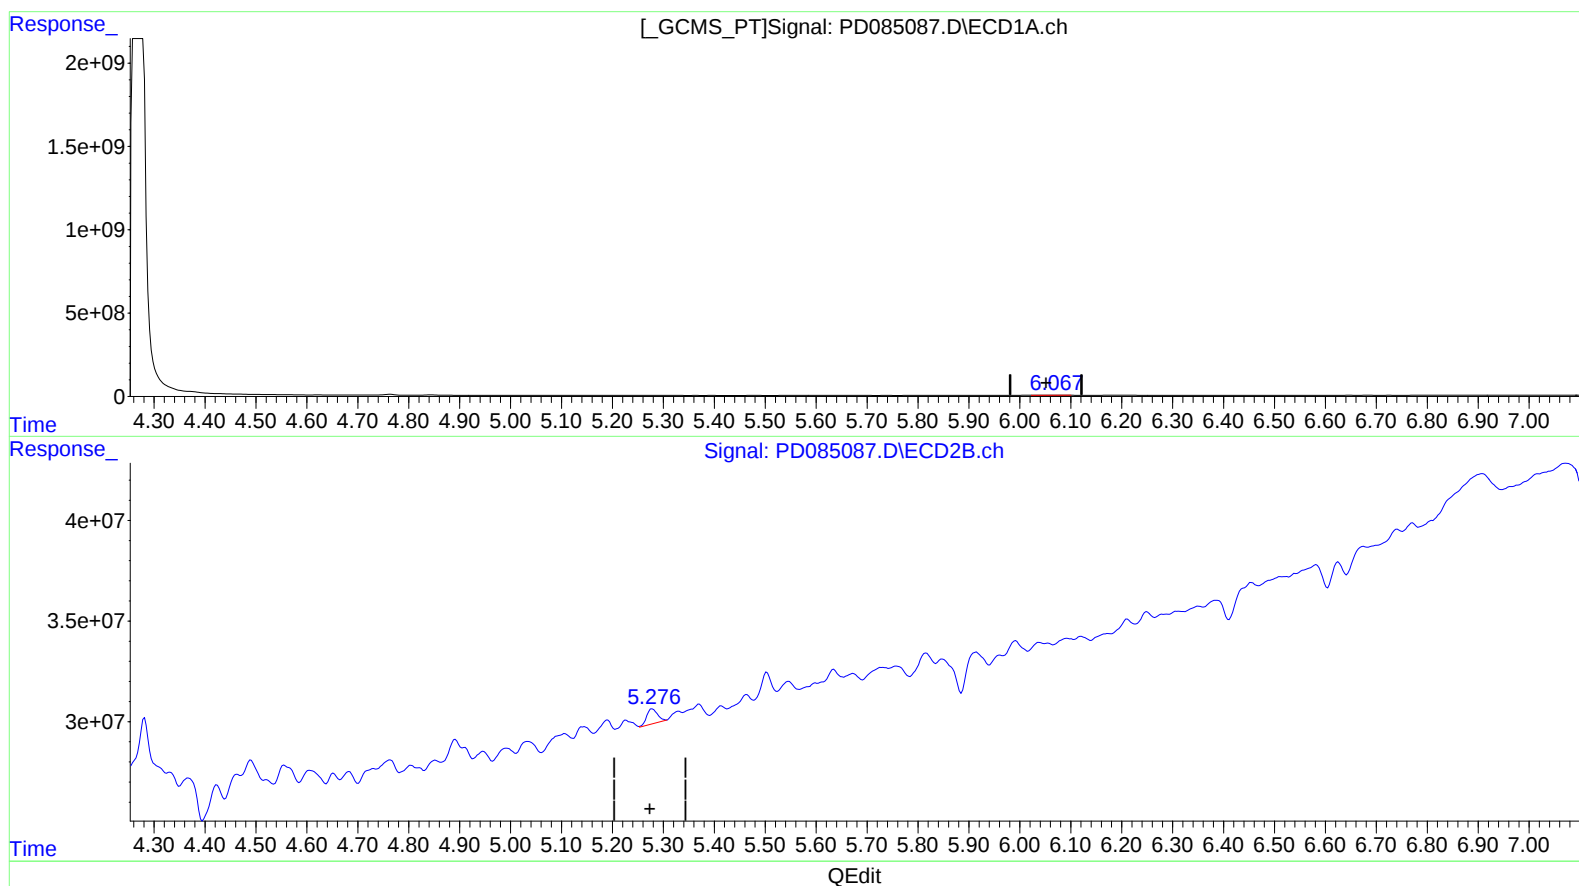

(9) Endosulfan I (A)

6.067min 13.414 ng/ml

response 18454857

(9) Endosulfan I #2 (A)

5.278min 2.804 ng/ml

response 10748074

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE


## Manual IntegrationsAPPROVED

Reviewed By :Abdul  
Mirza  
09/15/2024

Supervised By :Ankita  
Jodhani  
09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

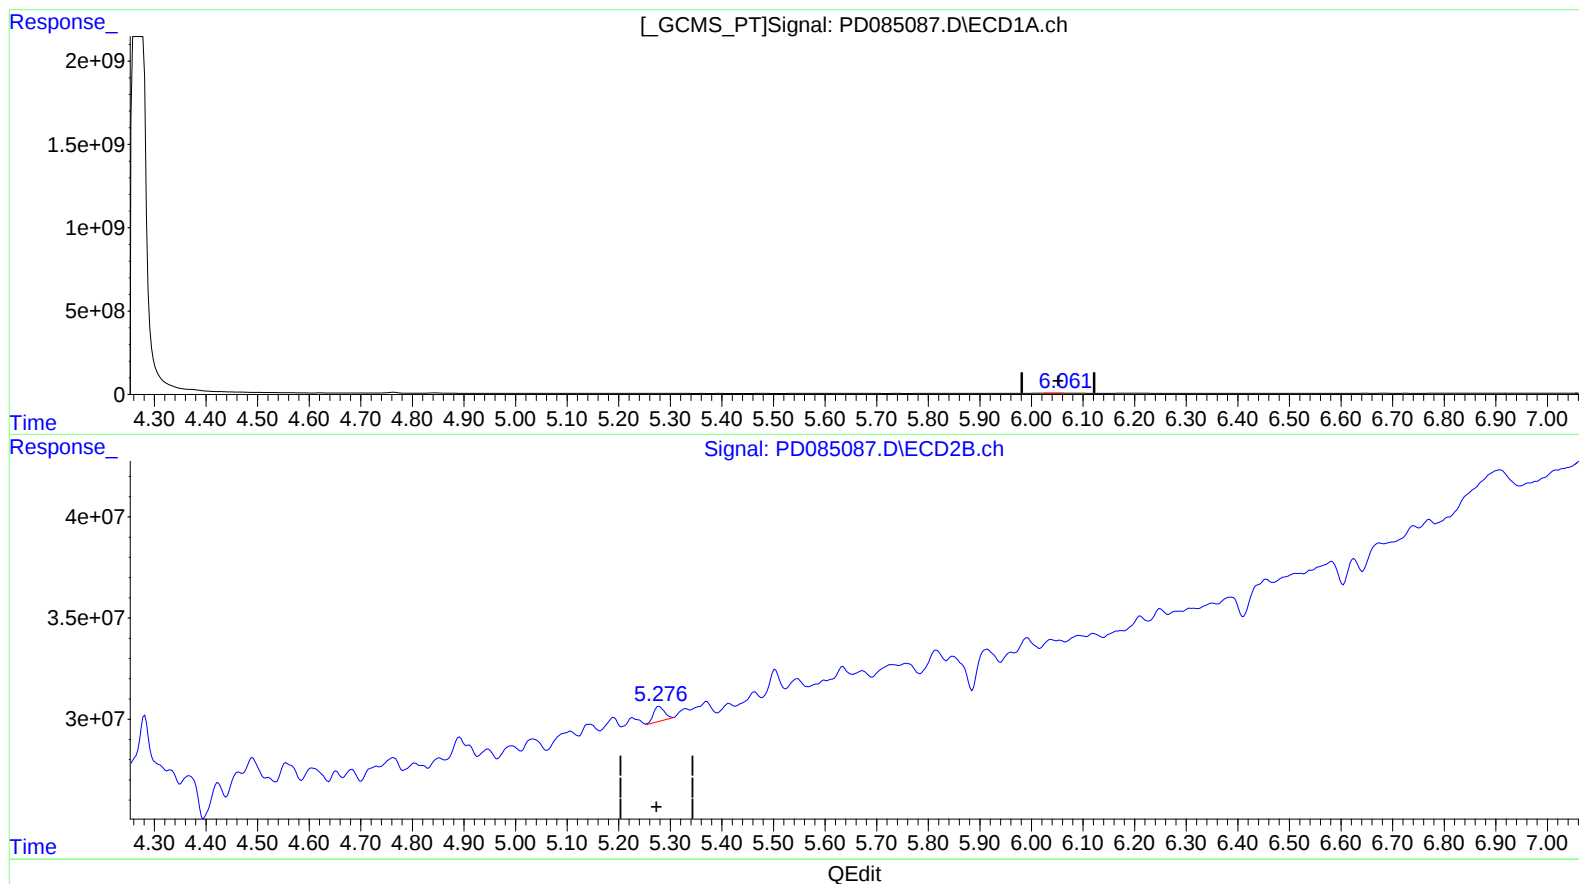

(9) Endosulfan I (A)  
6.061min 3.841 ng/ml m  
response 5284266

(9) Endosulfan I #2 (A)  
5.278min 2.804 ng/ml  
response 10748074

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE

## Manual IntegrationsAPPROVED

Reviewed By :Abdul

Mirza

09/15/2024



Supervised By :Ankita

Jodhani

09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

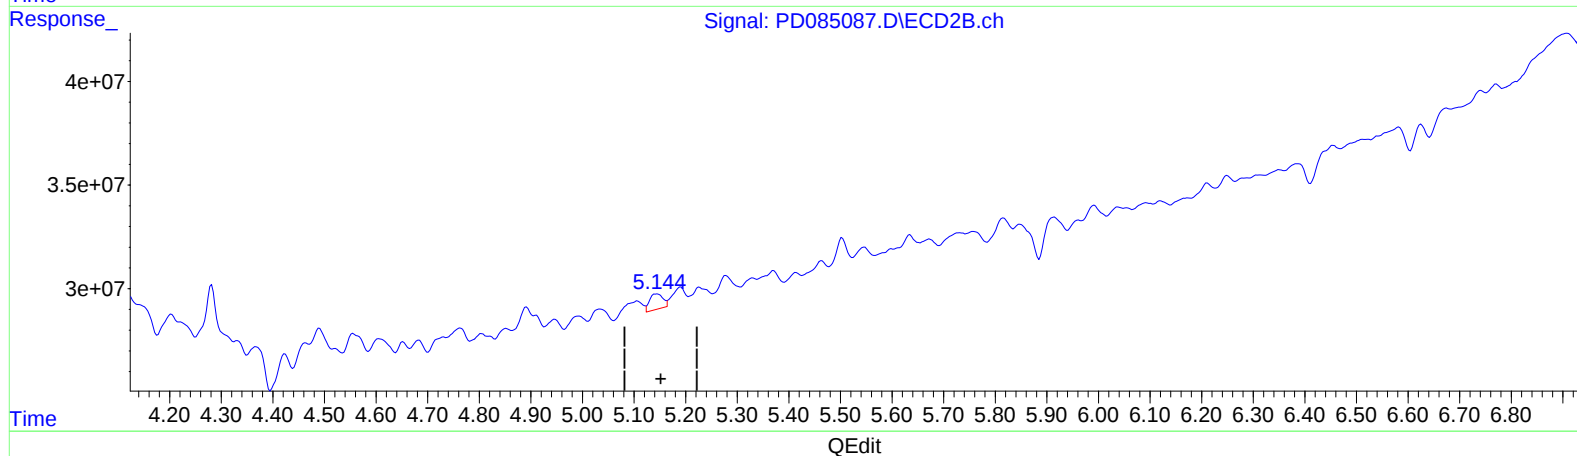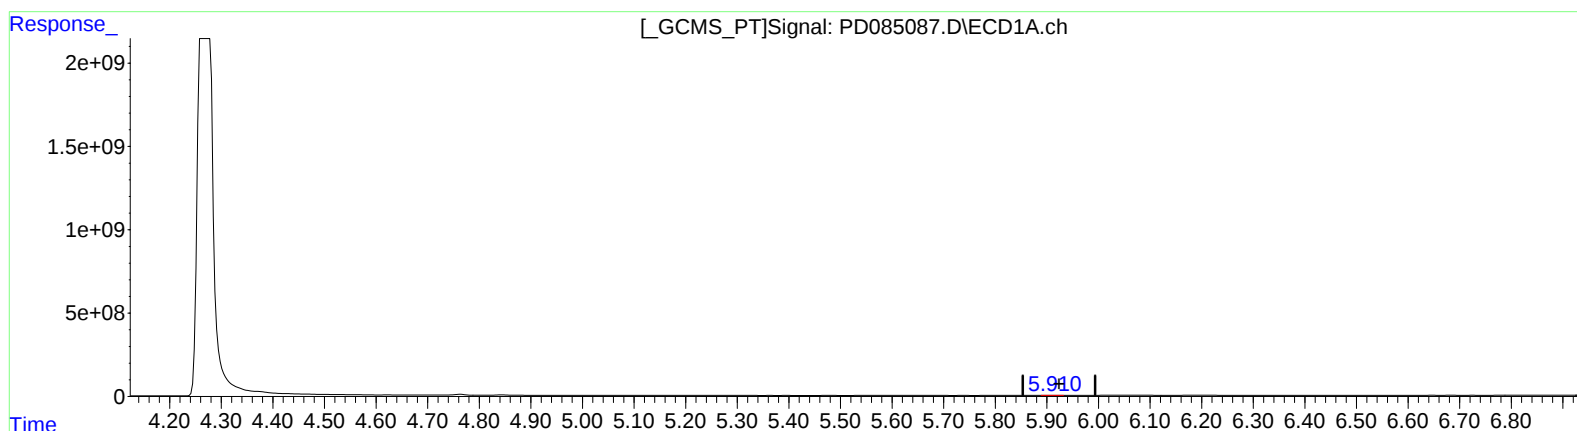

(10) trans-Chlordane (B)

5.912min 1.075 ng/ml

response 1516159

(10) trans-Chlordane #2 (B)

5.145min 3.277 ng/ml

response 13477060

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE



## Manual IntegrationsAPPROVED

Reviewed By :Abdul  
Mirza  
09/15/2024

Supervised By :Ankita  
Jodhani  
09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

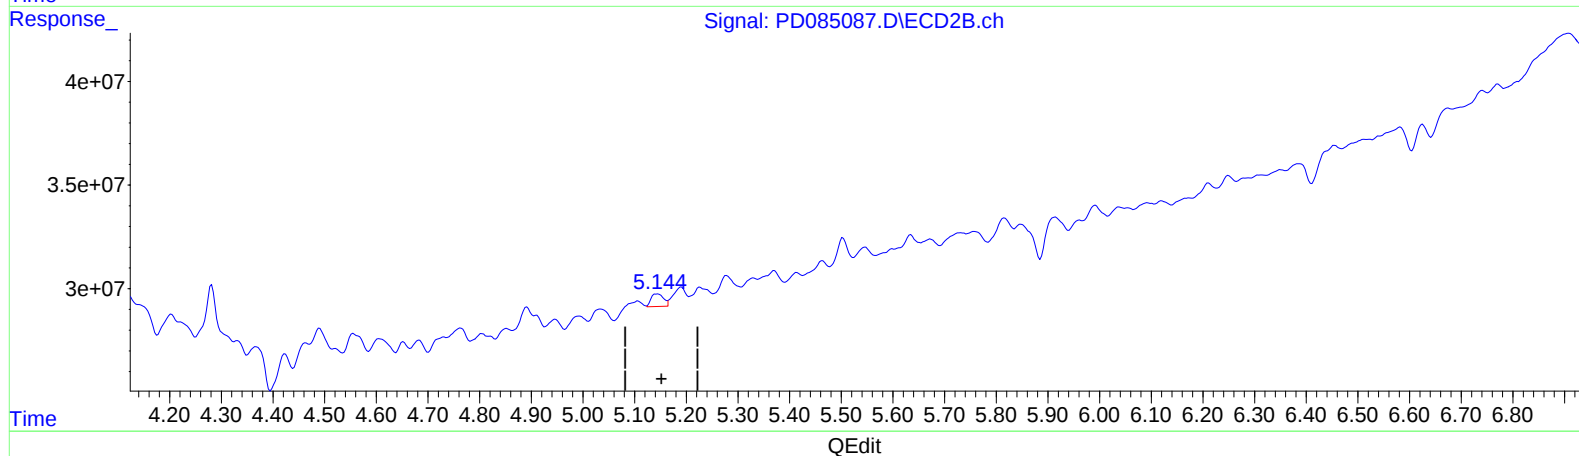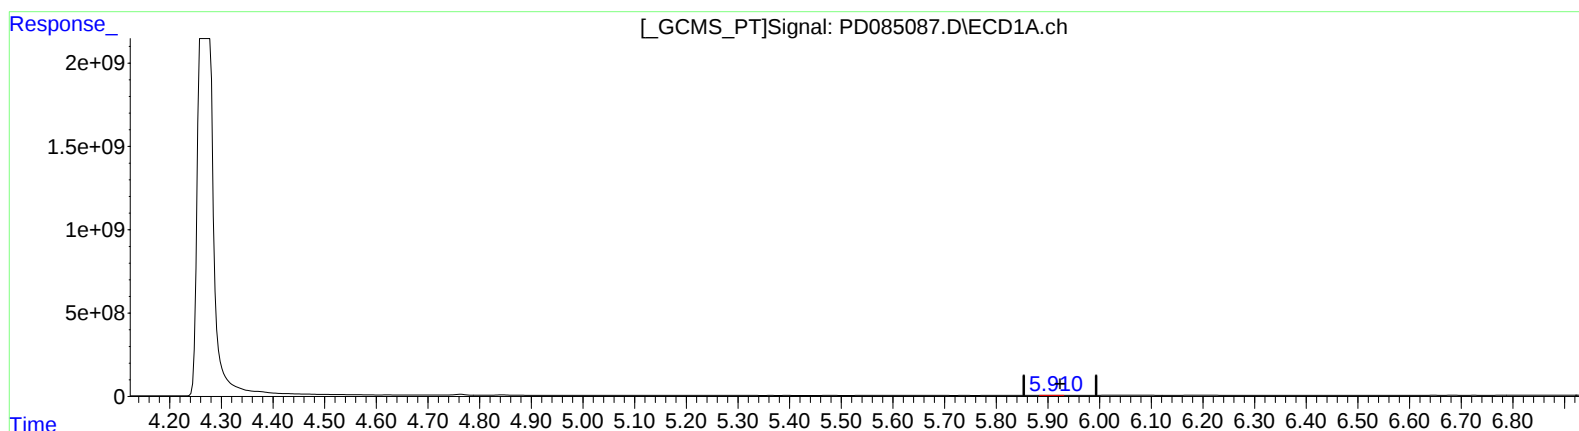

(10) trans-Chlordane (B)

5.910min 1.260 ng/ml m

response 1777182

(10) trans-Chlordane #2 (B)

5.144min 2.675 ng/ml m

response 11003759

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE

## Manual IntegrationsAPPROVED

Reviewed By :Abdul

Mirza

09/15/2024


Supervised By :Ankita

Jodhani

09/16/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

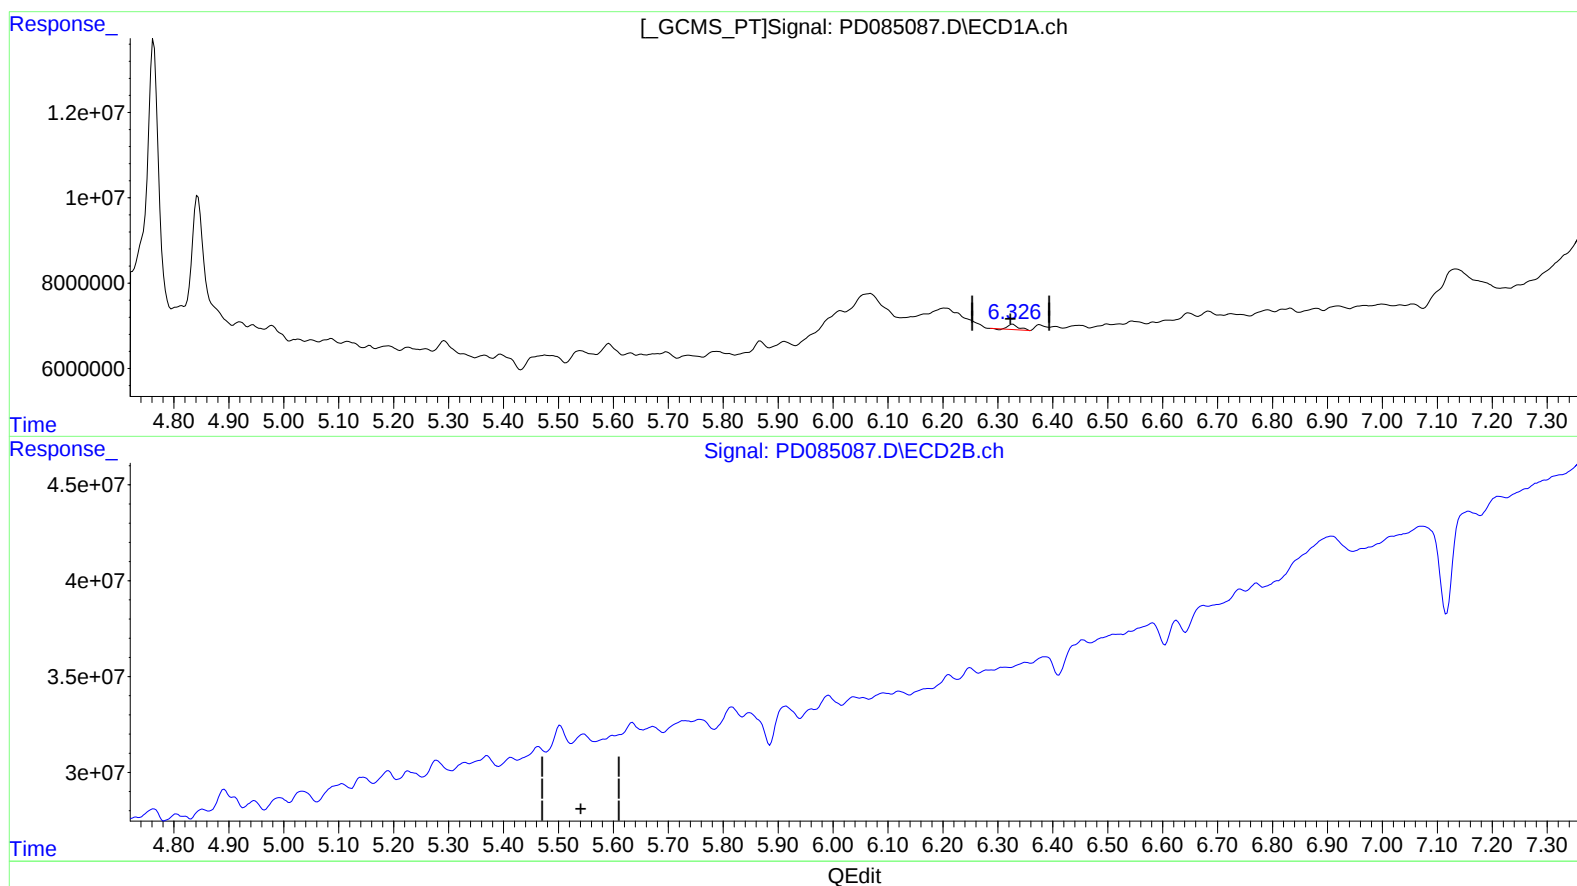

(13) Dieldrin (MA)

6.327min 1.112 ng/ml

response 1640938

(13) Dieldrin #2 (MA)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091324\  
Data File : PD085087.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Sep 2024 16:59  
Operator : AR\AJ  
Sample : P3877-16RXRE  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
DCVZ5RXRE

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 00:50:20 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Reviewed By :Abdul

Mirza


09/15/2024

Supervised By :Ankita

Jodhani

09/16/2024

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

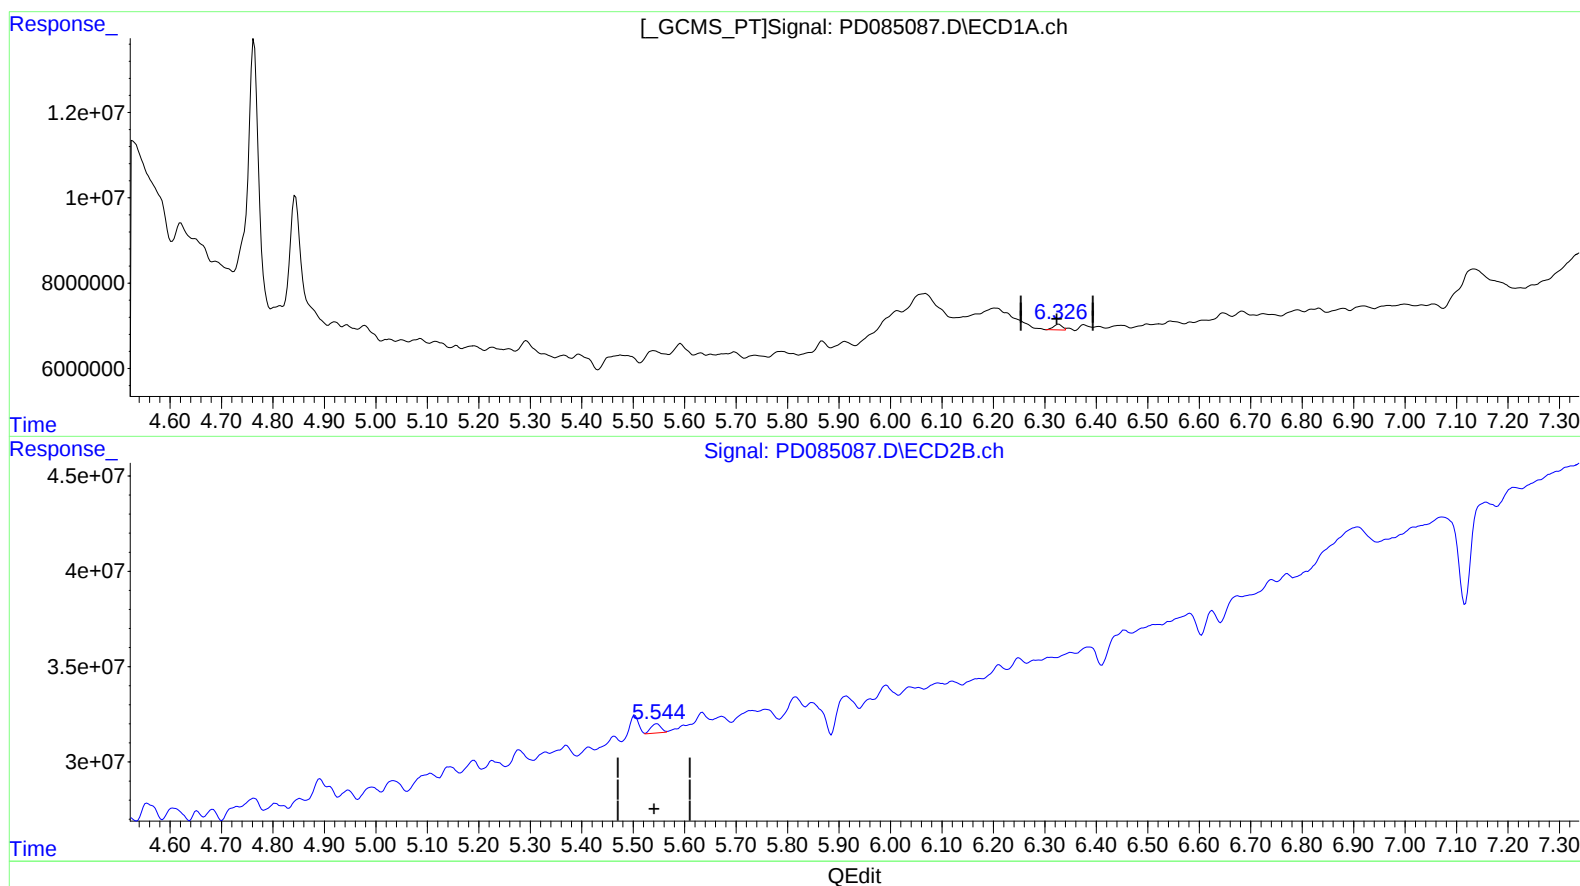

(13) Dieldrin (MA)

6.326min 1.056 ng/ml m

response 1557713

(13) Dieldrin #2 (MA)

5.544min 1.574 ng/ml m

response 6760900