

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
 Data File : PD065701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2021 16:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:40:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 15 03:40:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.495	4.013	17932211	152.9E6	22.966	24.138
28) SA Decachlor...	8.237	9.086	25594644	83407322	22.983	24.016
Target Compounds						
6) B beta-BHC	4.476	4.891f	1602307	3853657	2.508	0.909 #
15) B Endosulfa...	0.000	6.936	0	982596	N.D.	0.185 #
23) Chlordane-1	4.392f	0.000	2439083	0	78.034	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
Data File : PD065701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2021 16:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:40:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Wed Sep 15 03:40:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

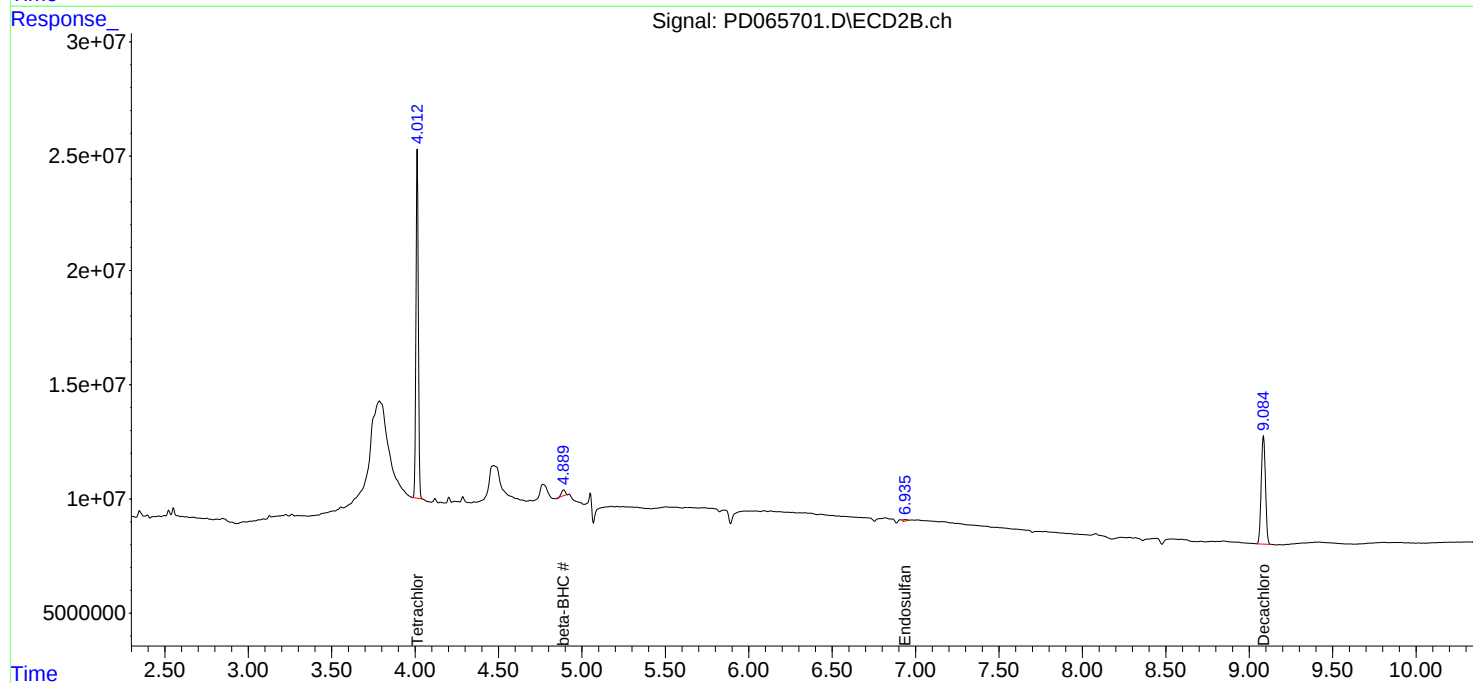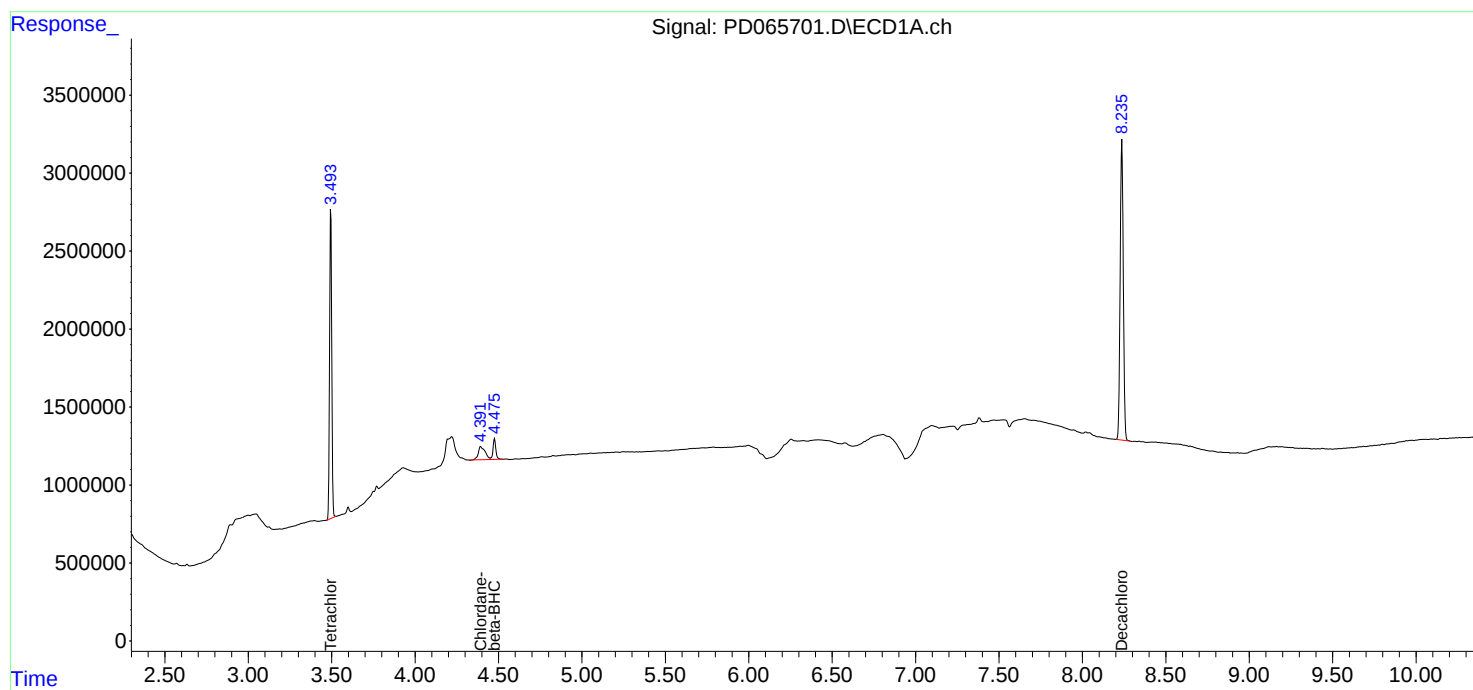


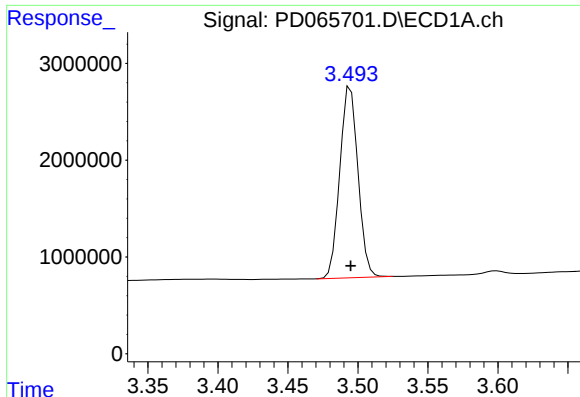

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 17932211
Conc: 22.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

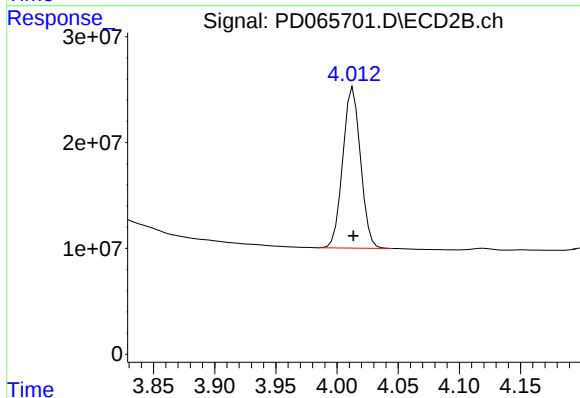


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 152906313
Conc: 24.14 ng/ml

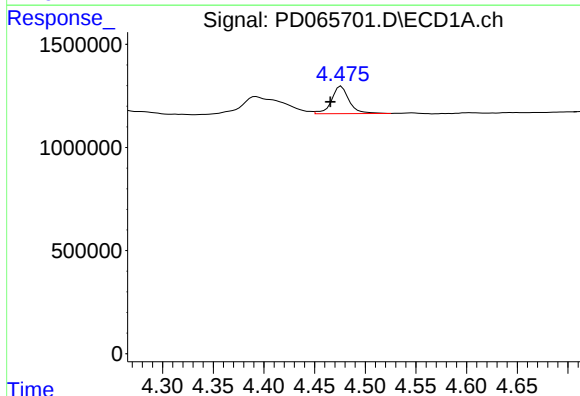


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.011 min
Response: 1602307
Conc: 2.51 ng/ml

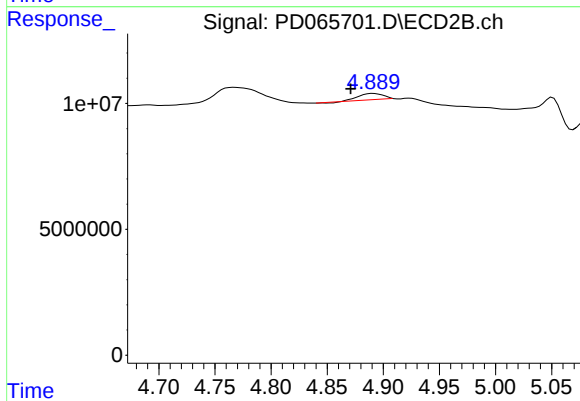

#6 beta-BHC


R.T.: 4.891 min
Delta R.T.: 0.020 min
Response: 3853657
Conc: 0.91 ng/ml

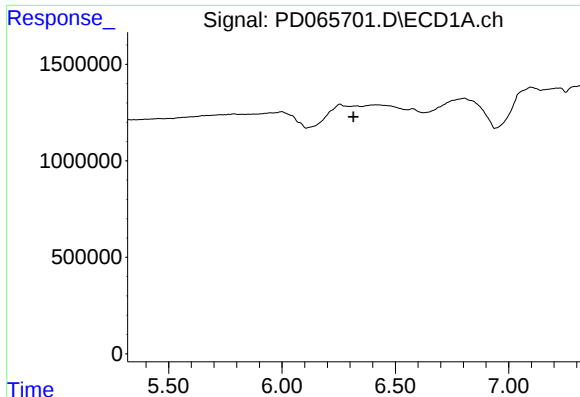

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

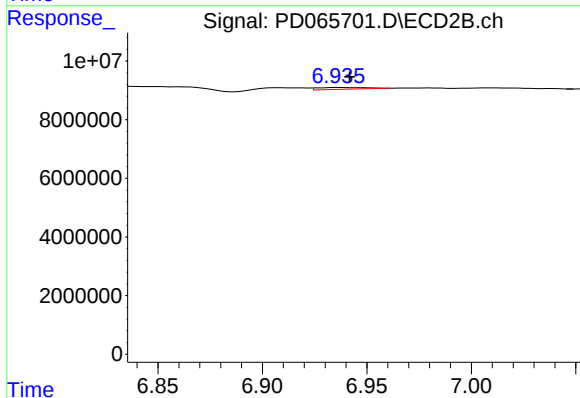


#15 Endosulfan II

R.T.: 6.936 min
Delta R.T.: -0.005 min
Response: 982596
Conc: 0.19 ng/ml

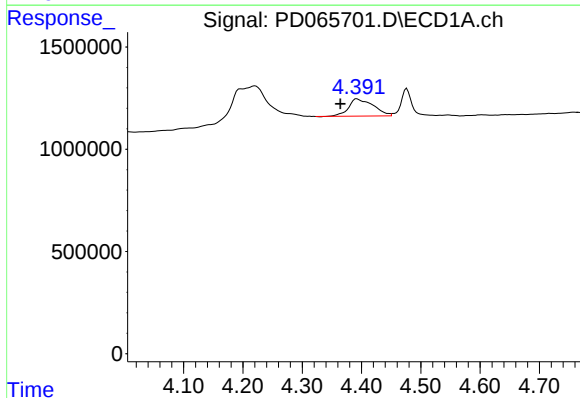


#23 Chlordane-1

R.T.: 4.392 min
Delta R.T.: 0.028 min
Response: 2439083
Conc: 78.03 ng/ml

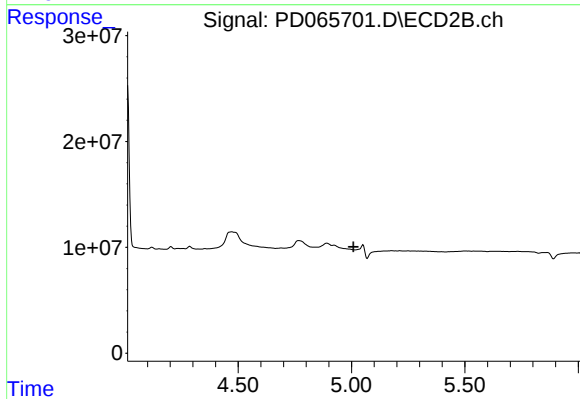

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

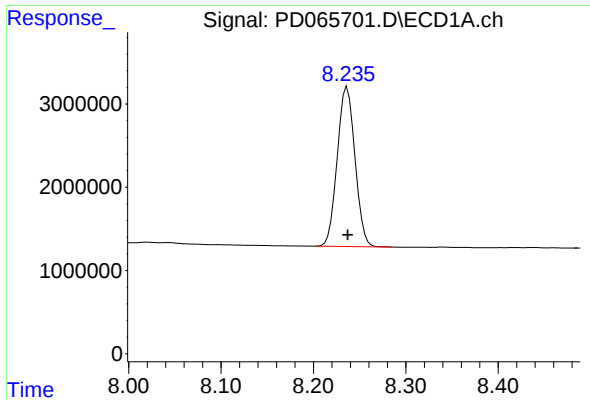

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 25594644
Conc: 22.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

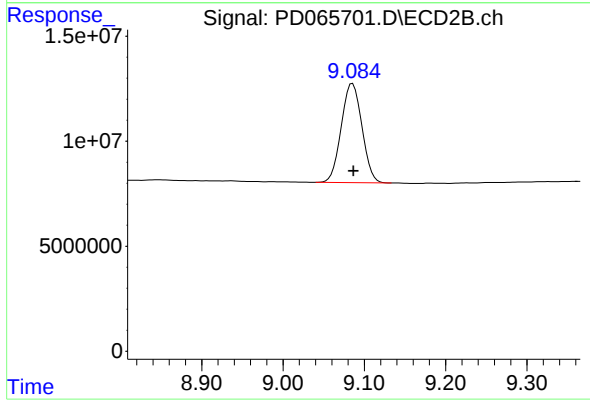

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 83407322
Conc: 24.02 ng/ml