

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
 Data File : PD065709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2021 18:16
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:24:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 15 03:24:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.014	97102298	632.8E6	101.059	98.268
28)	SA Decachlor...	8.236	9.086	109.1E6	332.4E6	97.809	97.200
Target Compounds							
23)	Chlordane-1	4.364	5.009	31272492	228.2E6	1000.251	985.832
24)	Chlordane-2	4.864	5.479	38519065	217.3E6	972.519	964.946
25)	Chlordane-3	5.431	6.127	118.4E6	831.3E6	1010.536	984.151
26)	Chlordane-4	5.489	6.199	97610618	957.4E6	1004.380	979.592
27)	Chlordane-5	6.324	7.010	45714974	186.0E6	995.143	980.939



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
Data File : PD065709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2021 18:16
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:24:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Wed Sep 15 03:24:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

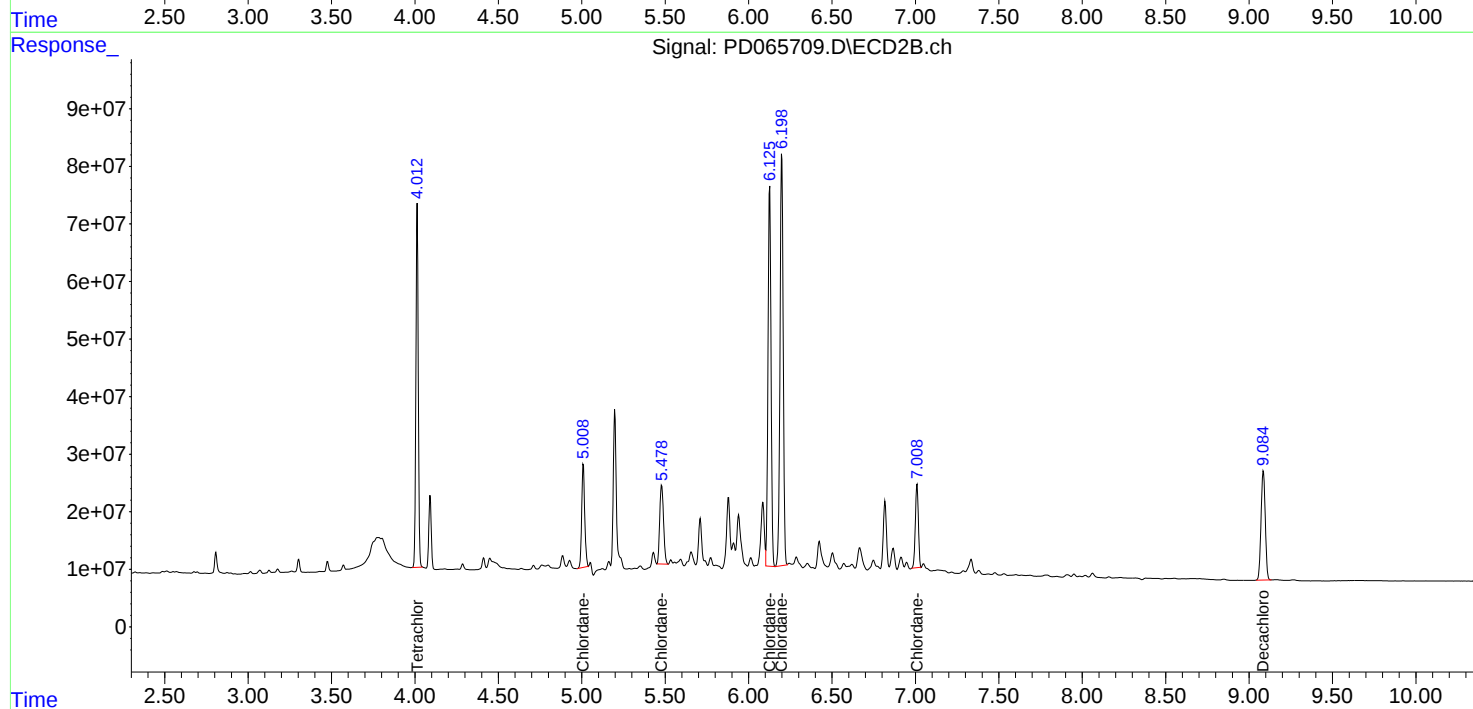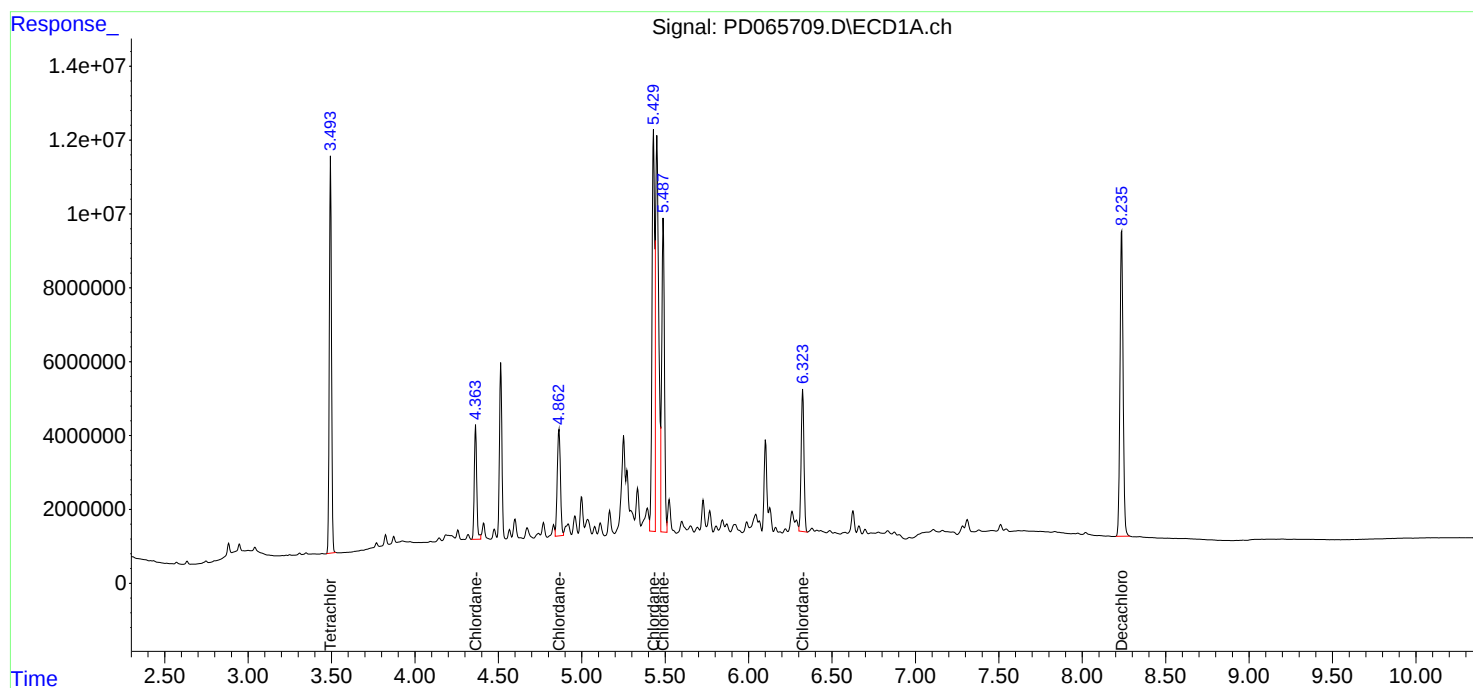


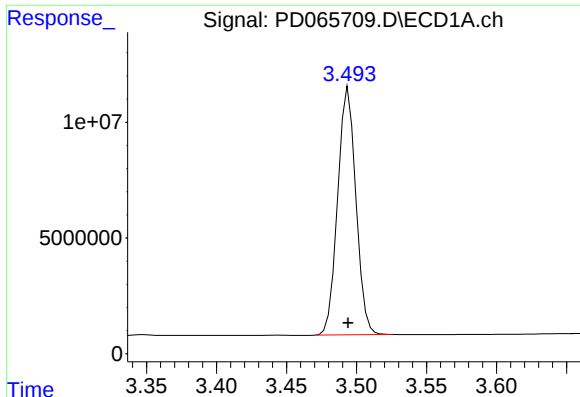

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 97102298
Conc: 101.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

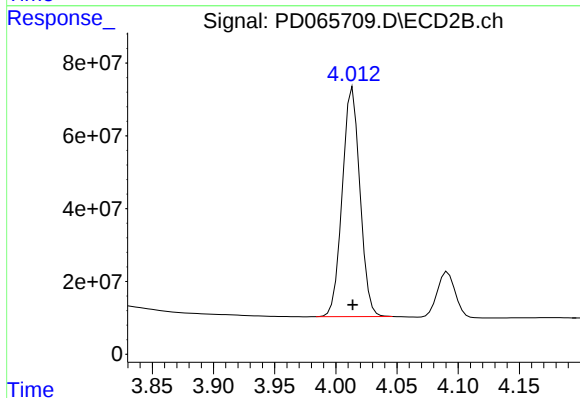


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 632782694
Conc: 98.27 ng/ml

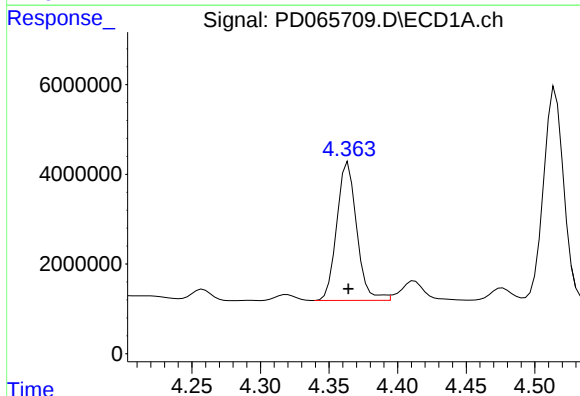


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 31272492
Conc: 1000.25 ng/ml

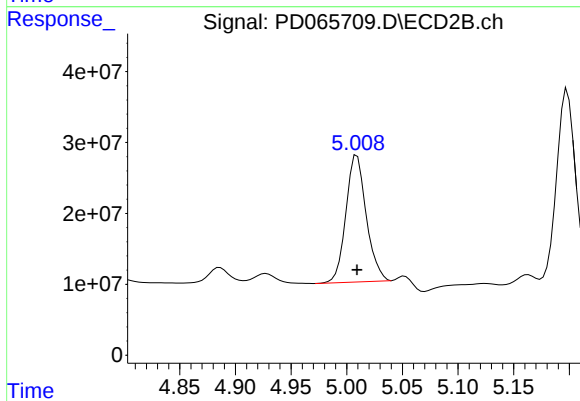

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 228219675
Conc: 985.83 ng/ml

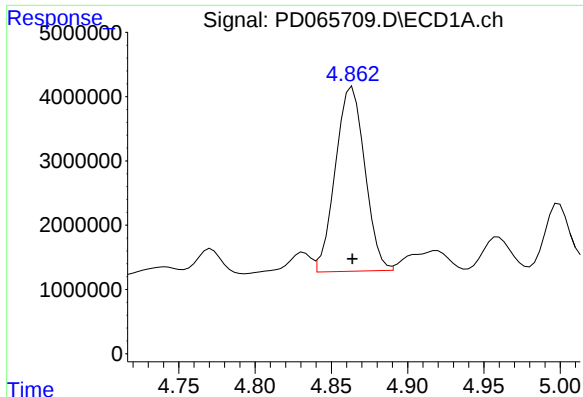

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 38519065
Conc: 972.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

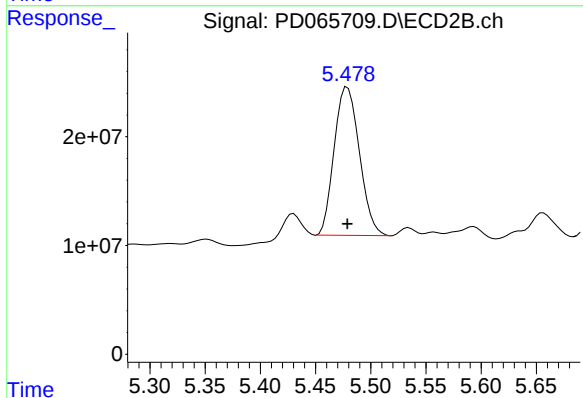


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 217308855
Conc: 964.95 ng/ml

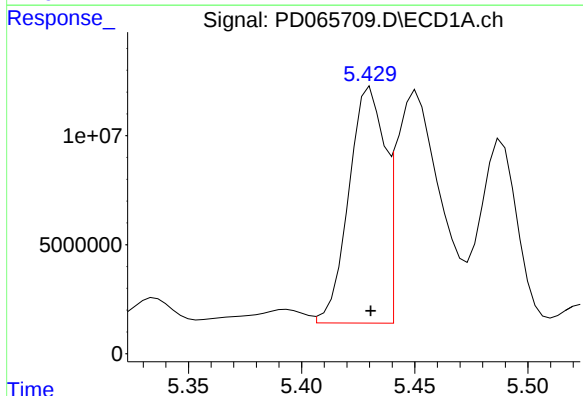


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.000 min
Response: 118393083
Conc: 1010.54 ng/ml

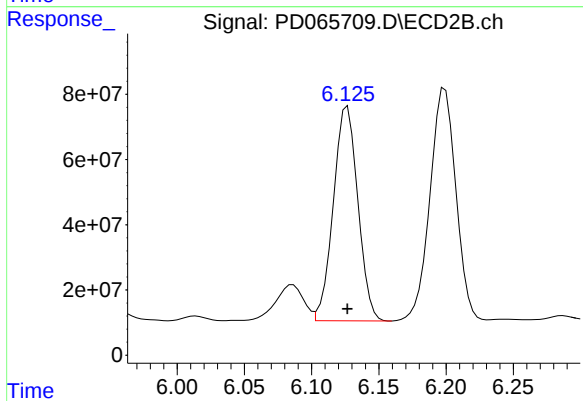

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 831325171
Conc: 984.15 ng/ml

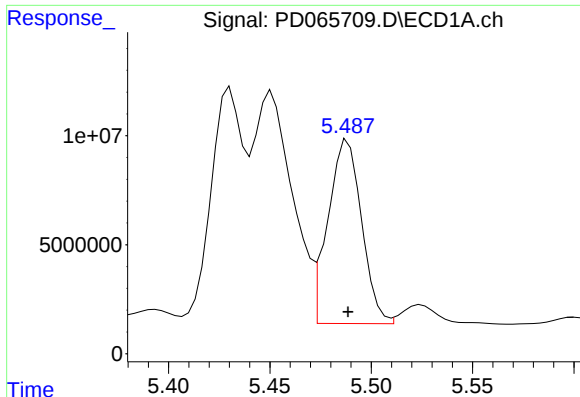

#26 Chlordane-4


R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 97610618
Conc: 1004.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

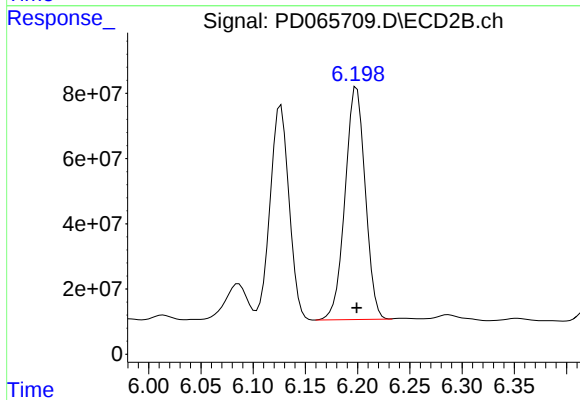


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 957421700
Conc: 979.59 ng/ml

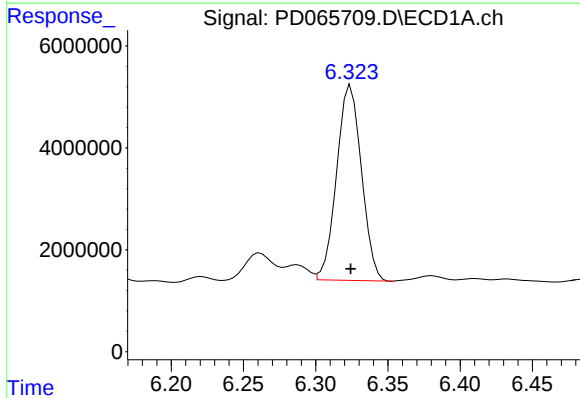


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 45714974
Conc: 995.14 ng/ml

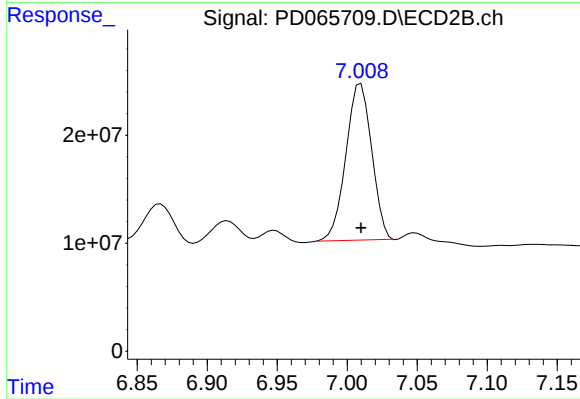

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 186028721
Conc: 980.94 ng/ml

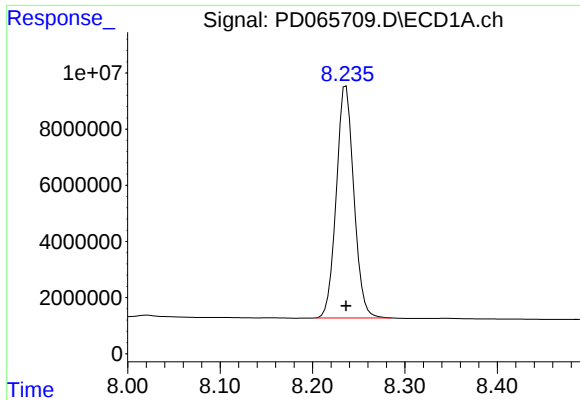

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 109094251
Conc: 97.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

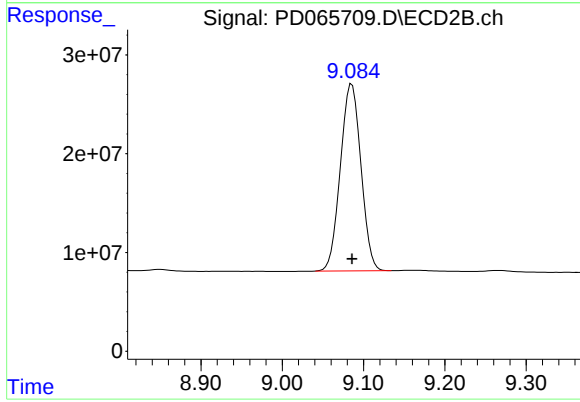

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 332442597
Conc: 97.20 ng/ml