

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
 Data File : PD065721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2021 21:01
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD091421TOX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:01:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091421.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 15 04:00:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.495	4.013	39552415	325.5E6	49.872	49.822
7) SA Decachlor...	8.236	9.086	57481687	181.5E6	50.369	51.022
Target Compounds						
2) Toxaphene-1	5.746	6.407	4414622	17010279	511.057	528.536
3) Toxaphene-2	5.907	6.599	4699529	27469680	523.179	516.990
4) Toxaphene-3	6.348	7.183	10874450	48402033	528.134	511.921
5) Toxaphene-4	6.595	7.269	11622241	47341306	507.441	519.056
6) Toxaphene-5	7.080	7.687	13764348	35015953	506.626	519.951

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
Data File : PD065721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2021 21:01
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:01:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091421.M
Quant Title : GC Extractables
QLast Update : Wed Sep 15 04:00:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

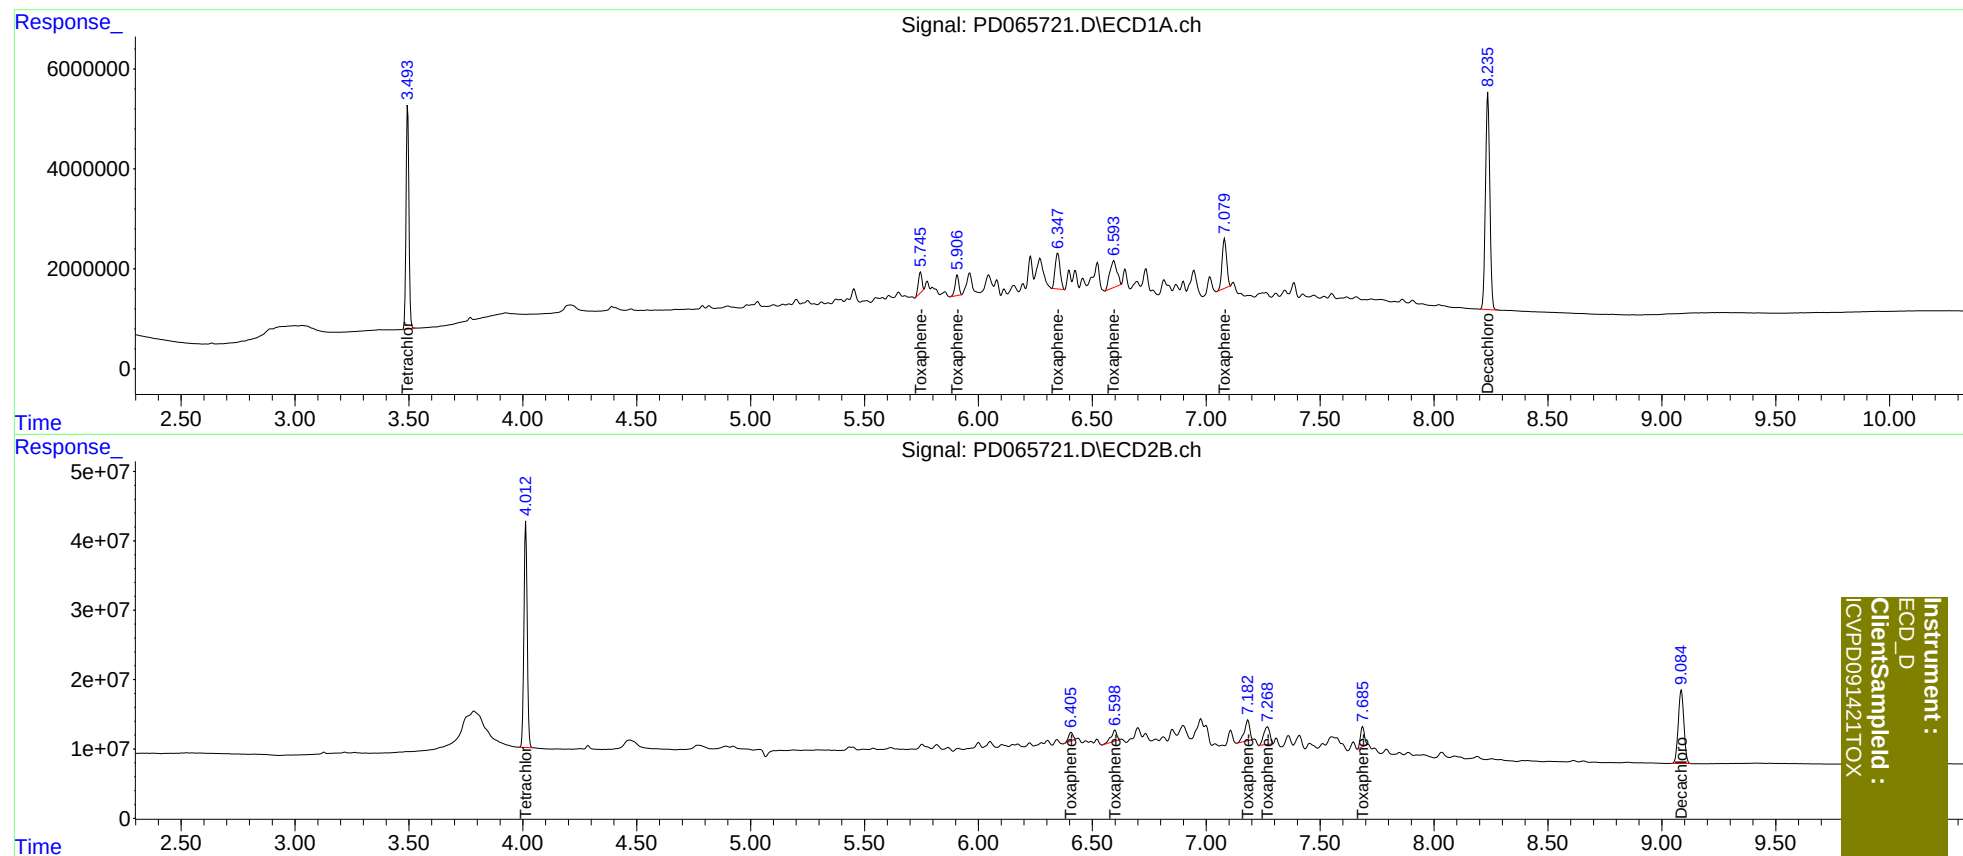

Instrument :
ECD_D
ClientSample :
ICV/PD091421TOX