

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
 Data File : PD065713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2021 19:11
 Operator : AR\AJ
 Sample : PCHLORICC050 (Sig #1); PCHLORICC50 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:31:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 15 03:30:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.014	12647314	94909329	9.947	10.492
28)	SA Decachlor...	8.237	9.085	17057839	51535910	10.731	10.609
Target Compounds							
23)	Chlordane-1	4.364	5.009	4490967	32867383	103.940	103.128
24)	Chlordane-2	4.864	5.479	5672410	36028256	103.198	109.417
25)	Chlordane-3	5.430	6.127	15240773	120.2E6	99.069	103.247
26)	Chlordane-4	5.488	6.199	13194477	142.1E6	101.126	104.400
27)	Chlordane-5	6.325	7.010	6197119	26039698	100.375	101.409



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
Data File : PD065713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2021 19:11
Operator : AR\AJ
Sample : PCHLORICC050 (Sig #1); PCHLORICC50 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:31:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Wed Sep 15 03:30:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

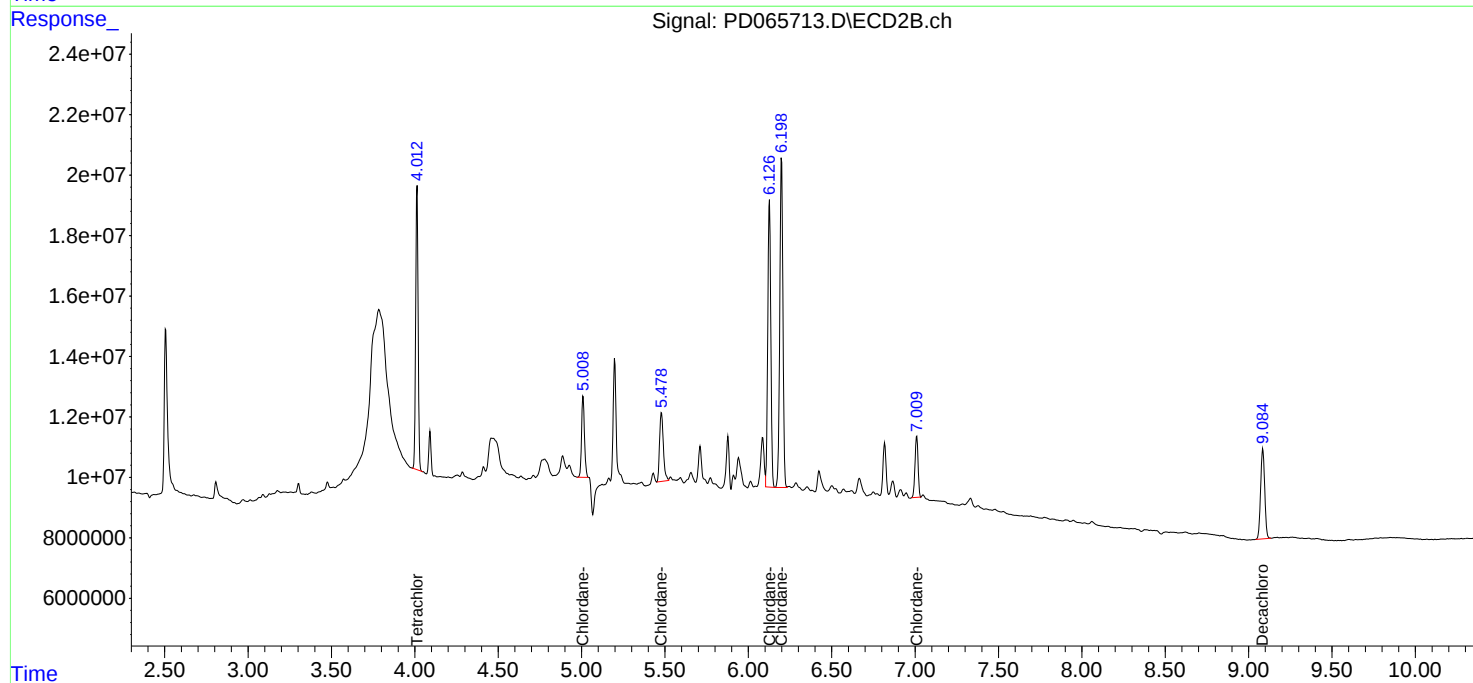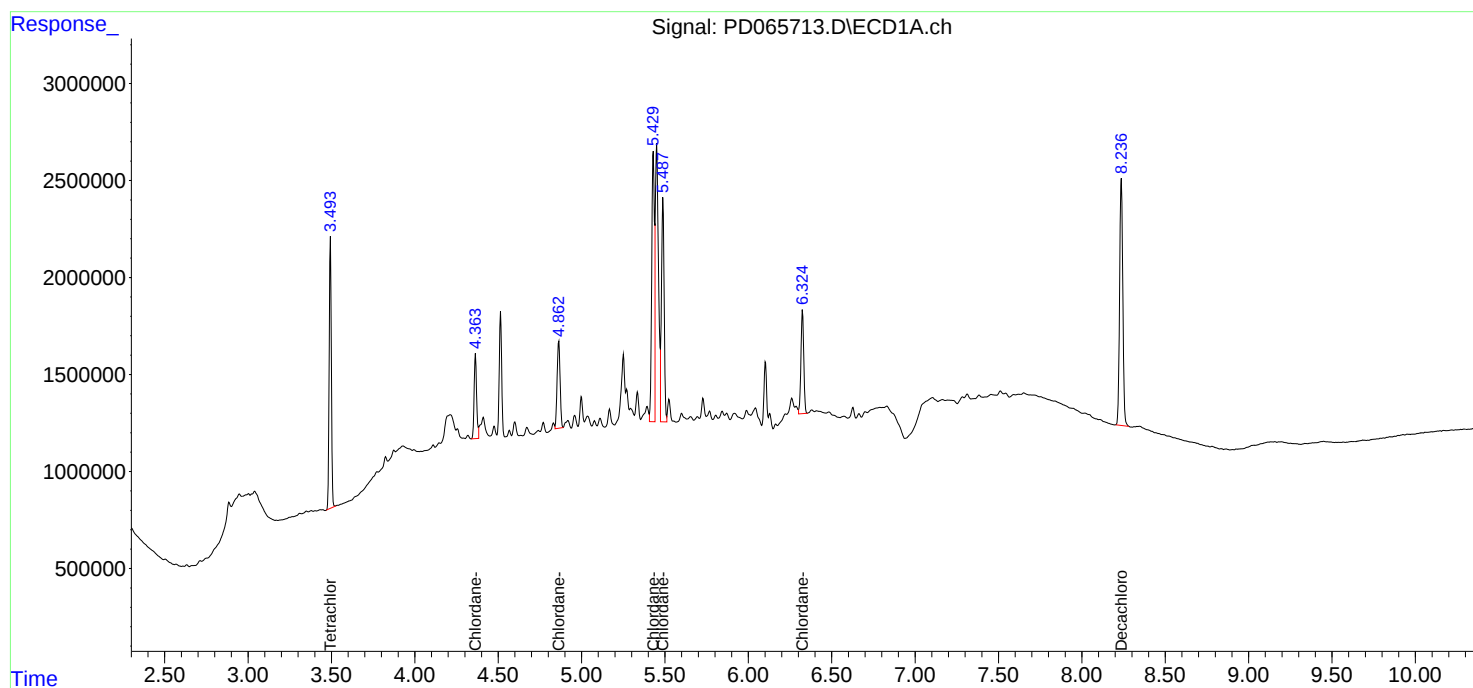


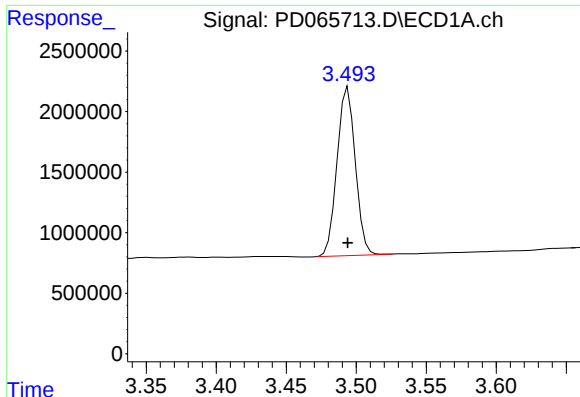

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 12647314
Conc: 9.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

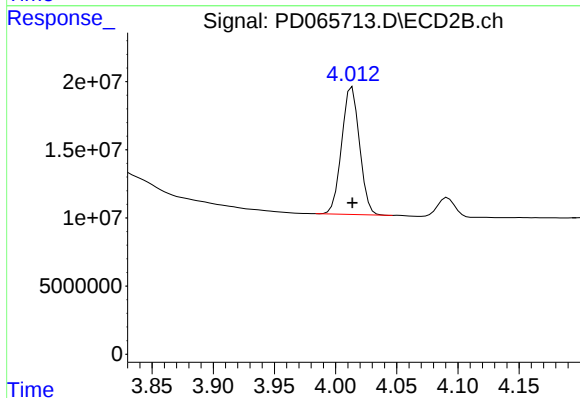


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 94909329
Conc: 10.49 ng/ml

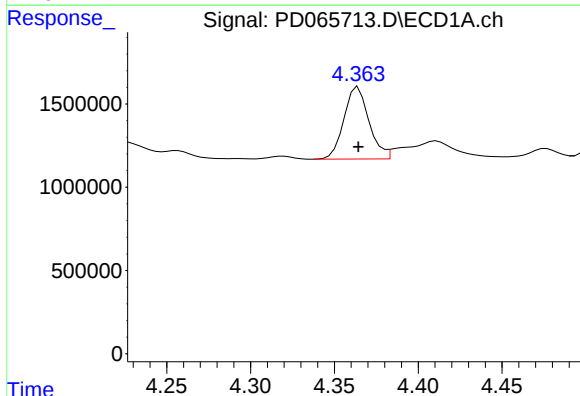


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 4490967
Conc: 103.94 ng/ml

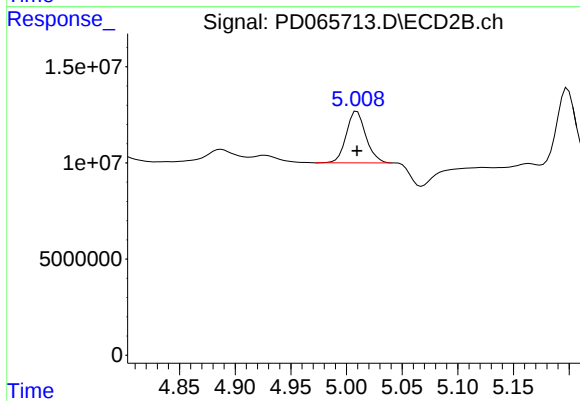

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 32867383
Conc: 103.13 ng/ml

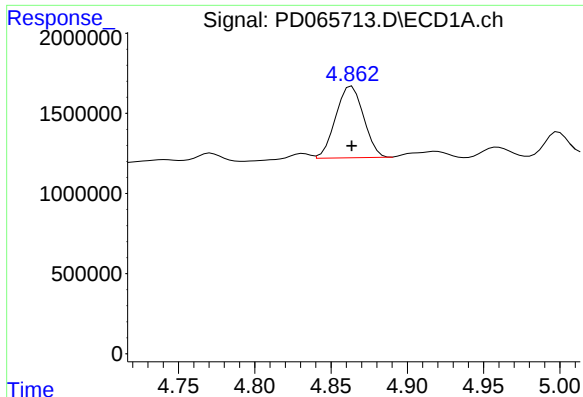

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 5672410
Conc: 103.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

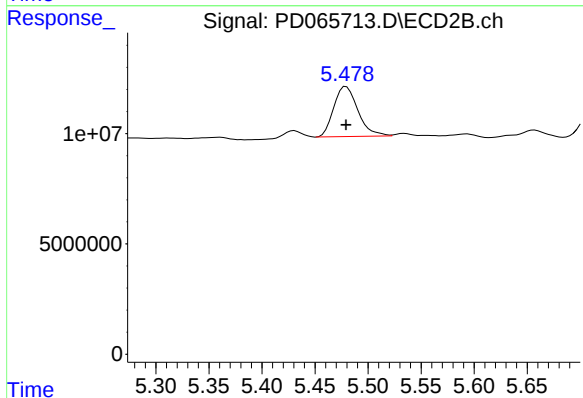


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 36028256
Conc: 109.42 ng/ml

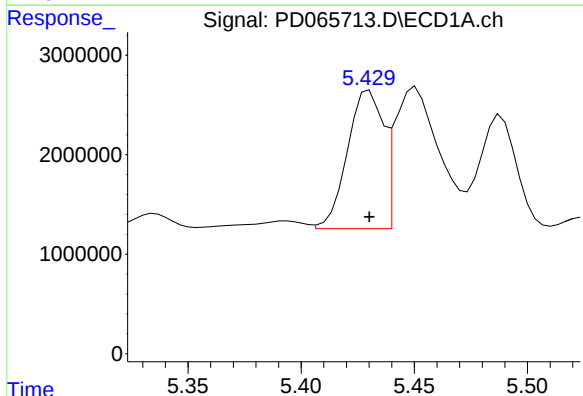


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 15240773
Conc: 99.07 ng/ml

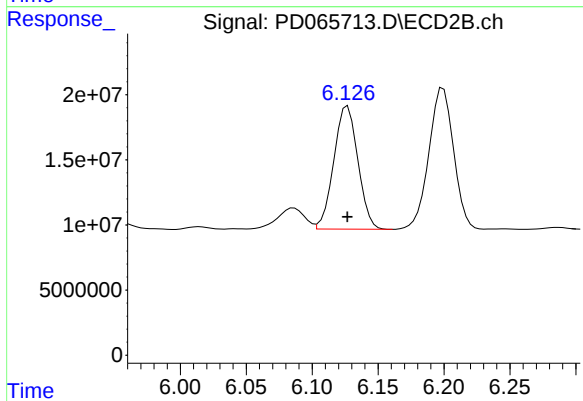

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 120173727
Conc: 103.25 ng/ml

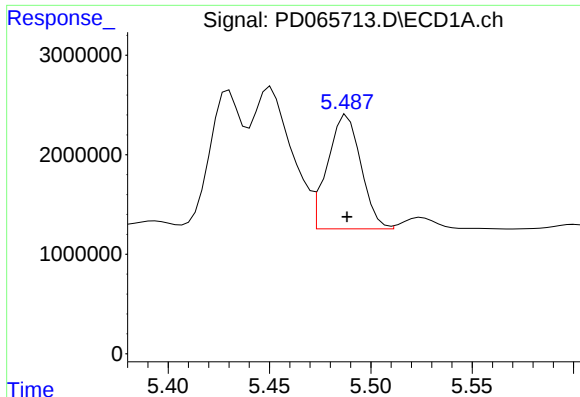

#26 Chlordane-4


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 13194477
Conc: 101.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

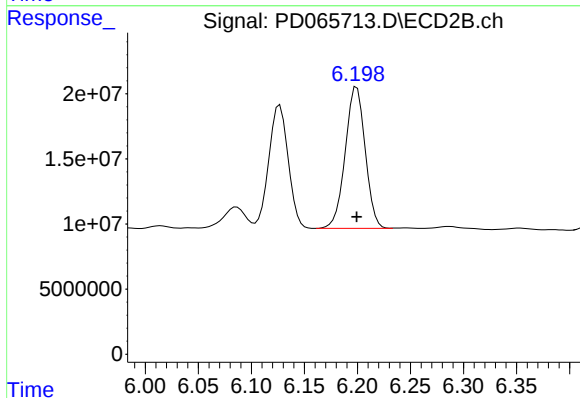


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 142100113
Conc: 104.40 ng/ml

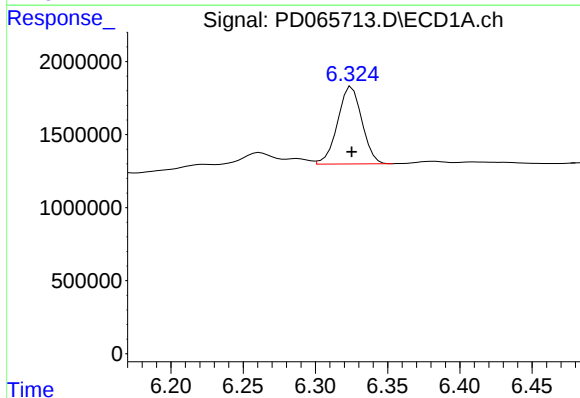


#27 Chlordane-5

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 6197119
Conc: 100.37 ng/ml

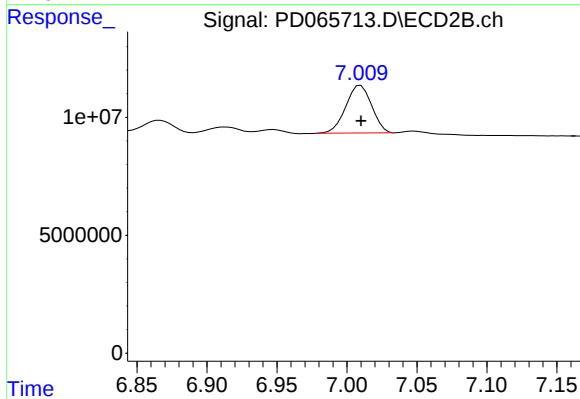

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 26039698
Conc: 101.41 ng/ml

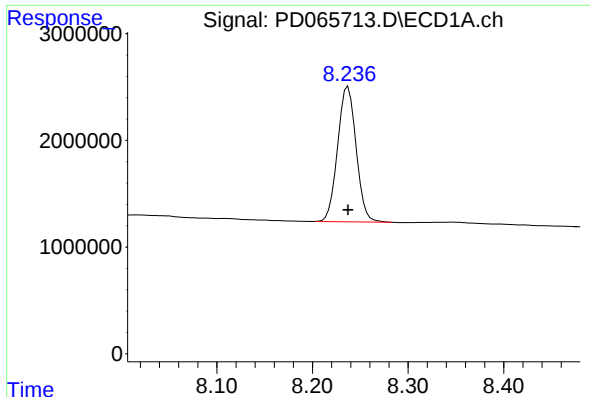

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 17057839
Conc: 10.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

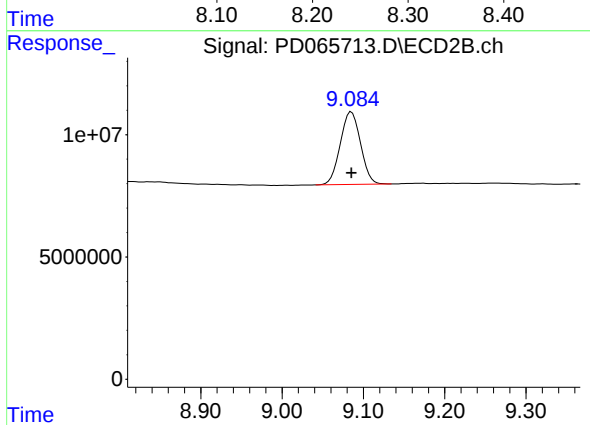

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 51535910
Conc: 10.61 ng/ml