

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
 Data File : PD065720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2021 20:47
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD091421CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:15:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 15 03:40:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	47627290	330.8E6	60.998	52.225
28)	SA Decachlor...	8.236	9.085	58577425	184.6E6	52.601	53.148
Target Compounds							
23)	Chlordane-1	4.363	5.008	15654328	119.6E6	500.829	509.556
24)	Chlordane-2	4.863	5.478	20396847	117.5E6	501.201	504.176
25)	Chlordane-3	5.430	6.126	58559104	434.0E6	505.150	505.819
26)	Chlordane-4	5.488	6.199	48666799	504.3E6	502.967	505.701
27)	Chlordane-5	6.324	7.010	23228115	97867460	503.196	506.408



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091421\
Data File : PD065720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2021 20:47
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD091421CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:15:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Wed Sep 15 03:40:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

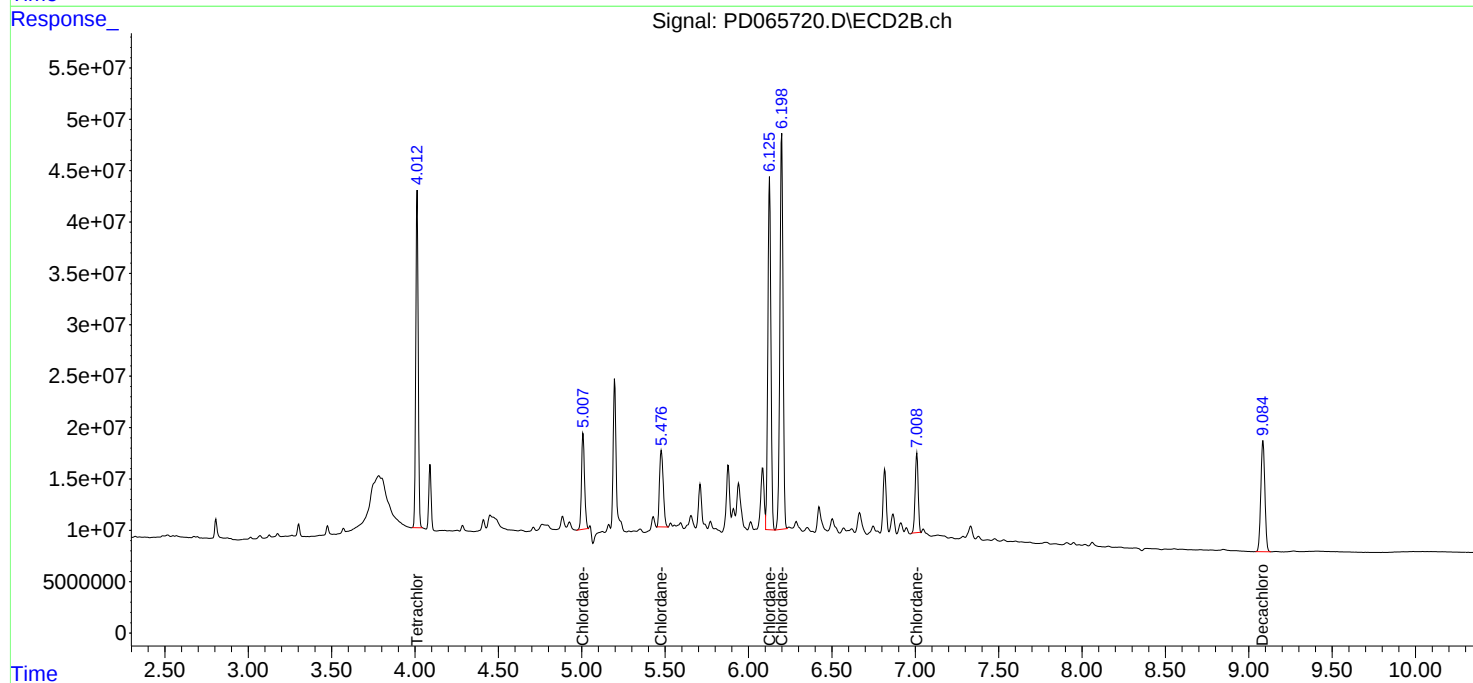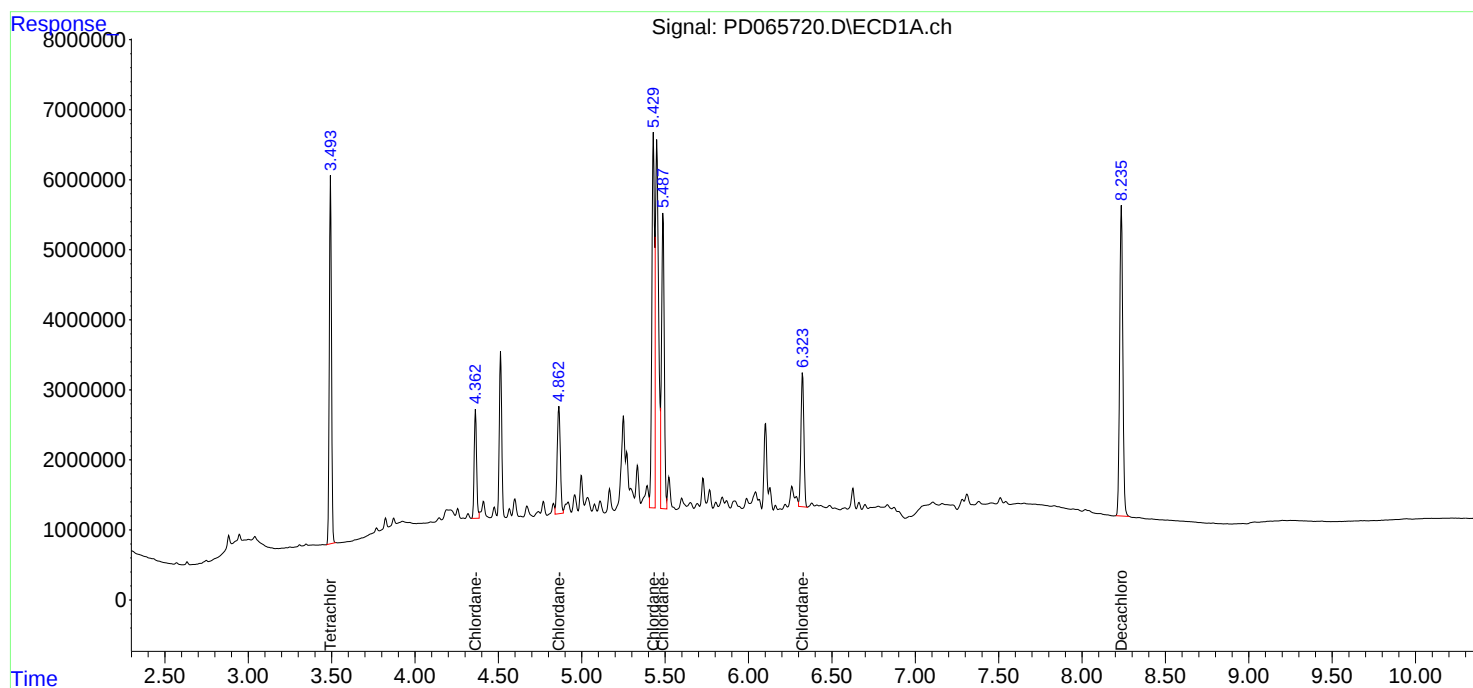


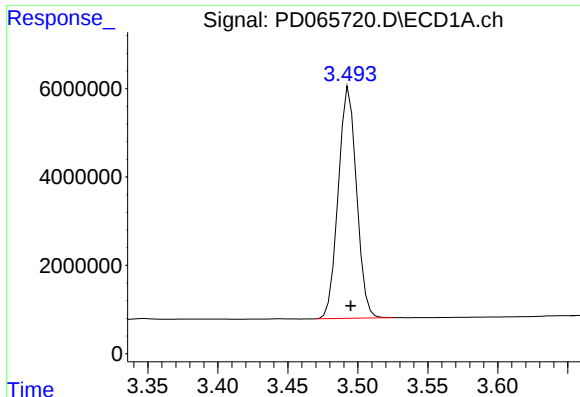

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: -0.001 min
Response: 47627290
Conc: 61.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091421CHLOR

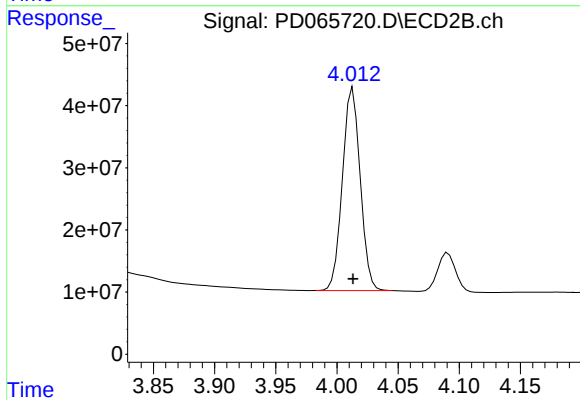


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 330827318
Conc: 52.22 ng/ml

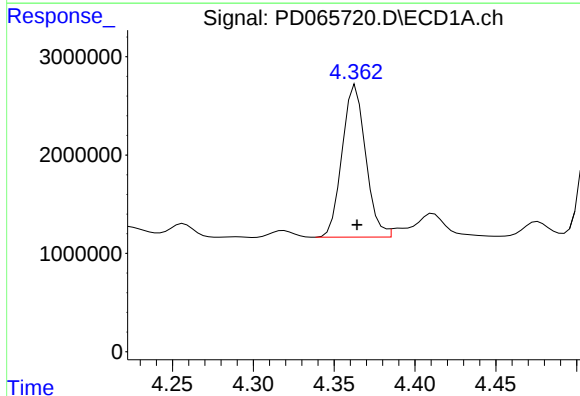


#23 Chlordane-1

R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 15654328
Conc: 500.83 ng/ml

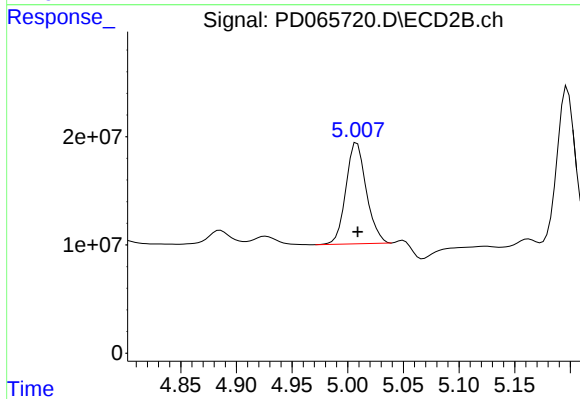

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 119633387
Conc: 509.56 ng/ml

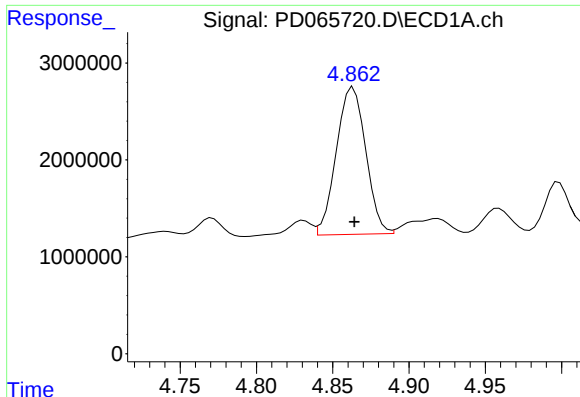

#24 Chlordane-2


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 20396847
Conc: 501.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091421CHLOR

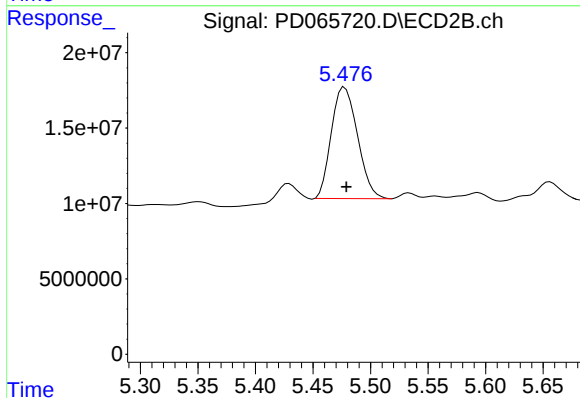


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: -0.001 min
Response: 117521935
Conc: 504.18 ng/ml

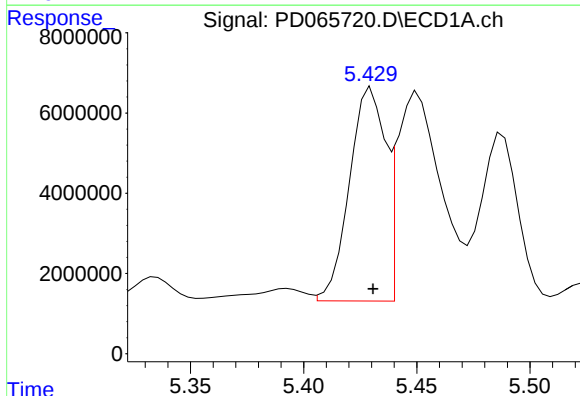


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 58559104
Conc: 505.15 ng/ml

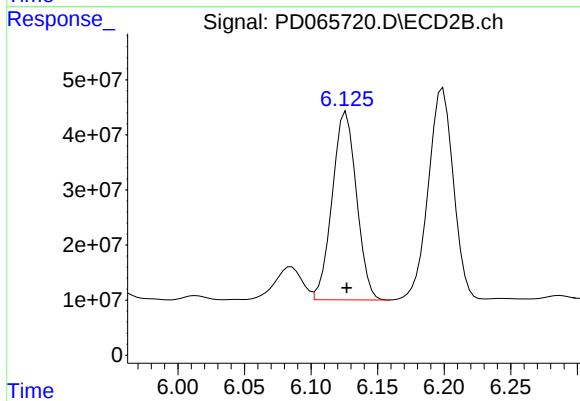

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 434043158
Conc: 505.82 ng/ml

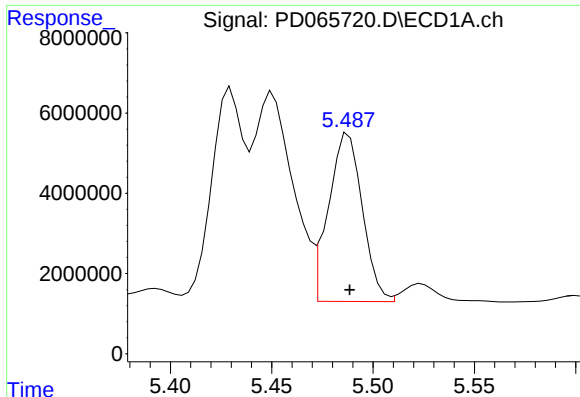

#26 Chlordane-4


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 48666799
Conc: 502.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091421CHLOR

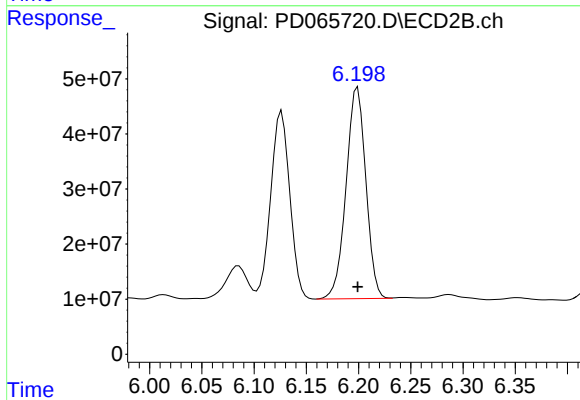


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 504342645
Conc: 505.70 ng/ml

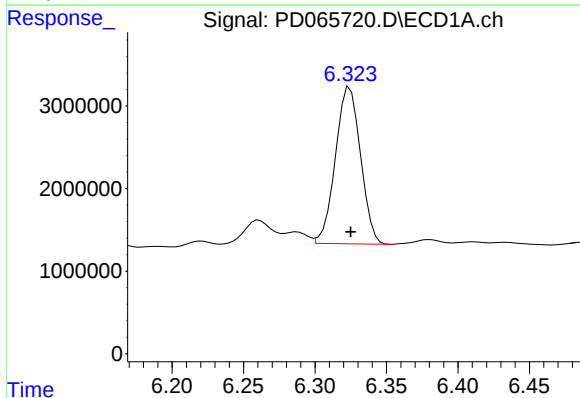


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 23228115
Conc: 503.20 ng/ml

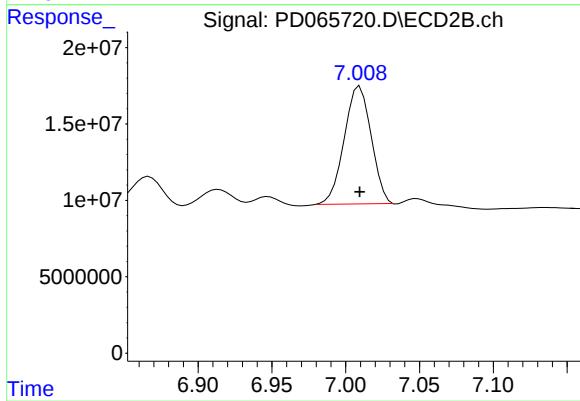

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 97867460
Conc: 506.41 ng/ml

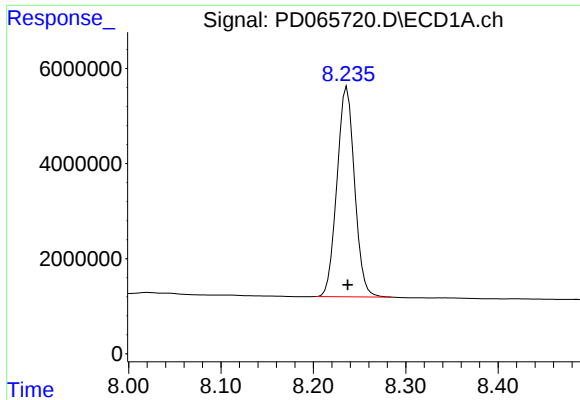

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 58577425
Conc: 52.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091421CHLOR

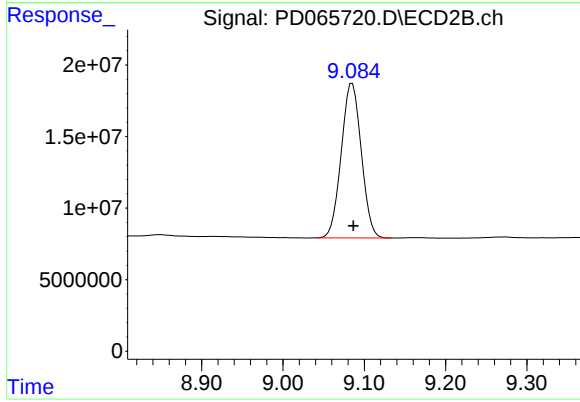

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.001 min
Response: 184587527
Conc: 53.15 ng/ml