

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091423\
 Data File : PD077931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 16:08
 Operator : AR\AJ
 Sample : PB155522BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 22:46:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.758	48334158	30445864	19.036	19.250
28)	SA Decachlor...	9.092	7.902	67867852	36503667	22.279	21.154
Target Compounds							
2)	A alpha-BHC	0.000	3.247	0	119591	N.D.	0.052 #
3)	MA gamma-BHC...	0.000	3.603	0	243208	N.D.	0.109 #
4)	MA Heptachlor	0.000	3.909f	0	42677	N.D.	0.019 #
5)	MB Aldrin	0.000	4.197	0	183285	N.D.	0.080 #
6)	B beta-BHC	0.000	3.893	0	114016	N.D.	0.128 #
7)	B delta-BHC	4.777	0.000	1573972	0	0.427	N.D. #
8)	B Heptachlo...	5.697	0.000	514710	0	0.144	N.D. #
13)	MA Dieldrin	6.374f	0.000	408525	0	0.115	N.D. #
21)	B Endrin ke...	7.657	0.000	597633	0	0.184	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091423\
Data File : PD077931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 16:08
Operator : AR\AJ
Sample : PB155522BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 22:46:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

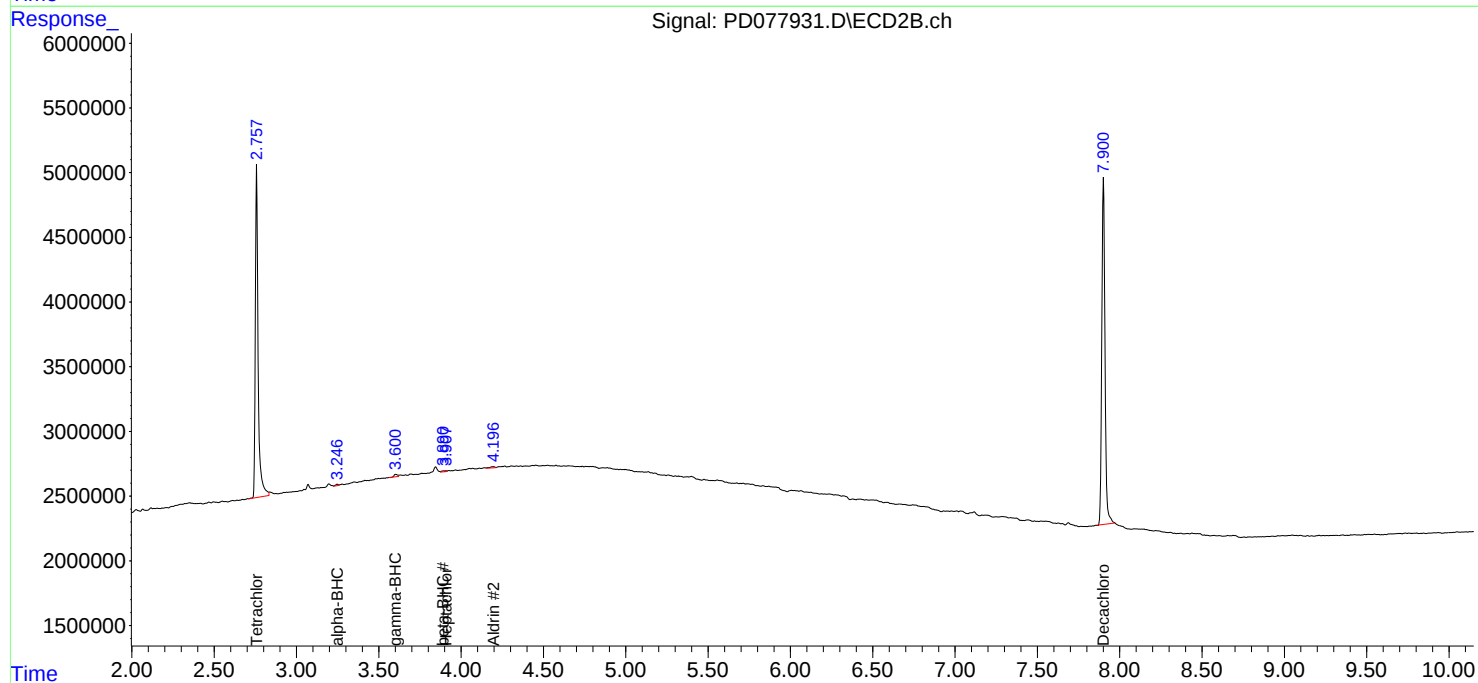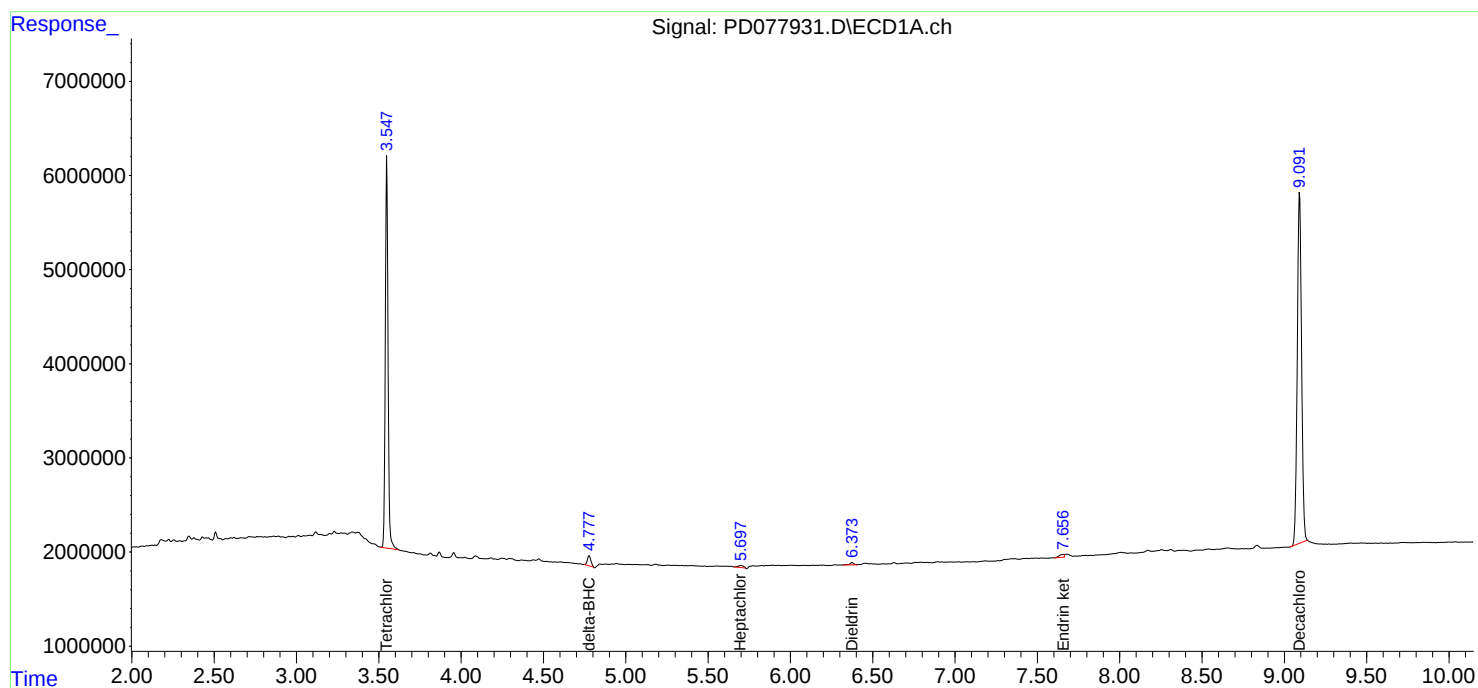


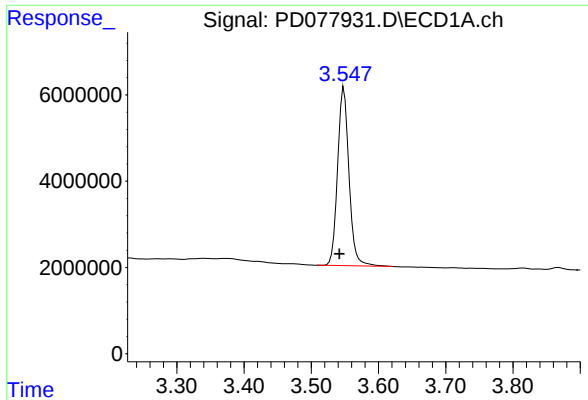

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.006 min
Response: 48334158
Conc: 19.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

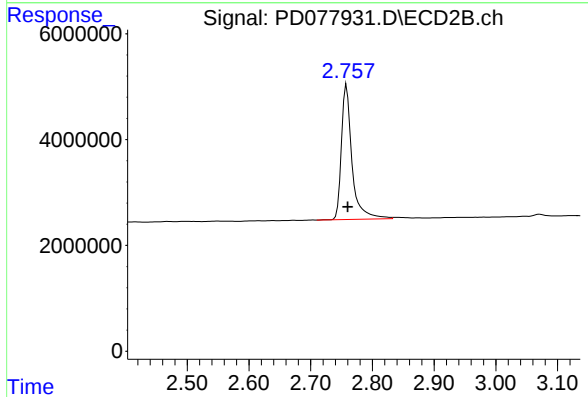


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.002 min
Response: 30445864
Conc: 19.25 ng/ml

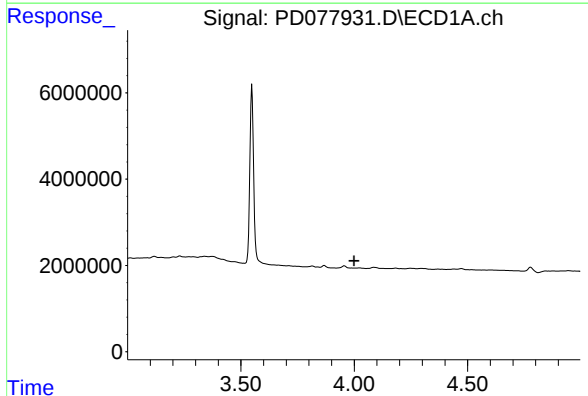


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.999 min
Response: 0
Conc: N.D.

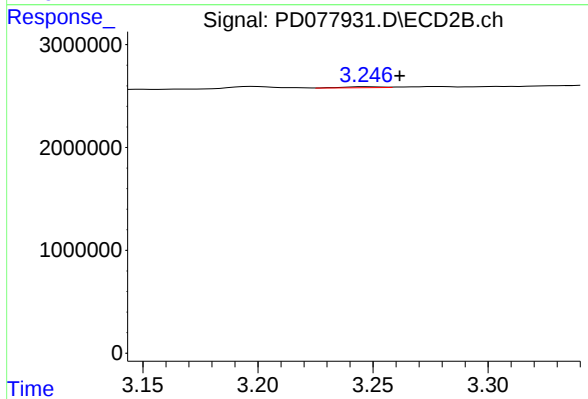

#2 alpha-BHC


R.T.: 3.247 min
Delta R.T.: -0.014 min
Response: 119591
Conc: 0.05 ng/ml

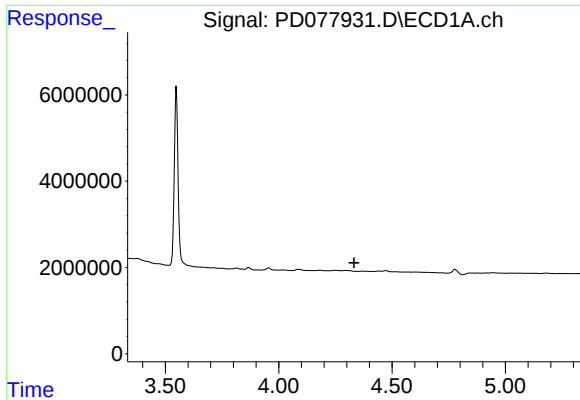

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

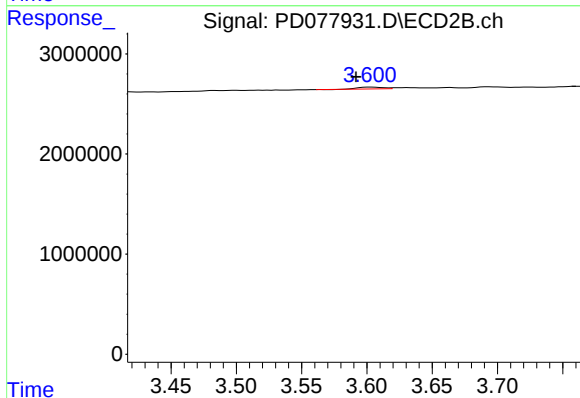


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.011 min
Response: 243208
Conc: 0.11 ng/ml

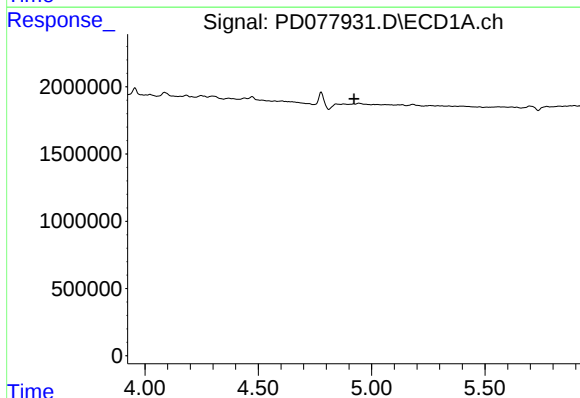


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.923 min
Response: 0
Conc: N.D.

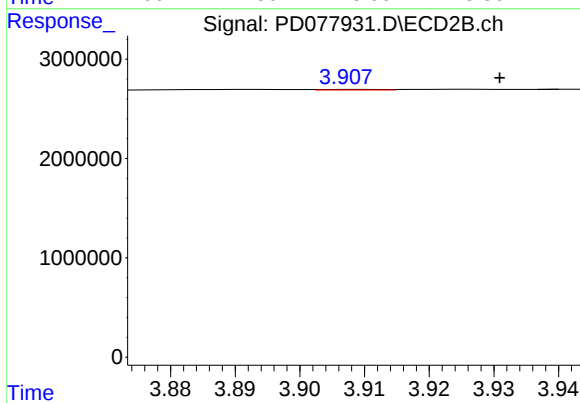

#4 Heptachlor


R.T.: 3.909 min
Delta R.T.: -0.022 min
Response: 42677
Conc: 0.02 ng/ml

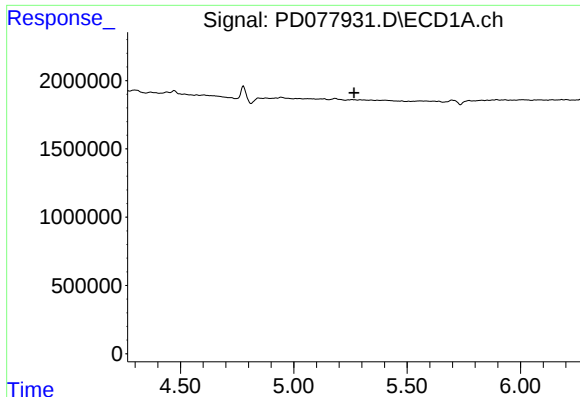

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

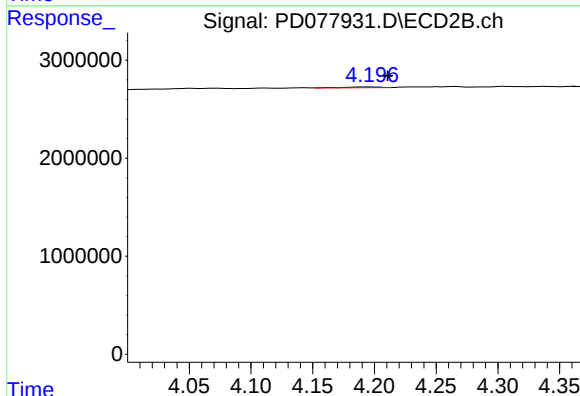


#5 Aldrin

R.T.: 4.197 min
Delta R.T.: -0.013 min
Response: 183285
Conc: 0.08 ng/ml

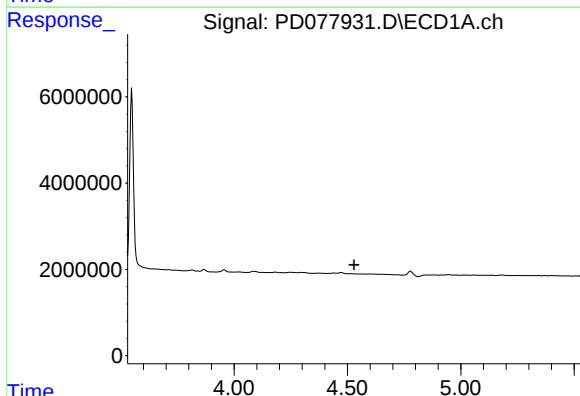


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.529 min
Response: 0
Conc: N.D.

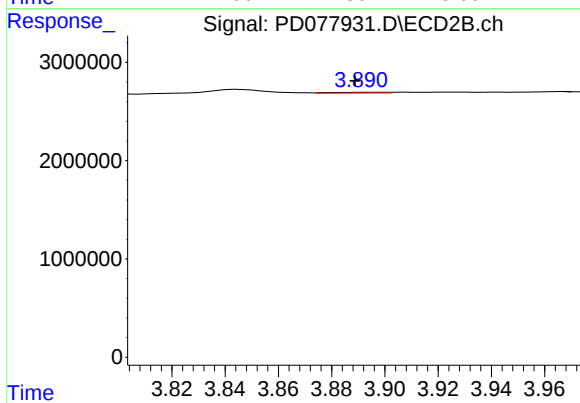

#6 beta-BHC


R.T.: 3.893 min
Delta R.T.: 0.004 min
Response: 114016
Conc: 0.13 ng/ml

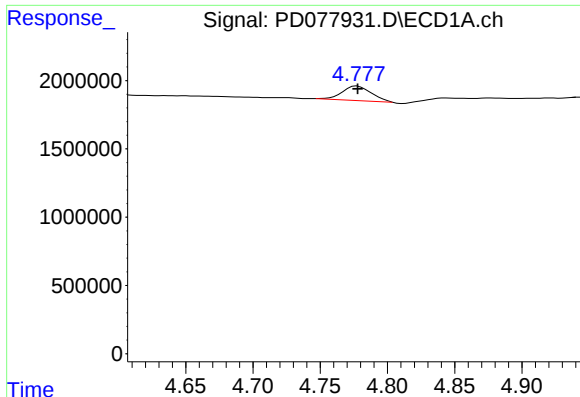

#7 delta-BHC


R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 1573972
Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

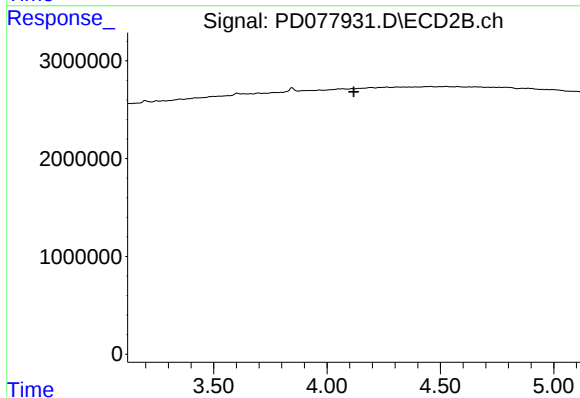


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.119 min
Response: 0
Conc: N.D.

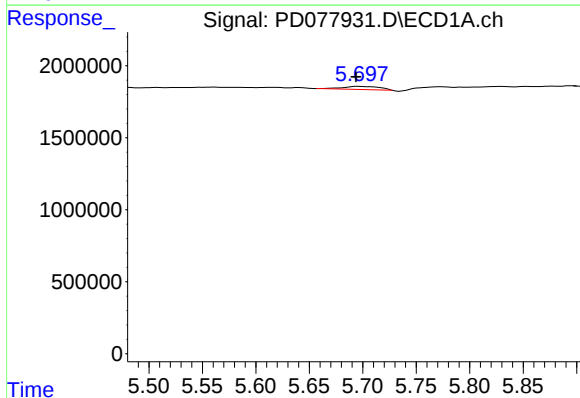


#8 Heptachlor epoxide

R.T.: 5.697 min
Delta R.T.: 0.003 min
Response: 514710
Conc: 0.14 ng/ml

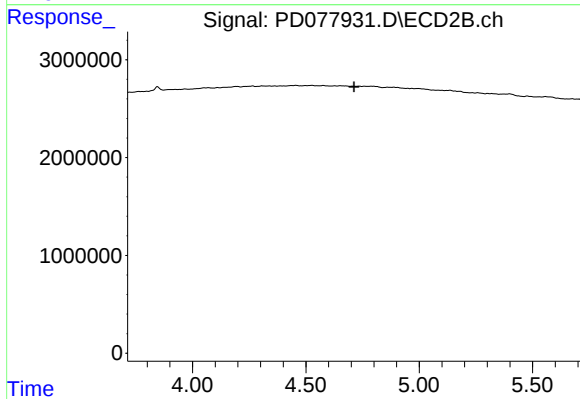

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.713 min
Response: 0
Conc: N.D.

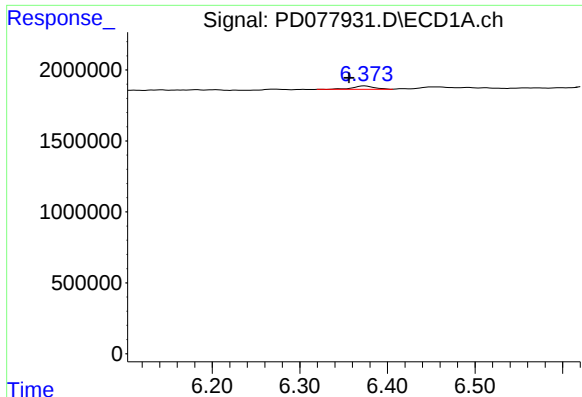

#13 Dieldrin


R.T.: 6.374 min
Delta R.T.: 0.018 min
Response: 408525
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

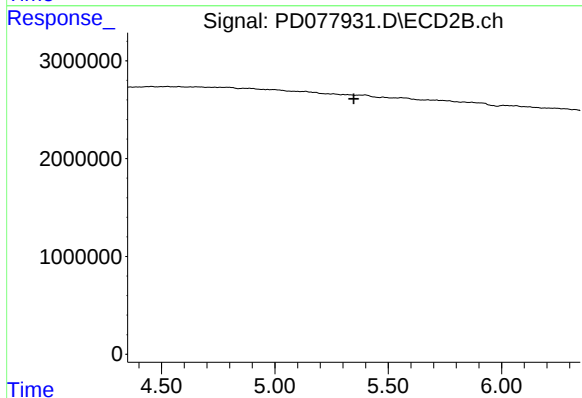


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.348 min
Response: 0
Conc: N.D.

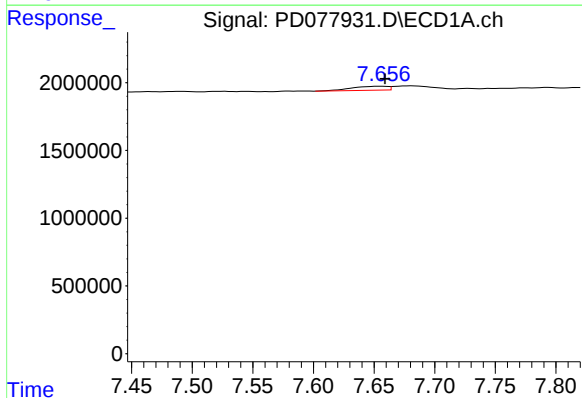


#21 Endrin ketone

R.T.: 7.657 min
Delta R.T.: -0.002 min
Response: 597633
Conc: 0.18 ng/ml

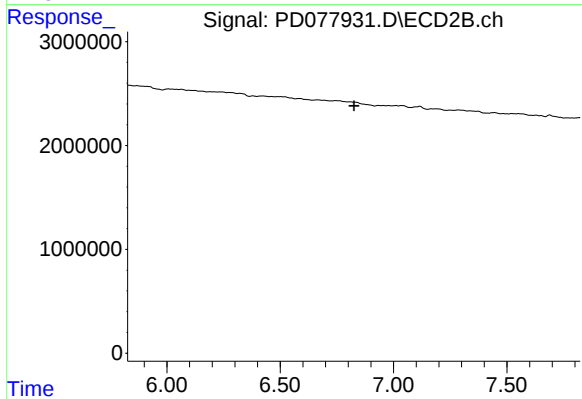

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.827 min
Response: 0
Conc: N.D.

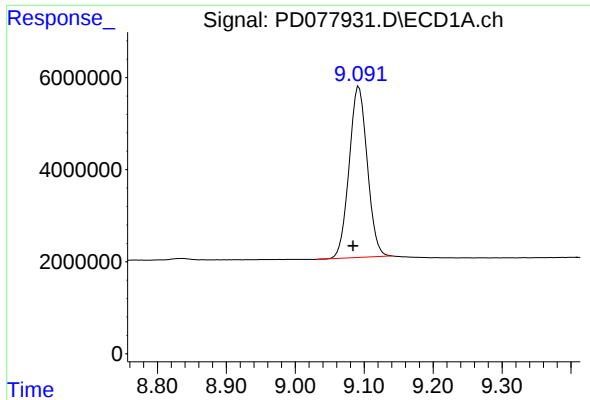

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.009 min
Response: 67867852
Conc: 22.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

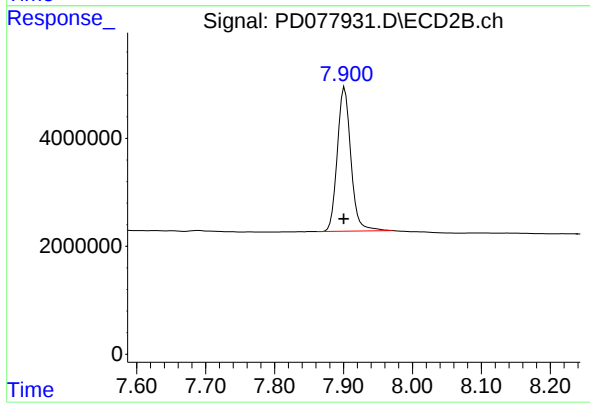

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.001 min
Response: 36503667
Conc: 21.15 ng/ml