

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091423\
 Data File : PD077935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 17:17
 Operator : AR\AJ
 Sample : 04397-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B103-04

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/14/2023
 Supervised By : Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 22:49:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.760	24136877	16185625	9.506	10.233
28) SA Decachlor...	9.082	7.898	25001673	12850452	8.207	7.447
Target Compounds						
17) MA 4,4'-DDT	7.032	6.015	848856	835123	0.325m	0.591m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091423\
Data File : PD077935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 17:17
Operator : AR\AJ
Sample : 04397-04
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B103-04


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/14/2023
Supervised By : Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 22:49:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

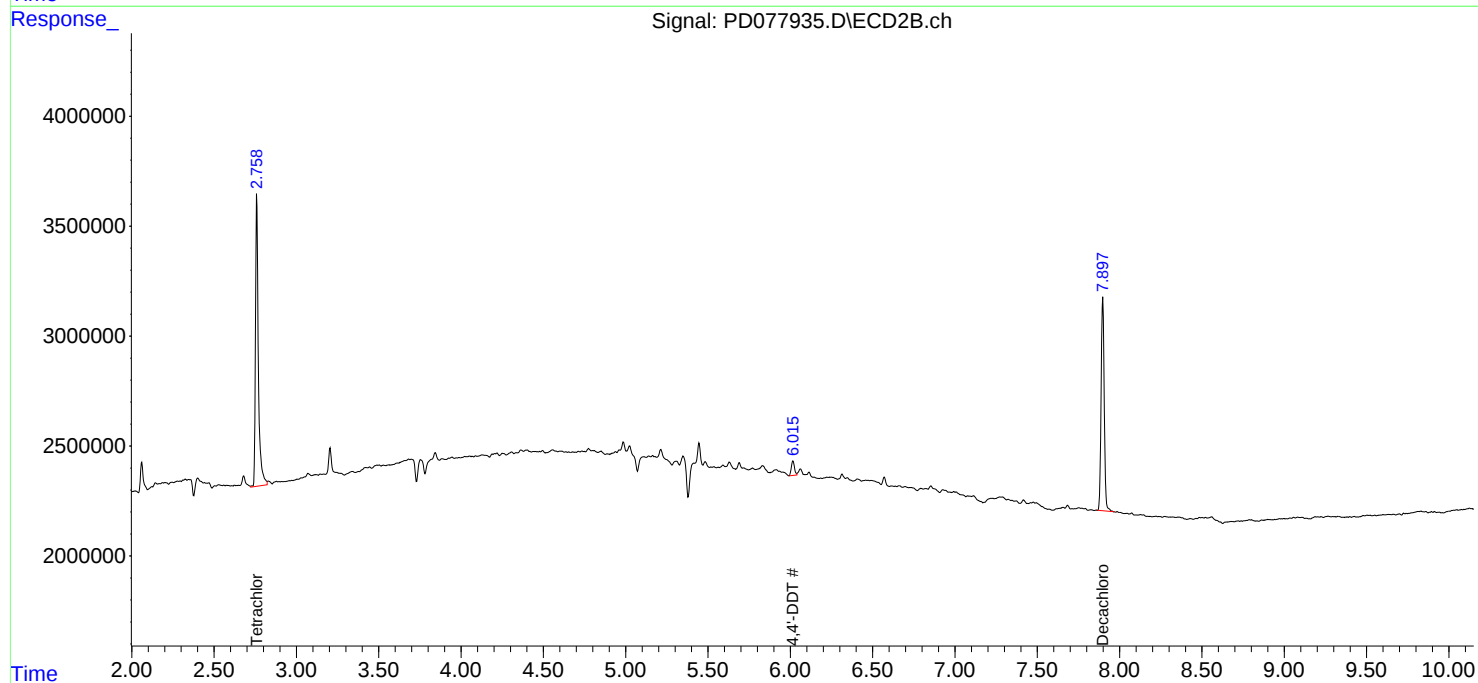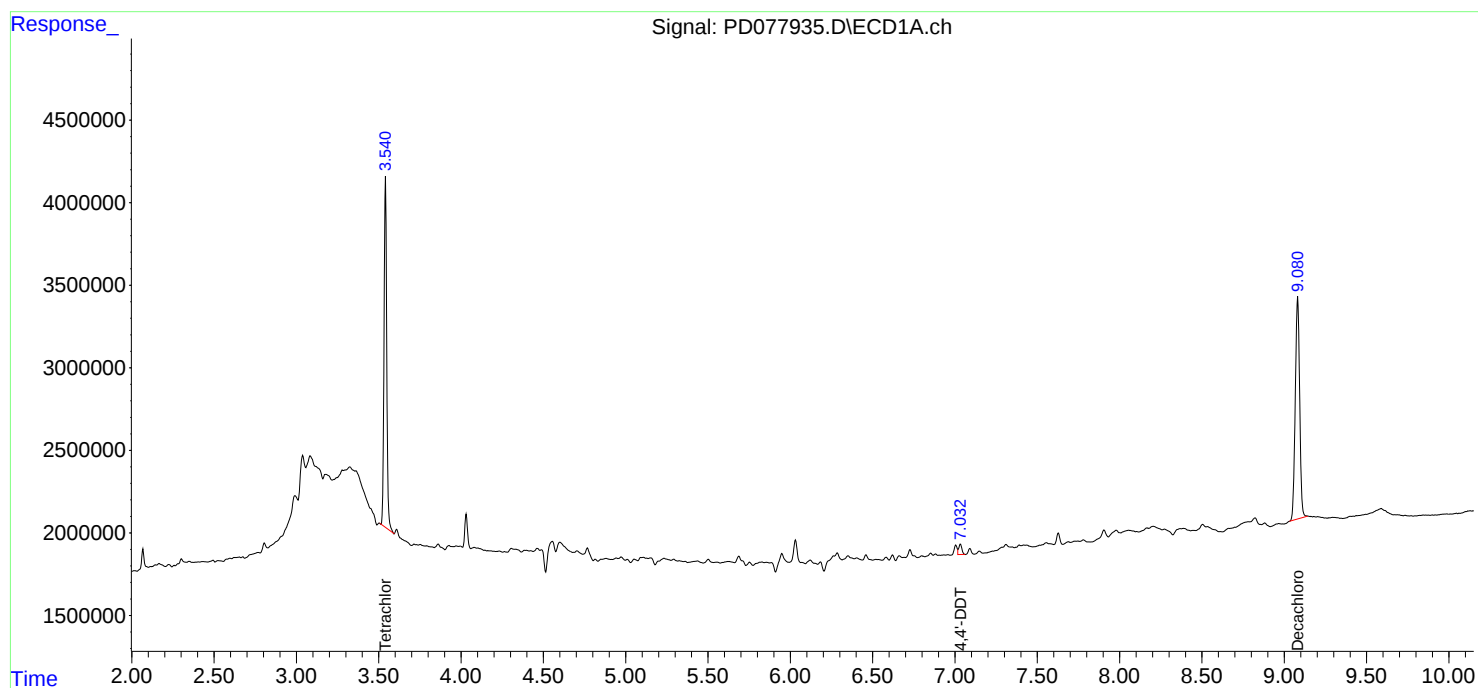

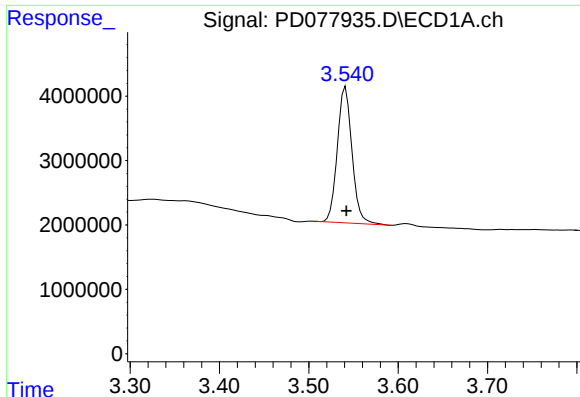


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 24136877
Conc: 9.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
B103-04


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

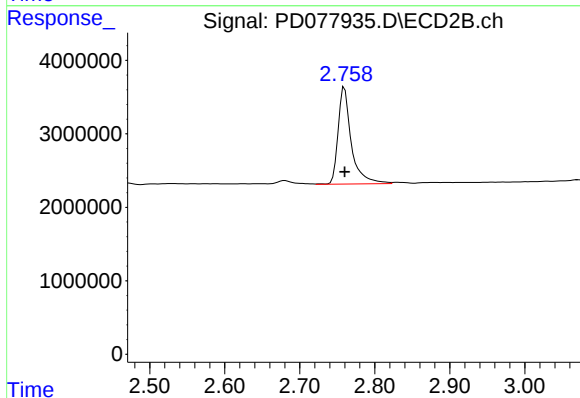


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 16185625
Conc: 10.23 ng/ml

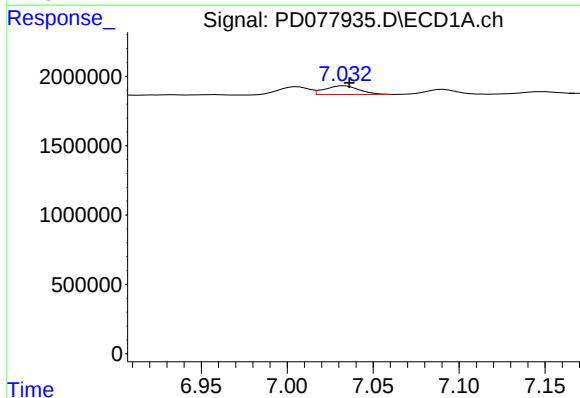


#17 4,4'-DDT

R.T.: 7.032 min
Delta R.T.: -0.004 min
Response: 848856
Conc: 0.32 ng/ml m

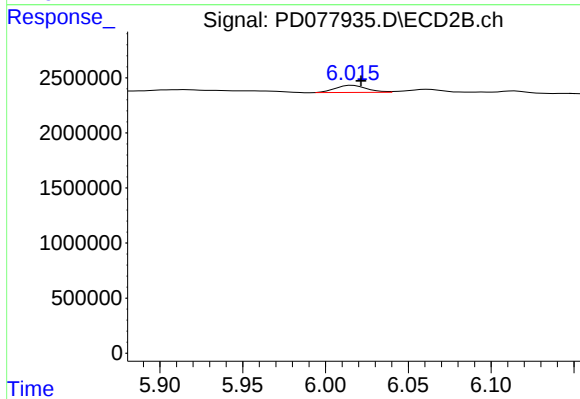

#17 4,4'-DDT

R.T.: 6.015 min
Delta R.T.: -0.007 min
Response: 835123
Conc: 0.59 ng/ml m

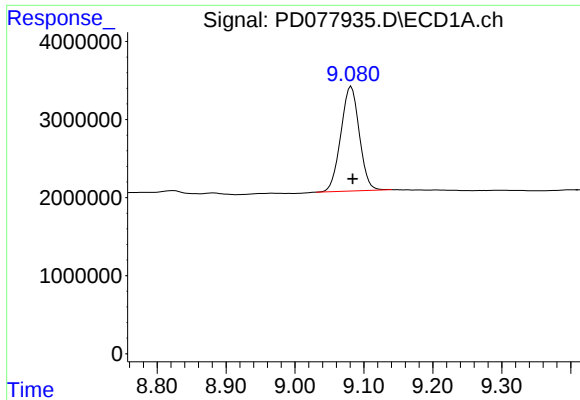


#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.002 min
Response: 25001673
Conc: 8.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
B103-04

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

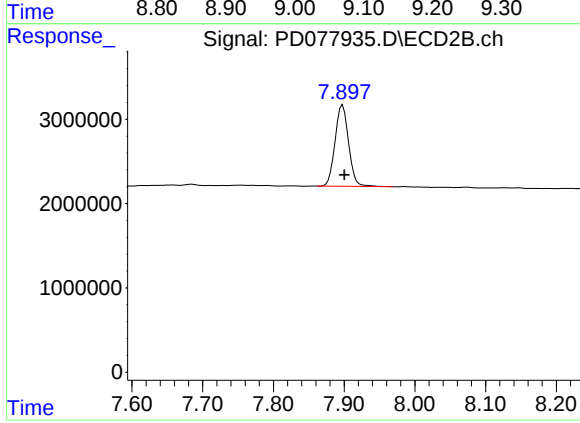

#28 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.002 min
Response: 12850452
Conc: 7.45 ng/ml