

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 14:25
 Operator : AR\AJ
 Sample : P3993-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:05:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.903	23653871	50332261	23.387	14.223 #
2)	SA Decachlor...	9.033	8.102	18373919	47404940	14.069	13.633
Target Compounds							
4)	MA Heptachlor	0.000	4.088	0	10509726	N.D.	2.469
6)	B beta-BHC	0.000	4.088f	0	10509726	N.D.	4.848
7)	B delta-BHC	4.762	0.000	5686213	0	3.467	N.D. #
19)	B Endosulfa...	0.000	6.450f	0	4116392	N.D.	1.153


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 14:25
Operator : AR\AJ
Sample : P3993-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:05:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

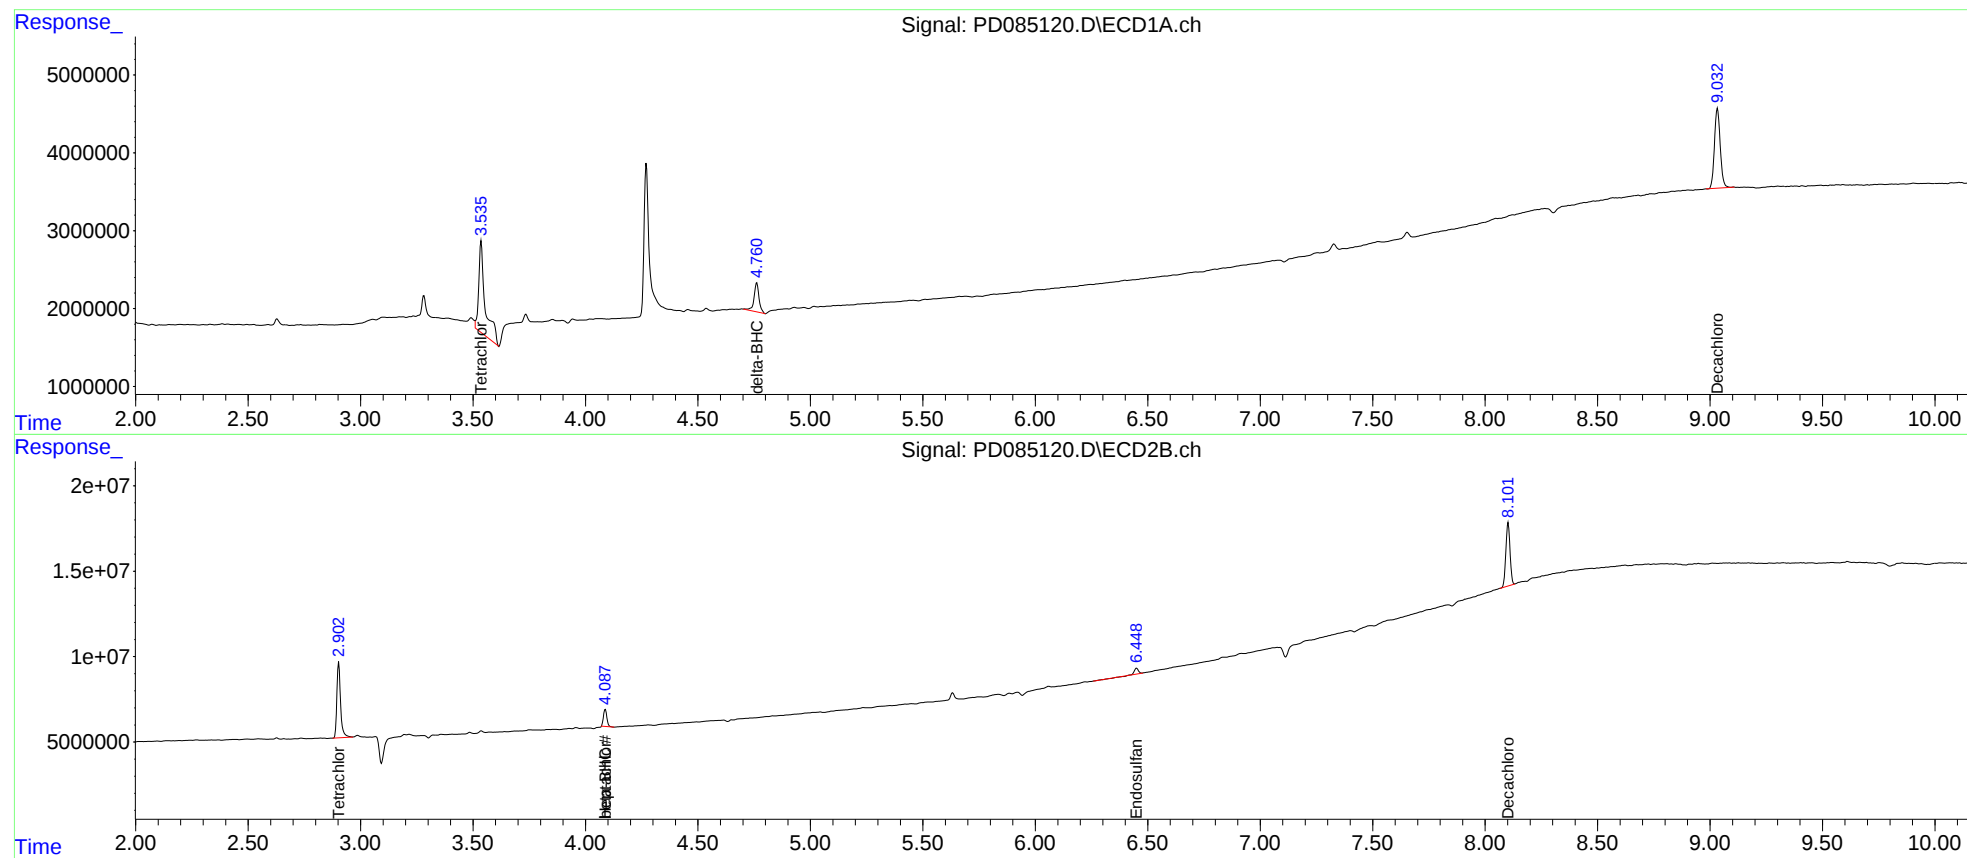

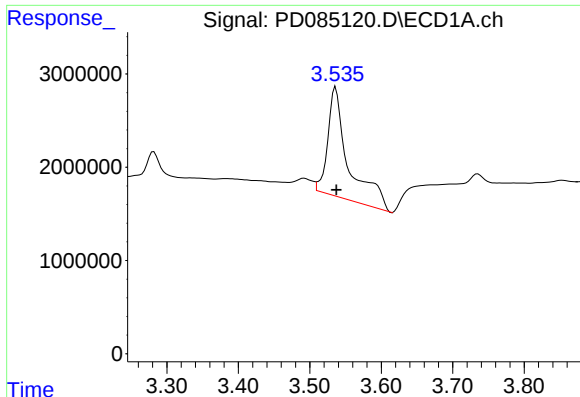


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 23653871
Conc: 23.39 ng/ml

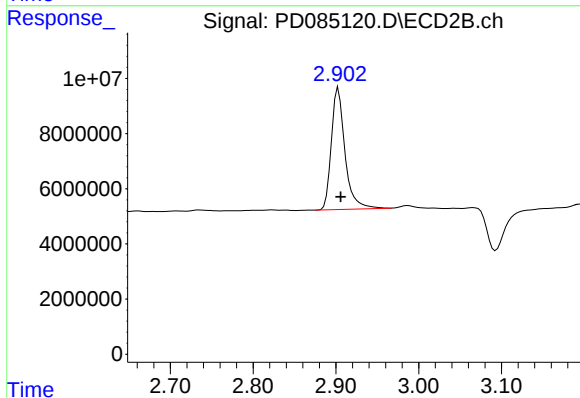


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.003 min
Response: 50332261
Conc: 14.22 ng/ml

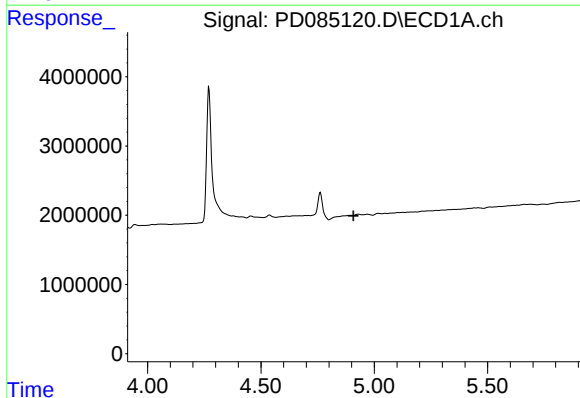


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

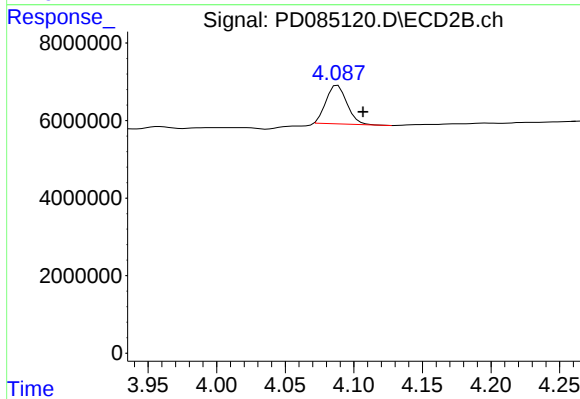


#4 Heptachlor

R.T.: 4.088 min
Delta R.T.: -0.018 min
Response: 10509726
Conc: 2.47 ng/ml

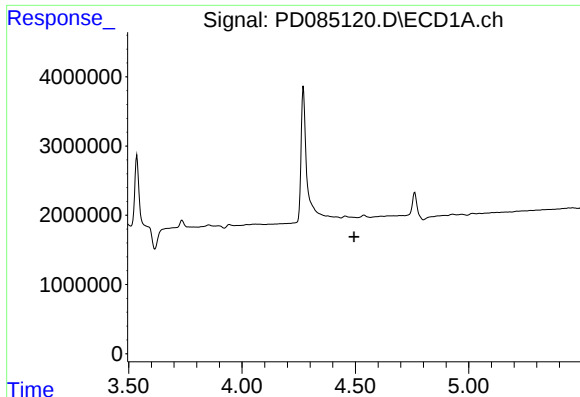


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.495 min
Response: 0
Conc: N.D.

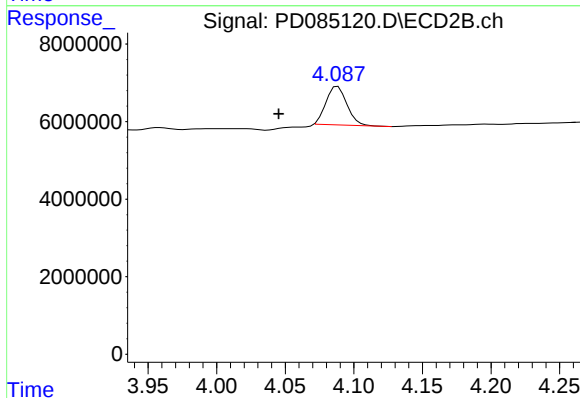


#6 beta-BHC

R.T.: 4.088 min
Delta R.T.: 0.043 min
Response: 10509726
Conc: 4.85 ng/ml

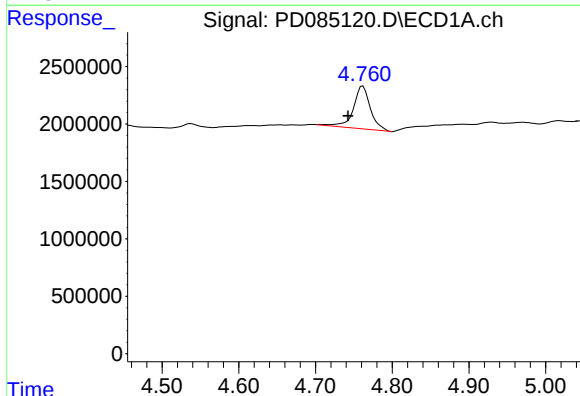


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: 0.019 min
Response: 5686213
Conc: 3.47 ng/ml

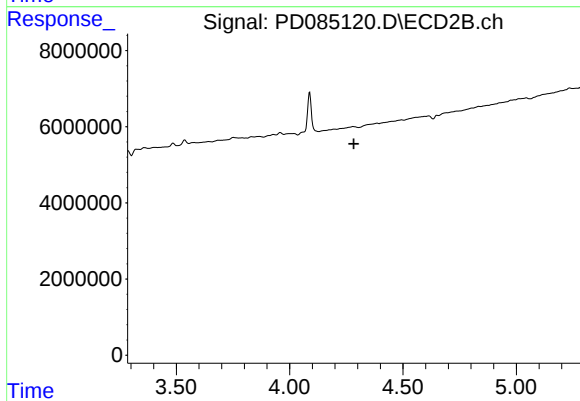


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

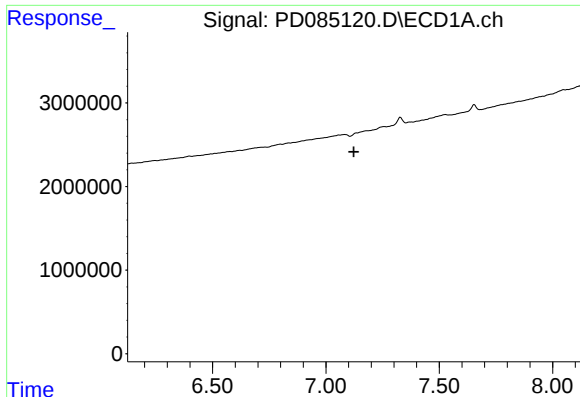


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

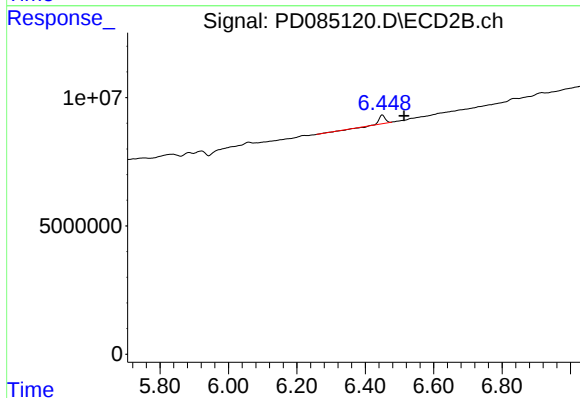


#19 Endosulfan Sulfate

R.T.: 6.450 min
Delta R.T.: -0.063 min
Response: 4116392
Conc: 1.15 ng/ml

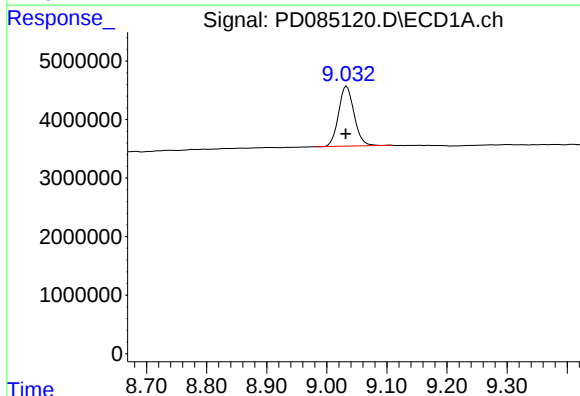

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.002 min
Response: 18373919
Conc: 14.07 ng/ml

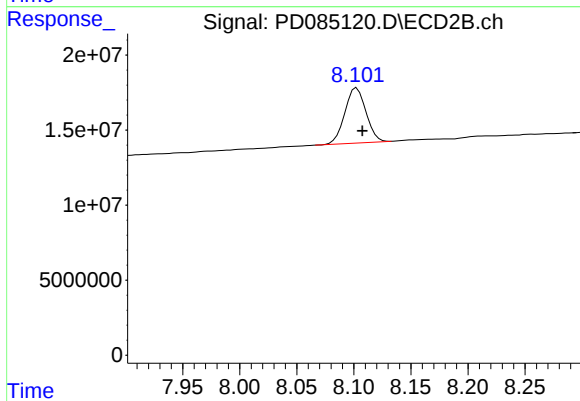

#27 Decachlorobiphenyl

R.T.: 8.102 min
Delta R.T.: -0.005 min
Response: 47404940
Conc: 13.63 ng/ml