

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 14:51
 Operator : AR\AJ
 Sample : P3993-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:05:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.903	23578439	51766636	23.313	14.628 #
2)	SA Decachlor...	9.033	8.103	15488884	39851187	11.860	11.461
Target Compounds							
4)	MA Heptachlor	0.000	4.088	0	21193114	N.D.	4.978
6)	B beta-BHC	0.000	4.088f	0	21193114	N.D.	9.776
7)	B delta-BHC	4.762	0.000	9974563	0	6.082	N.D. #
19)	B Endosulfa...	0.000	6.451f	0	3238054	N.D.	0.907


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 14:51
Operator : AR\AJ
Sample : P3993-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:05:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

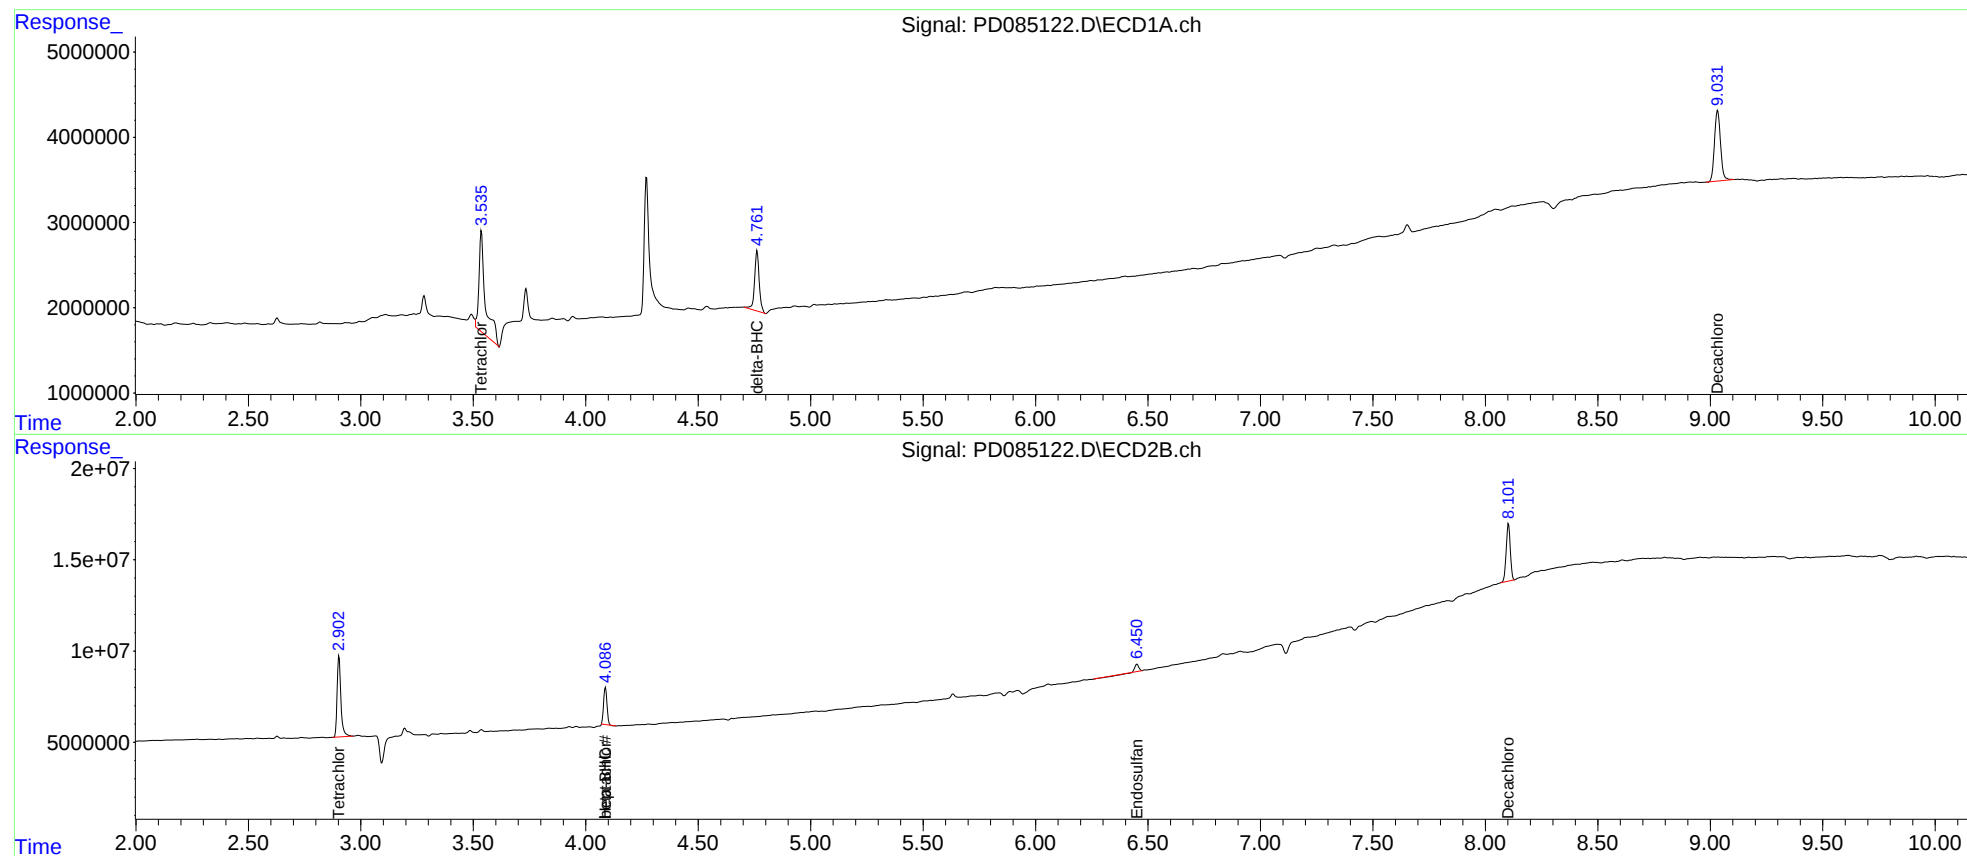

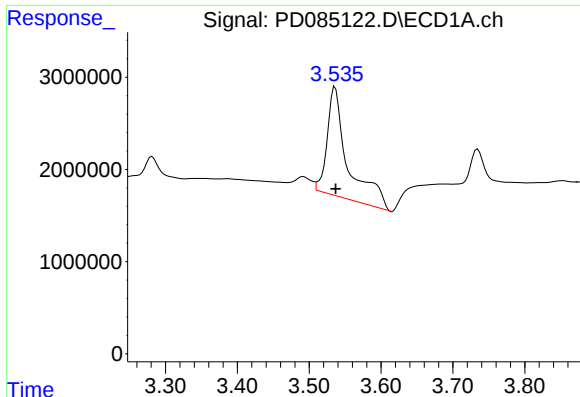


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 23578439
Conc: 23.31 ng/ml

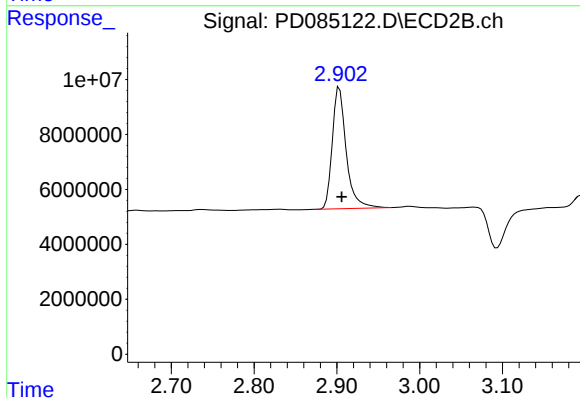


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.003 min
Response: 51766636
Conc: 14.63 ng/ml

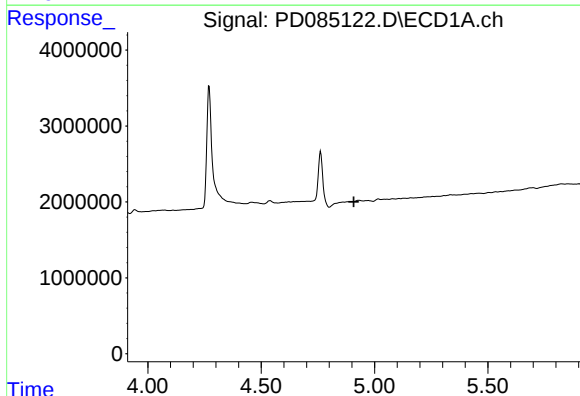


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

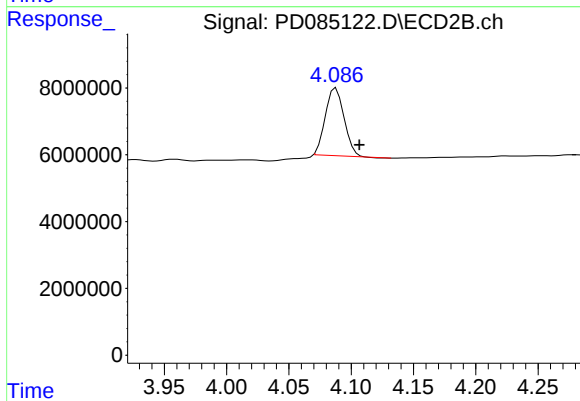


#4 Heptachlor

R.T.: 4.088 min
Delta R.T.: -0.019 min
Response: 21193114
Conc: 4.98 ng/ml

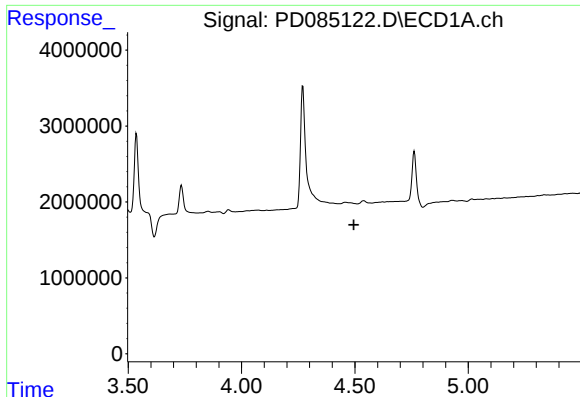


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.495 min
Response: 0
Conc: N.D.

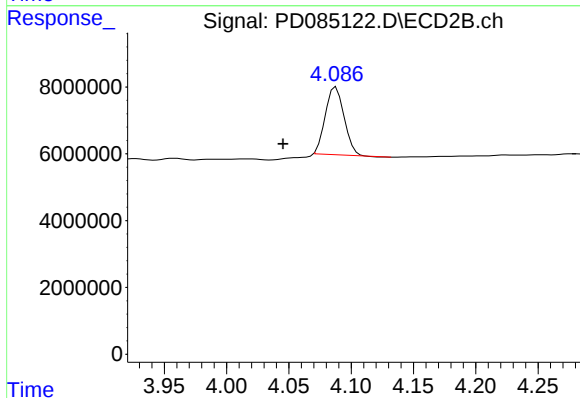


#6 beta-BHC

R.T.: 4.088 min
Delta R.T.: 0.042 min
Response: 21193114
Conc: 9.78 ng/ml

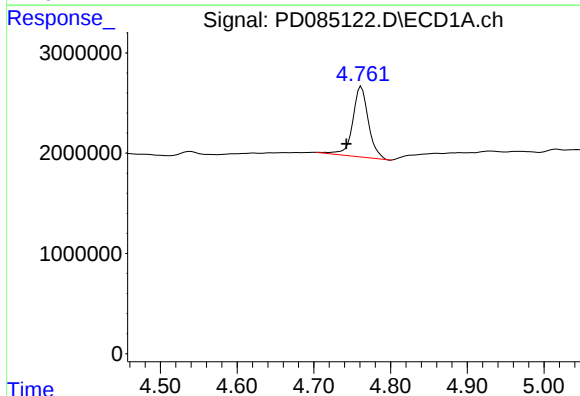


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: 0.019 min
Response: 9974563
Conc: 6.08 ng/ml

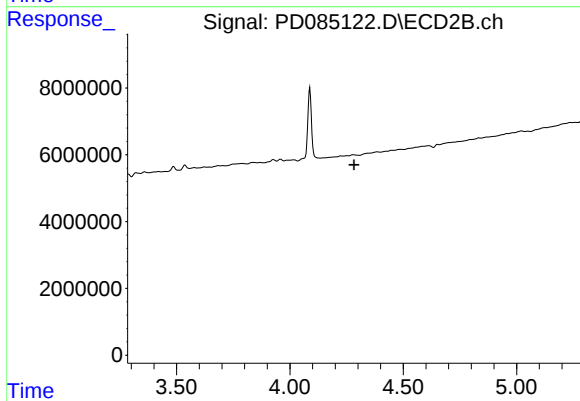


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

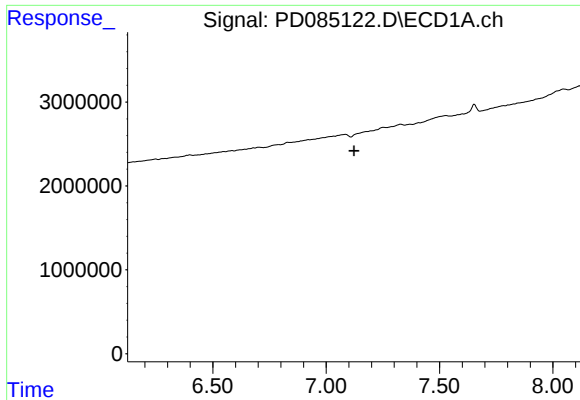


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.123 min
Response: 0
Conc: N.D.

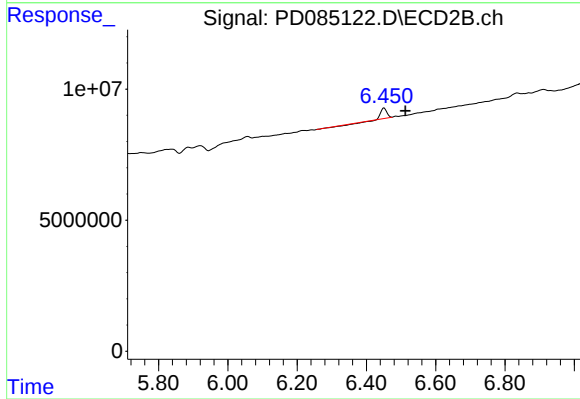


#19 Endosulfan Sulfate

R.T.: 6.451 min
Delta R.T.: -0.062 min
Response: 3238054
Conc: 0.91 ng/ml

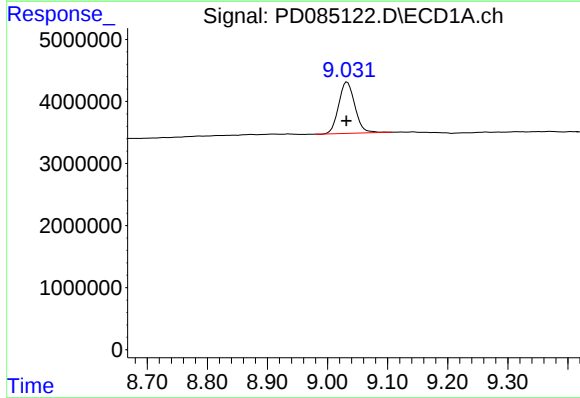

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.001 min
Response: 15488884
Conc: 11.86 ng/ml

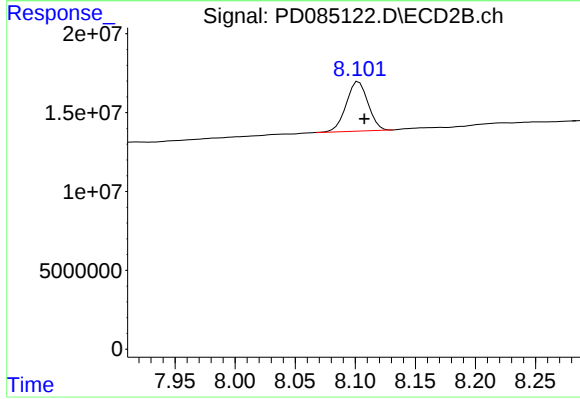

#27 Decachlorobiphenyl

R.T.: 8.103 min
Delta R.T.: -0.005 min
Response: 39851187
Conc: 11.46 ng/ml