

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 15:05
 Operator : AR\AJ
 Sample : P3993-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:06:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.903	22529140	48049111	22.275	13.578 #
27)	SA Decachlor...	9.033	8.102	14735417	37397003	11.283	10.755
Target Compounds							
4)	MA Heptachlor	0.000	4.088	0	20164878	N.D.	4.737
6)	B beta-BHC	0.000	4.088f	0	20164878	N.D.	9.301
7)	B delta-BHC	4.762	0.000	9774567	0	5.960	N.D. #
19)	B Endosulfa...	0.000	6.451f	0	4043397	N.D.	1.132


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 15:05
Operator : AR\AJ
Sample : P3993-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:06:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

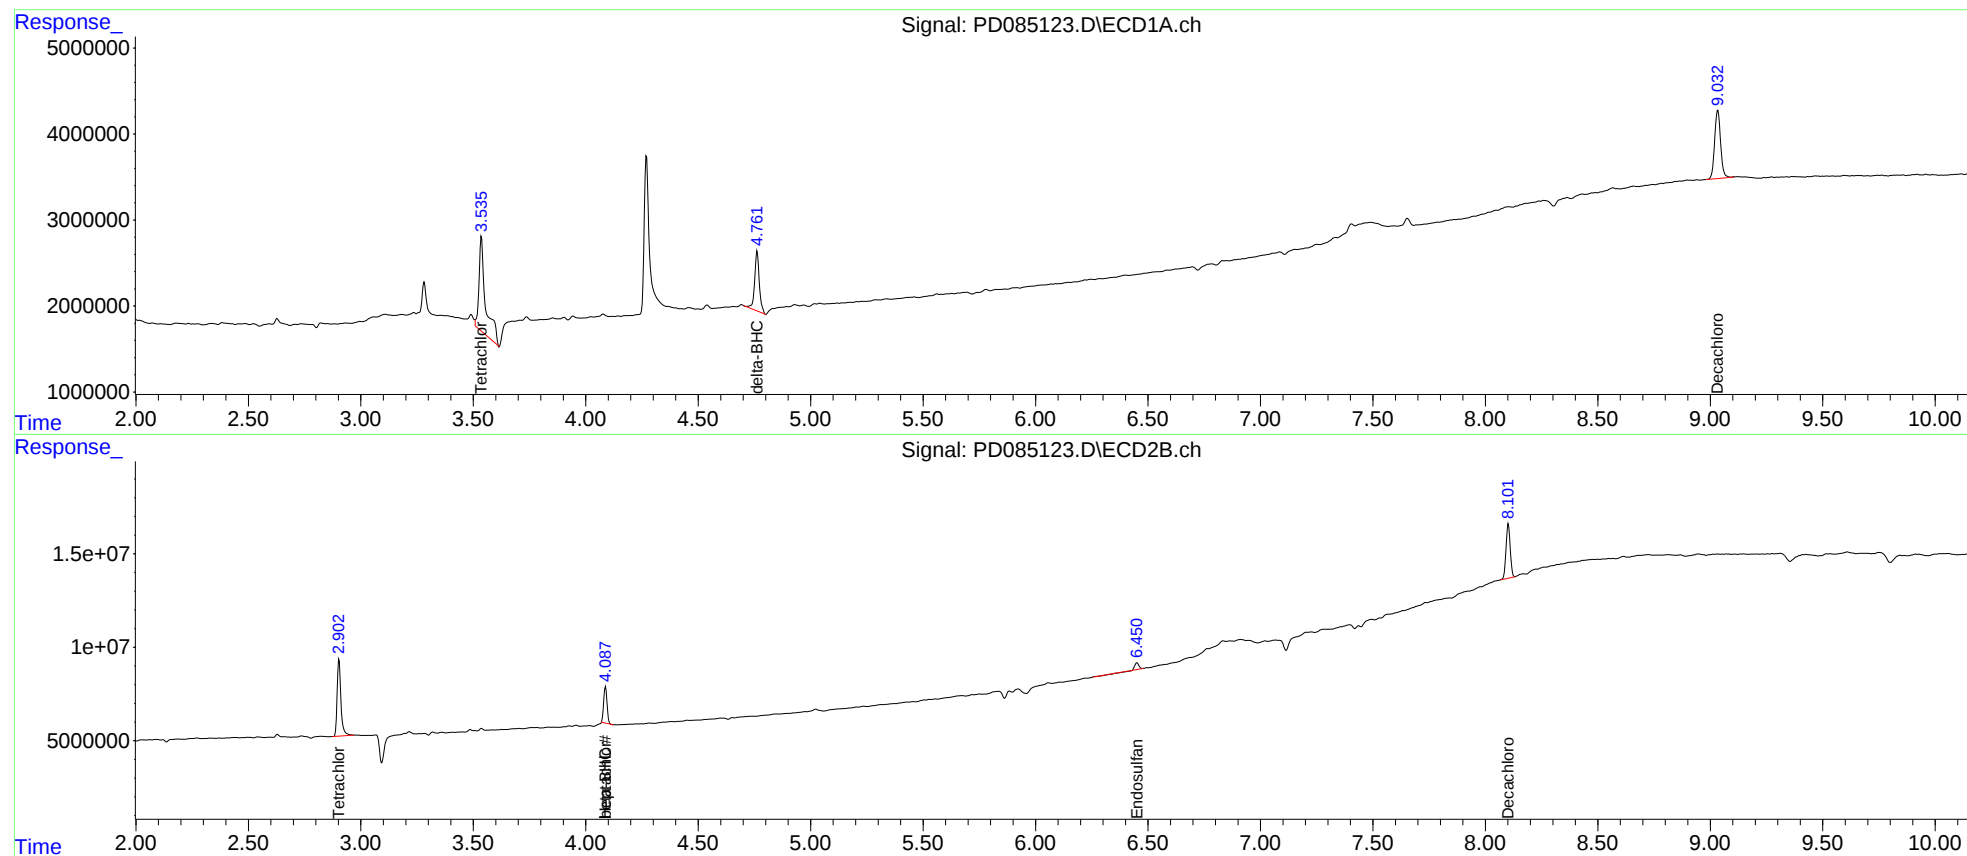

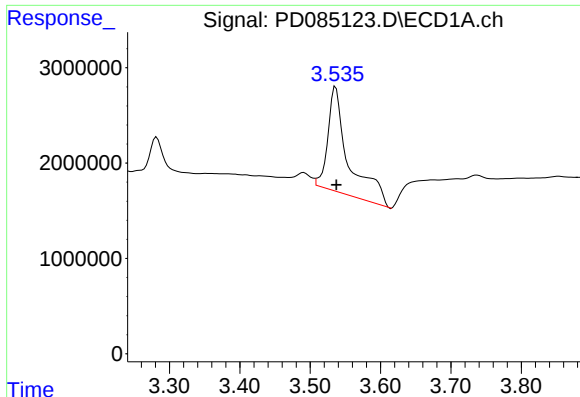


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 22529140
Conc: 22.28 ng/ml

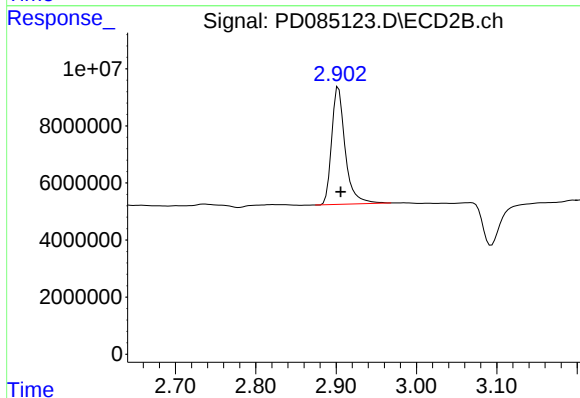


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.003 min
Response: 48049111
Conc: 13.58 ng/ml

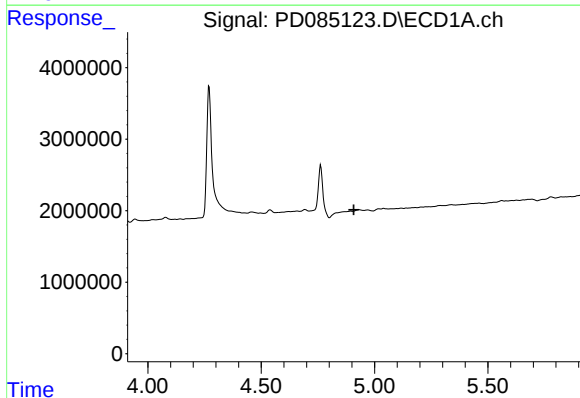


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

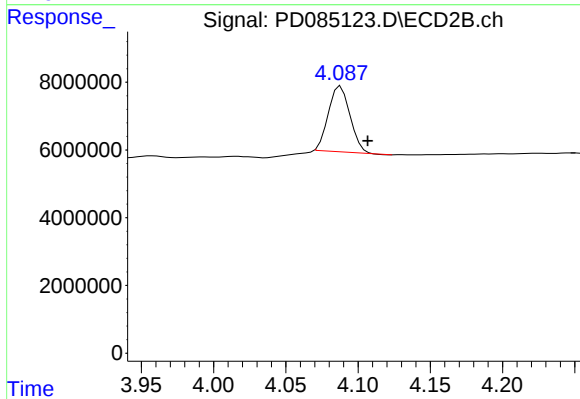


#4 Heptachlor

R.T.: 4.088 min
Delta R.T.: -0.019 min
Response: 20164878
Conc: 4.74 ng/ml

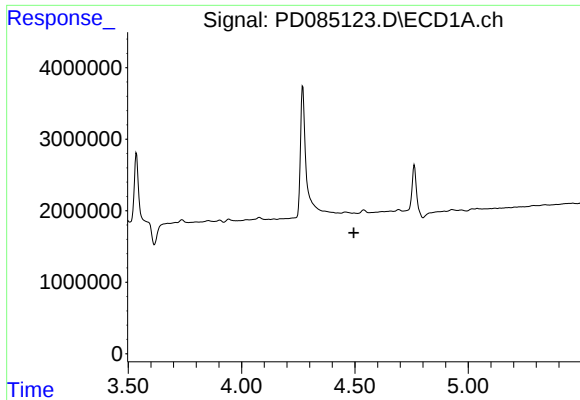


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.495 min
Response: 0
Conc: N.D.

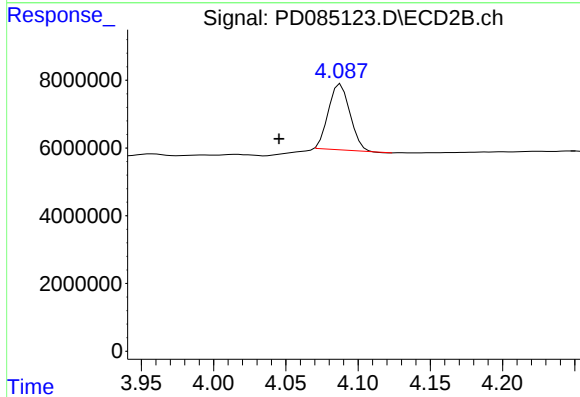


#6 beta-BHC

R.T.: 4.088 min
Delta R.T.: 0.043 min
Response: 20164878
Conc: 9.30 ng/ml

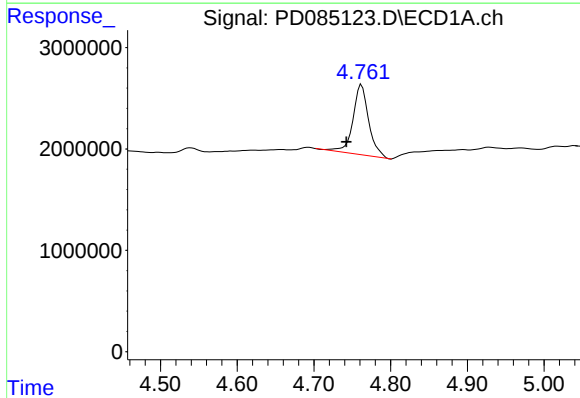


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: 0.020 min
Response: 9774567
Conc: 5.96 ng/ml

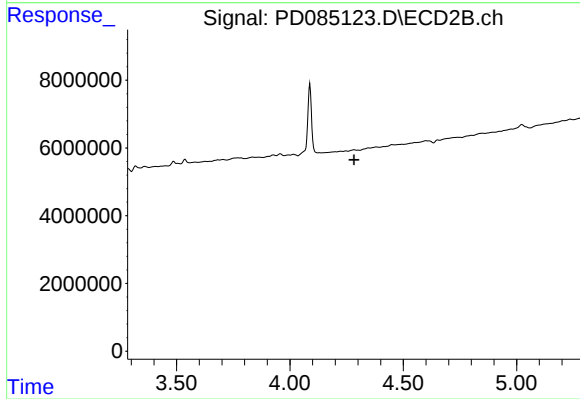


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

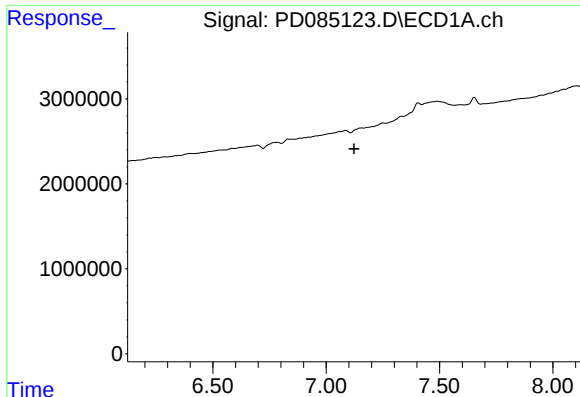


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

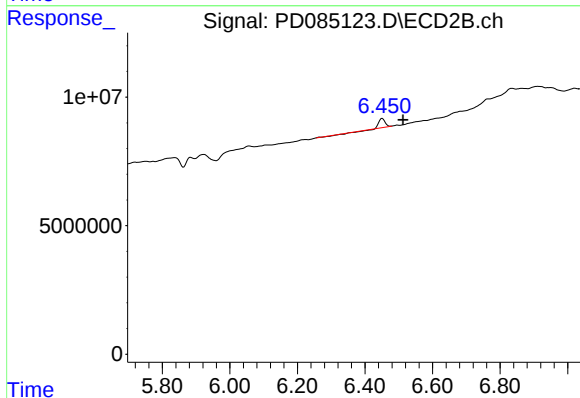


#19 Endosulfan Sulfate

R.T.: 6.451 min
Delta R.T.: -0.062 min
Response: 4043397
Conc: 1.13 ng/ml

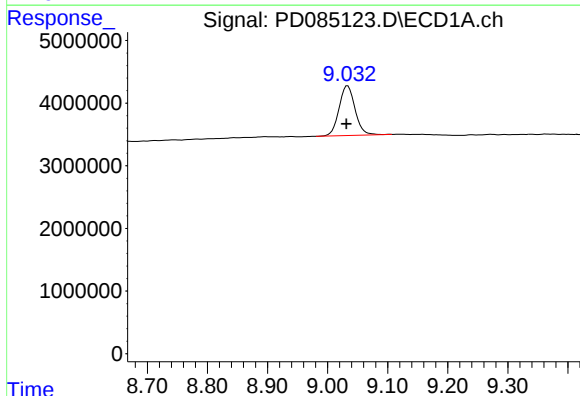

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.002 min
Response: 14735417
Conc: 11.28 ng/ml

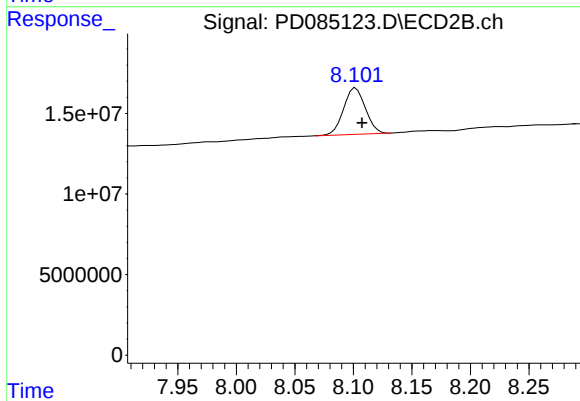

#27 Decachlorobiphenyl

R.T.: 8.102 min
Delta R.T.: -0.005 min
Response: 37397003
Conc: 10.75 ng/ml