

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 18:43
 Operator : AR\AJ
 Sample : P3899-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:09:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.905	18927417	114.3E6	18.714	32.300 #
2)	SA Decachlor...	9.032	8.102	27530264	71817741	21.079	20.654
Target Compounds							
3)	MA gamma-BHC...	4.268f	0.000	112.1E6	0	69.279	N.D. #
4)	MA Heptachlor	0.000	4.088	0	49971778	N.D.	11.739
6)	B beta-BHC	0.000	4.088f	0	49971778	N.D.	23.050
7)	B delta-BHC	4.762	0.000	24457901	0	14.913	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 18:43
Operator : AR\AJ
Sample : P3899-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:09:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

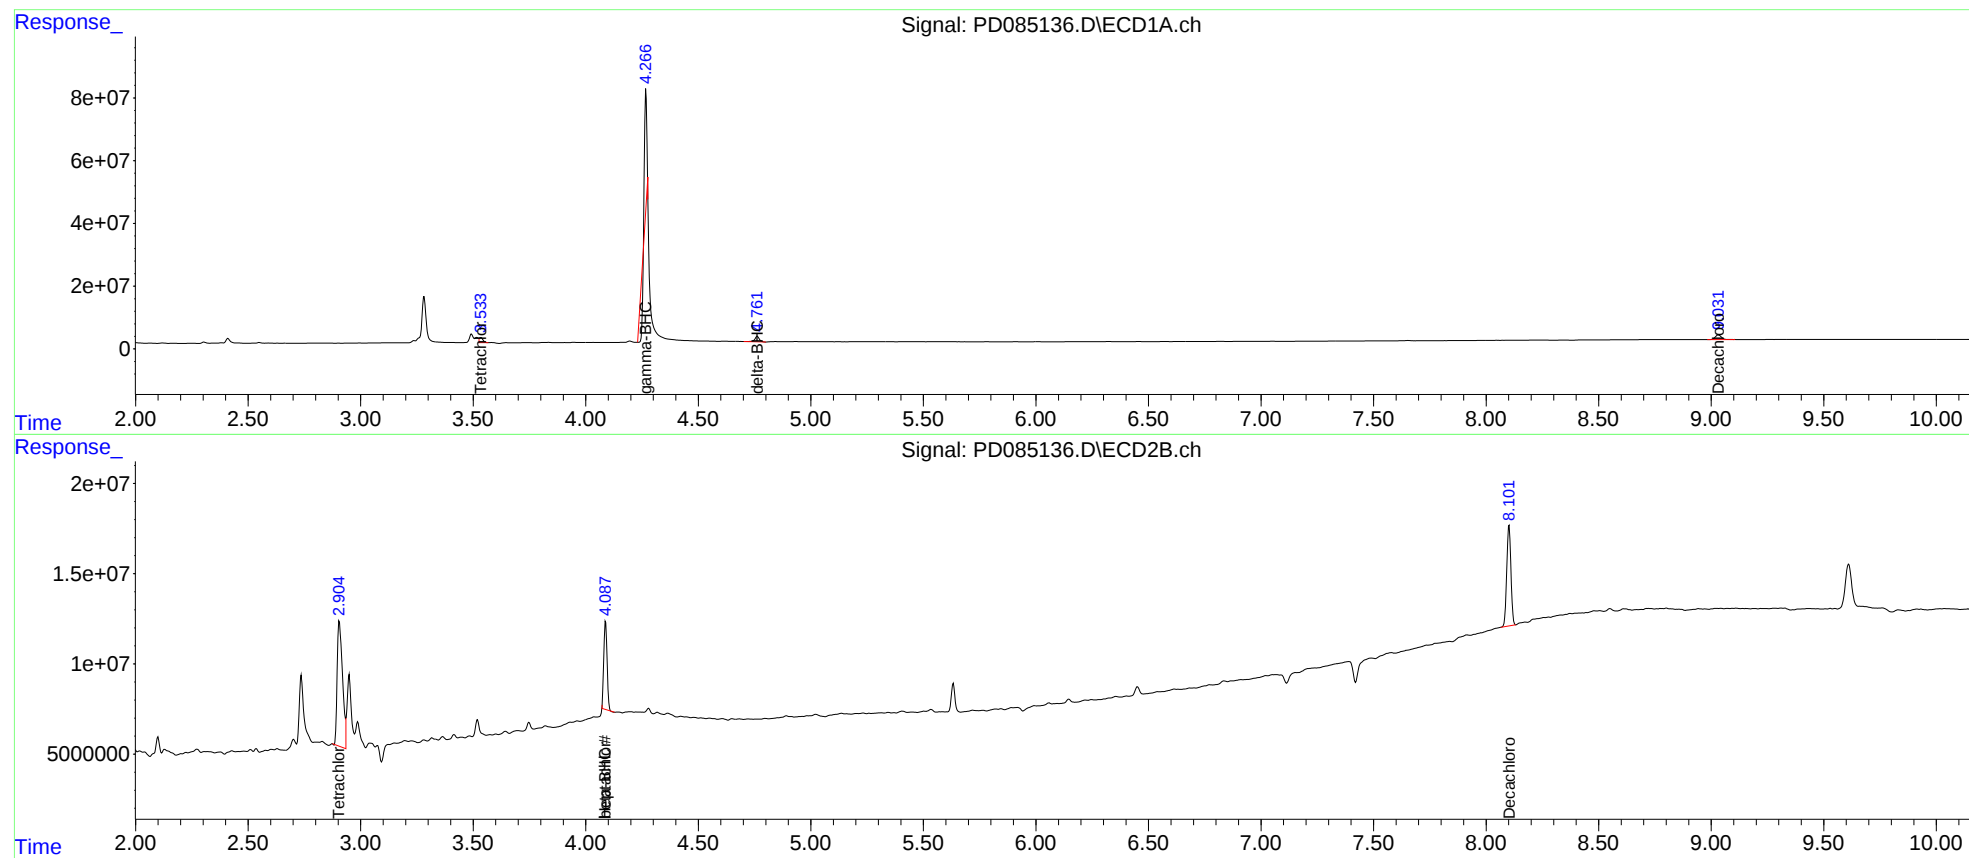

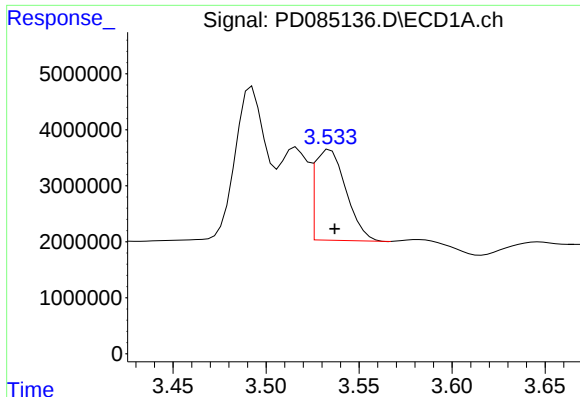


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.003 min
Response: 18927417
Conc: 18.71 ng/ml

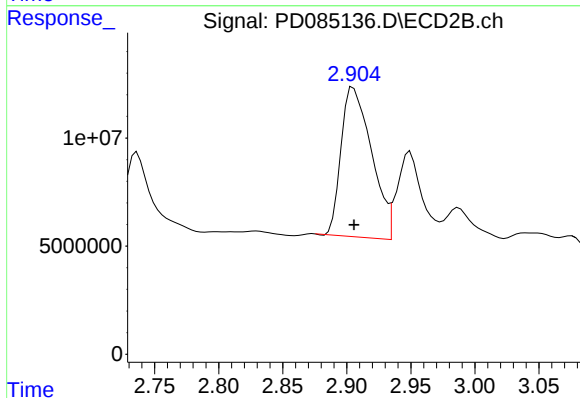


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: 0.000 min
Response: 114303162
Conc: 32.30 ng/ml

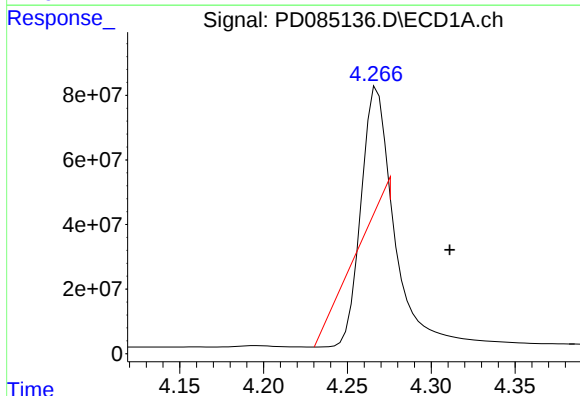


#3 gamma-BHC (Lindane)

R.T.: 4.268 min
Delta R.T.: -0.043 min
Response: 112084016
Conc: 69.28 ng/ml

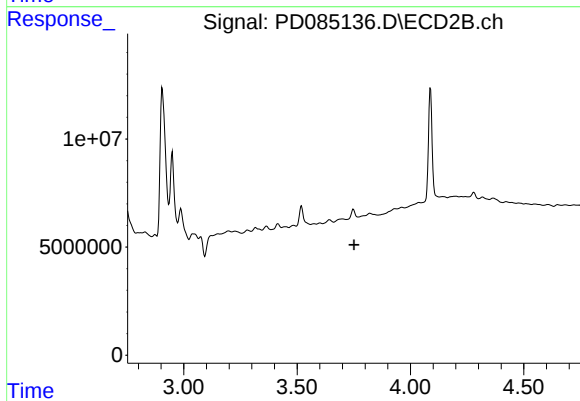


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.752 min
Response: 0
Conc: N.D.

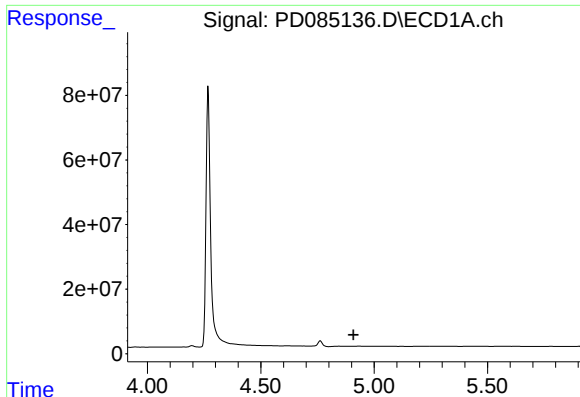


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

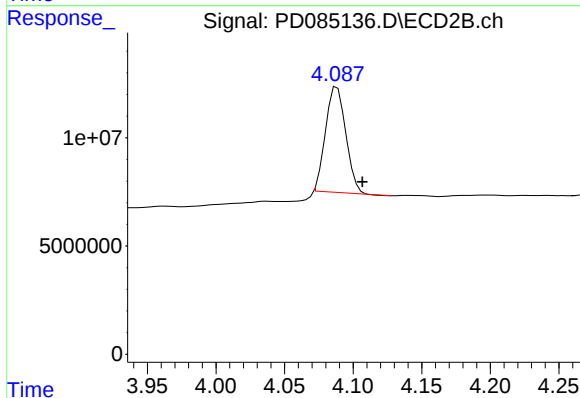


#4 Heptachlor

R.T.: 4.088 min
Delta R.T.: -0.018 min
Response: 49971778
Conc: 11.74 ng/ml

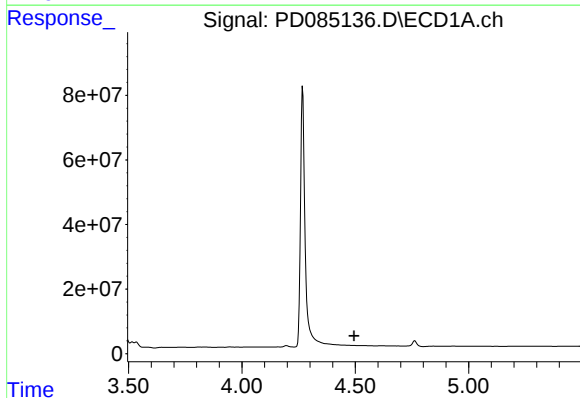


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.495 min
Response: 0
Conc: N.D.

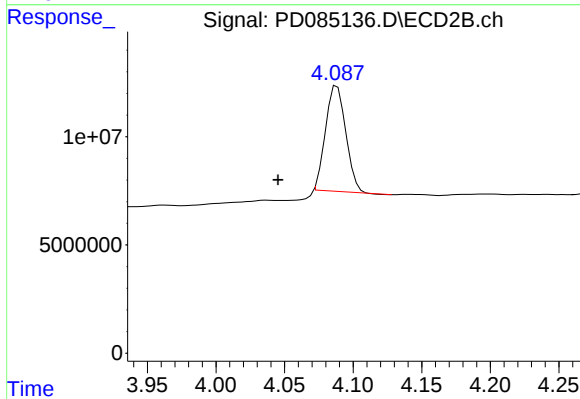


#6 beta-BHC

R.T.: 4.088 min
Delta R.T.: 0.043 min
Response: 49971778
Conc: 23.05 ng/ml

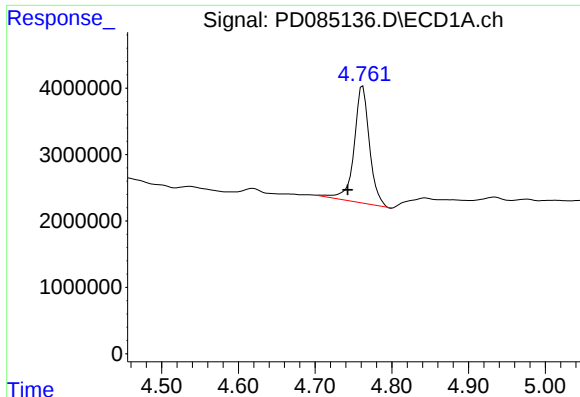


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: 0.020 min
Response: 24457901
Conc: 14.91 ng/ml

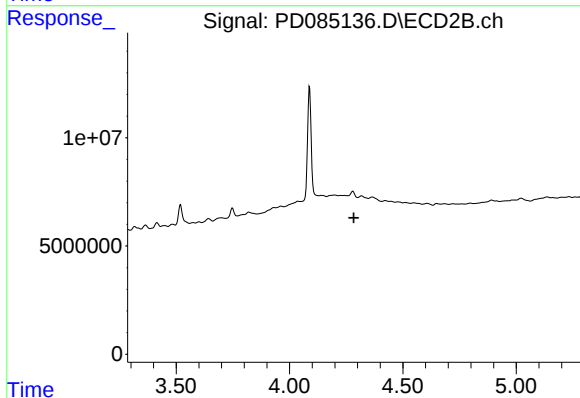


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

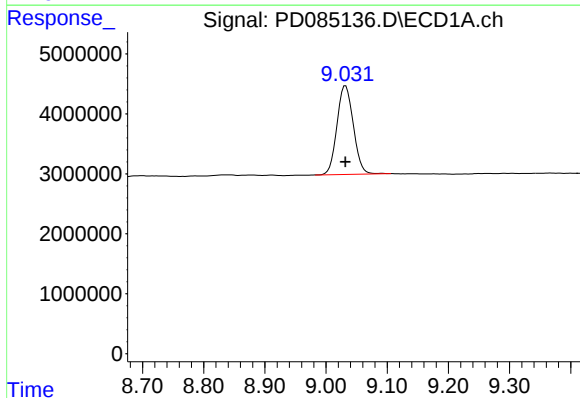

#27 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 27530264
Conc: 21.08 ng/ml

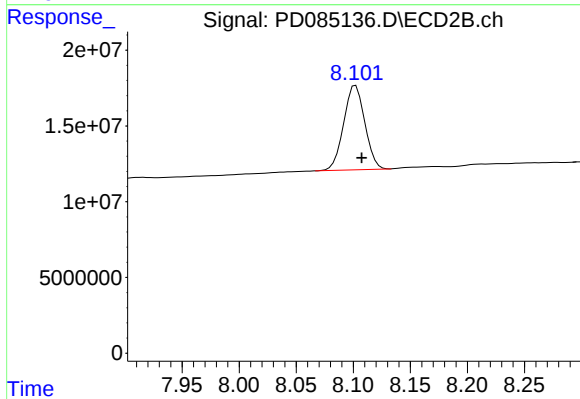

#27 Decachlorobiphenyl

R.T.: 8.102 min
Delta R.T.: -0.005 min
Response: 71817741
Conc: 20.65 ng/ml