

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 20:16
 Operator : AR\AJ
 Sample : P3899-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:11:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.913	21106751	94410655	20.869	26.679 #
27)	SA Decachlor...	9.032	8.102	14098574	32967417	10.795	9.481
Target Compounds							
3)	MA gamma-BHC...	4.268f	0.000	284.0E6	0	175.553	N.D. #
4)	MA Heptachlor	0.000	4.088	0	83075245	N.D.	19.515
6)	B beta-BHC	0.000	4.088f	0	83075245	N.D.	38.320
7)	B delta-BHC	4.762	0.000	36968933	0	22.542	N.D. #
19)	B Endosulfa...	0.000	6.451f	0	152766	N.D.	<MDL
20)	A Methoxychlor	7.473	0.000	4623393	0	8.876	N.D. #
26)	Toxaphene-5	0.000	7.399f	0	19234238	N.D.	467.597


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 20:16
Operator : AR\AJ
Sample : P3899-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:11:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

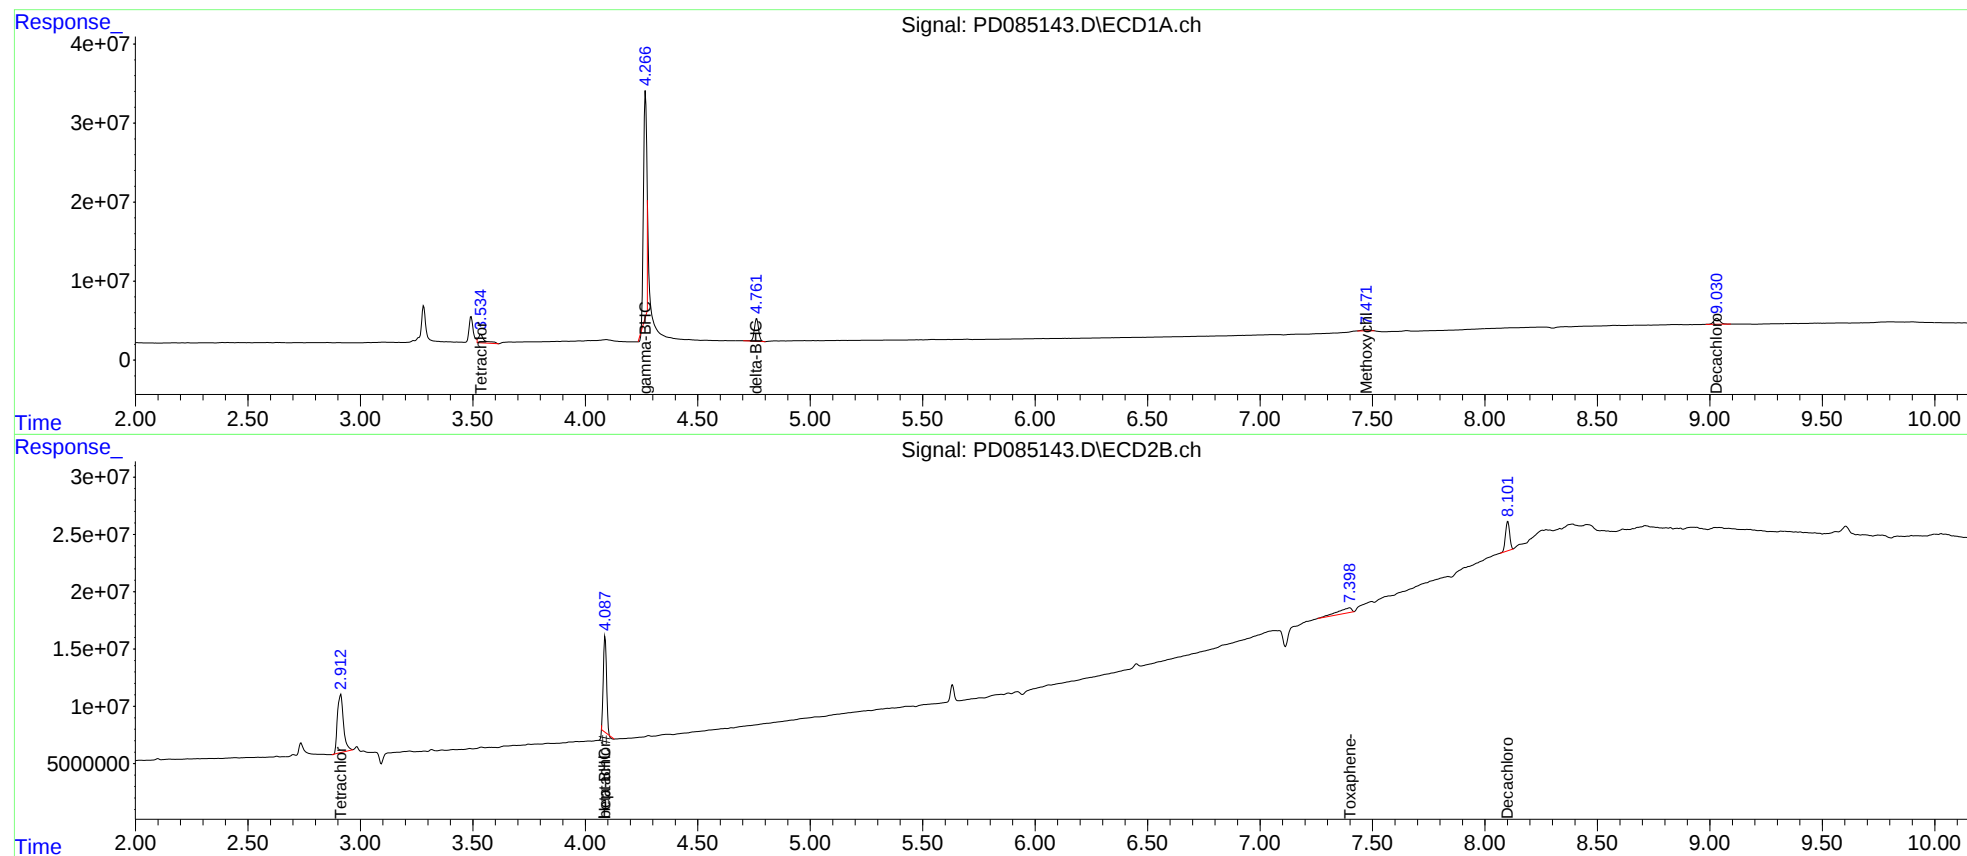

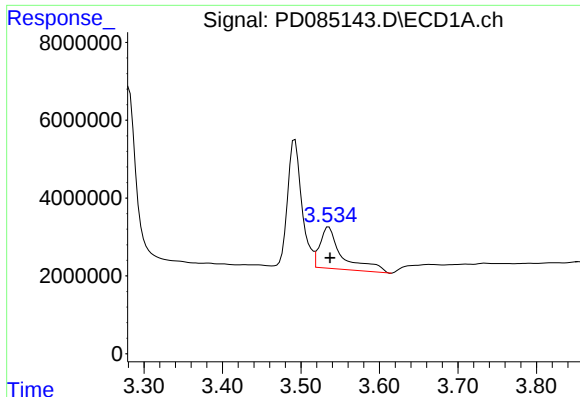


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 21106751
Conc: 20.87 ng/ml

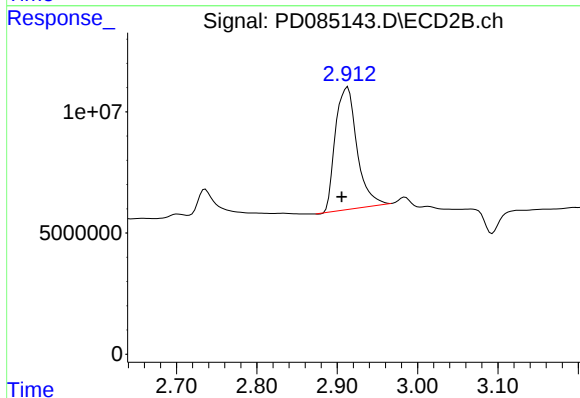


#1 Tetrachloro-m-xylene

R.T.: 2.913 min
Delta R.T.: 0.007 min
Response: 94410655
Conc: 26.68 ng/ml

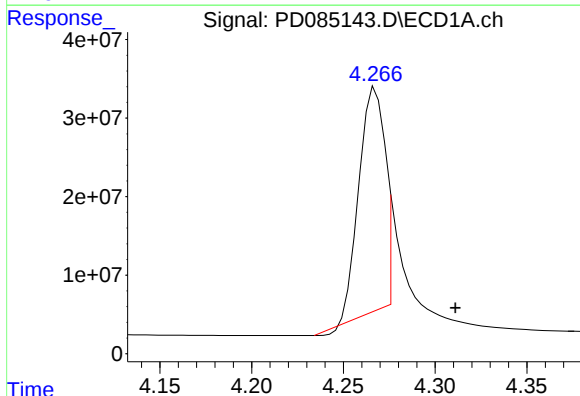


#3 gamma-BHC (Lindane)

R.T.: 4.268 min
Delta R.T.: -0.043 min
Response: 284019018
Conc: 175.55 ng/ml

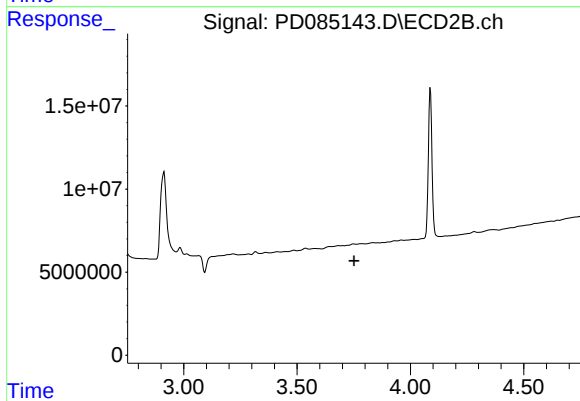


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.752 min
Response: 0
Conc: N.D.

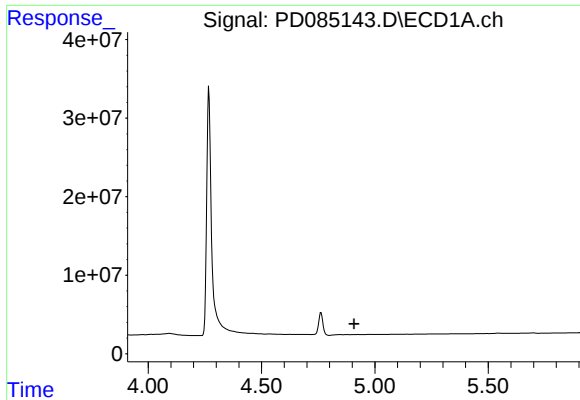


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

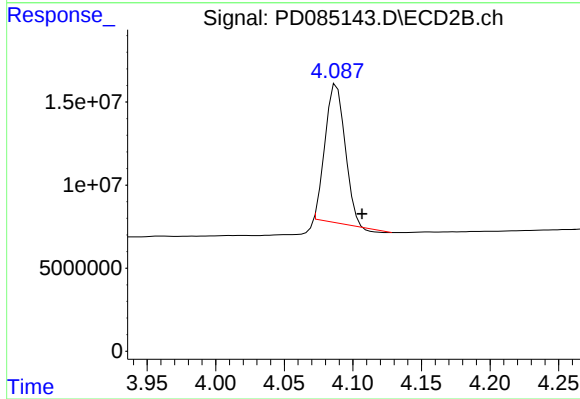


#4 Heptachlor

R.T.: 4.088 min
Delta R.T.: -0.019 min
Response: 83075245
Conc: 19.51 ng/ml

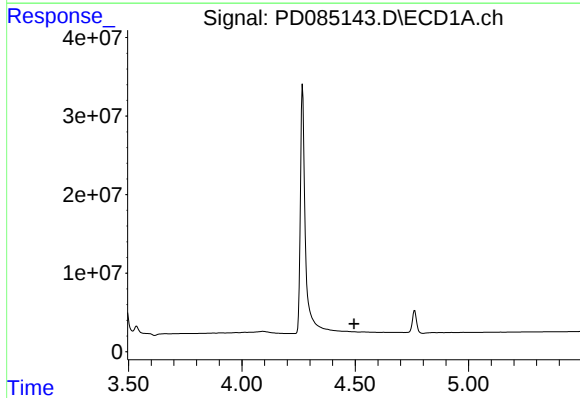


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.495 min
Response: 0
Conc: N.D.

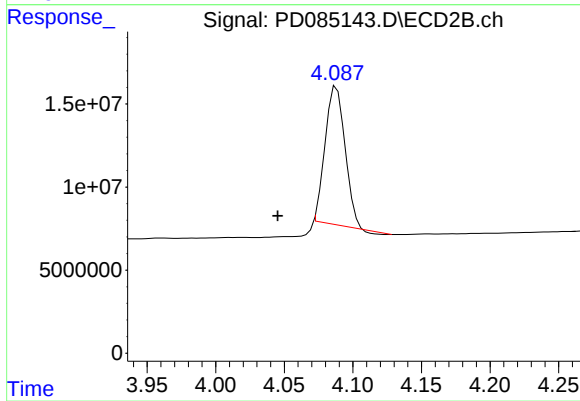


#6 beta-BHC

R.T.: 4.088 min
Delta R.T.: 0.043 min
Response: 83075245
Conc: 38.32 ng/ml

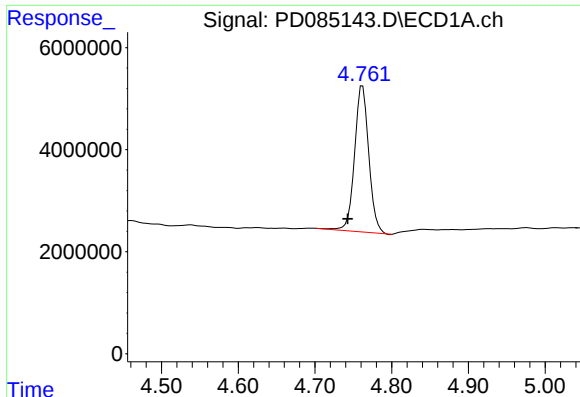


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: 0.020 min
Response: 36968933
Conc: 22.54 ng/ml

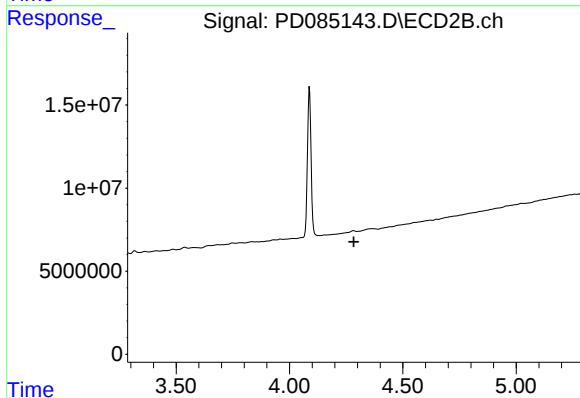


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

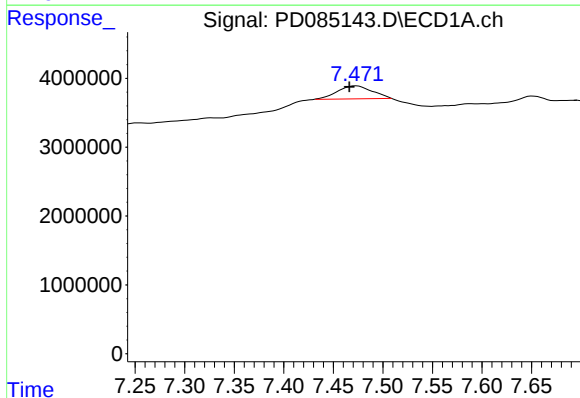


#20 Methoxychlor

R.T.: 7.473 min
Delta R.T.: 0.006 min
Response: 4623393
Conc: 8.88 ng/ml

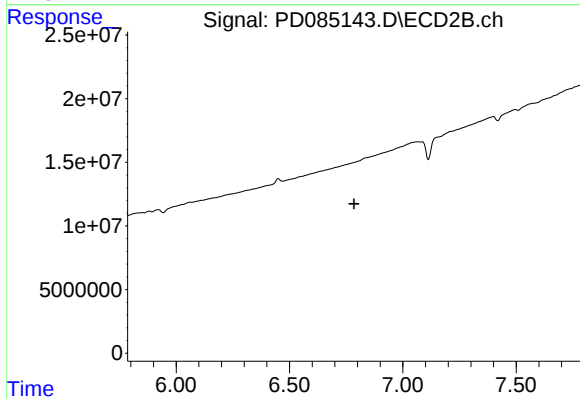


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

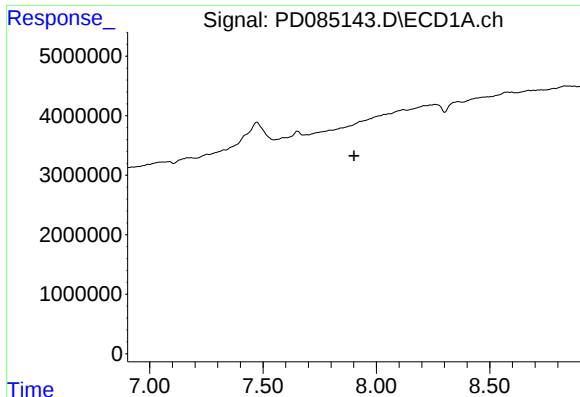


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.902 min
Response: 0
Conc: N.D.

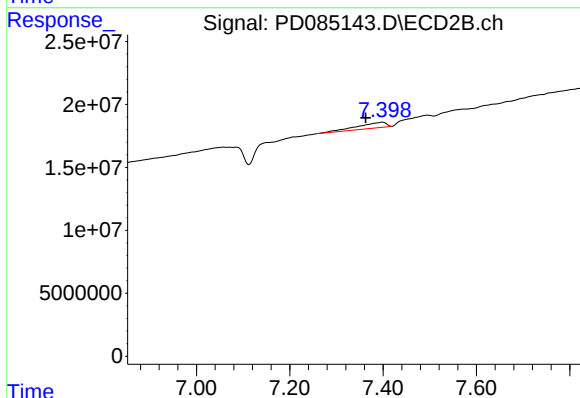


#26 Toxaphene-5

R.T.: 7.399 min
Delta R.T.: 0.036 min
Response: 19234238
Conc: 467.60 ng/ml

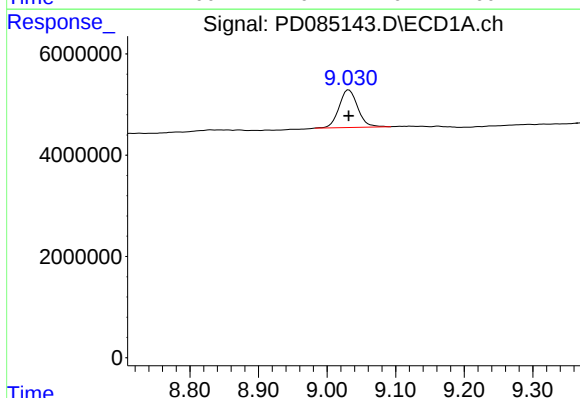

#27 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 14098574
Conc: 10.79 ng/ml

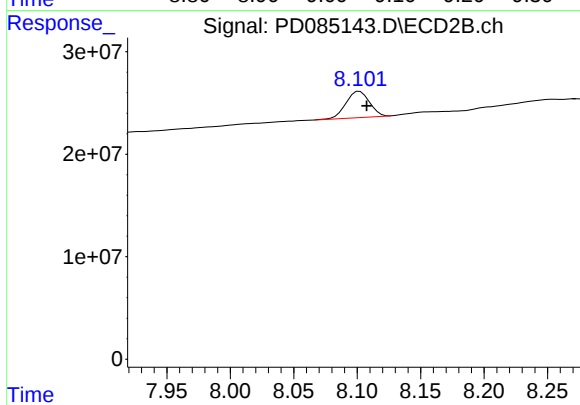

#27 Decachlorobiphenyl

R.T.: 8.102 min
Delta R.T.: -0.006 min
Response: 32967417
Conc: 9.48 ng/ml