

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2024 01:37
 Operator : AR\AJ
 Sample : P3900-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:17:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.903	18952873	65004479	18.739	18.369
27)	SA Decachlor...	9.031	8.101	25095927	67366056	19.215	19.374
Target Compounds							
4)	MA Heptachlor	4.896	0.000	3928768	0	2.553	N.D. #
5)	MB Aldrin	0.000	4.400	0	21922570	N.D.	4.936
7)	B delta-BHC	4.756	0.000	55116014	0	33.607	N.D. #
9)	A Endosulfan I	0.000	5.220f	0	4629027	N.D.	1.208
10)	B trans-Chl...	5.906	5.220f	1867356	4629027	1.324	1.125
11)	B cis-Chlor...	0.000	5.220	0	4629027	N.D.	1.103
22)	Toxaphene-1	0.000	5.220f	0	4629027	N.D.	182.578


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2024 01:37
Operator : AR\AJ
Sample : P3900-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:17:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

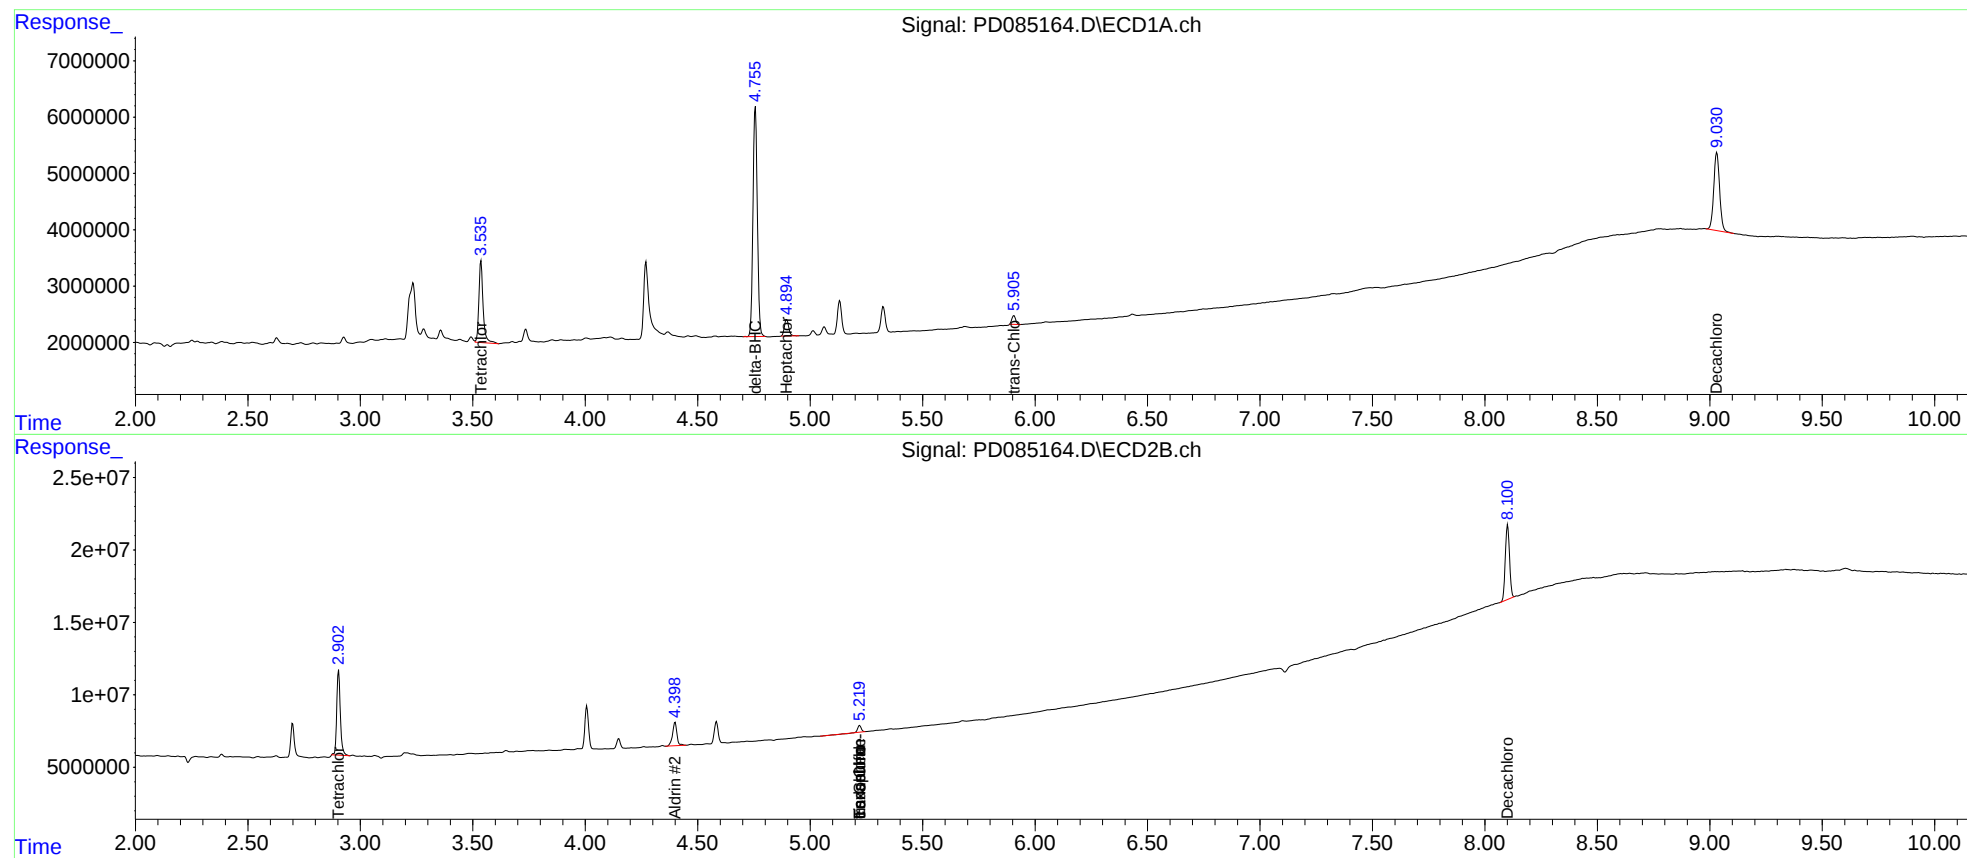

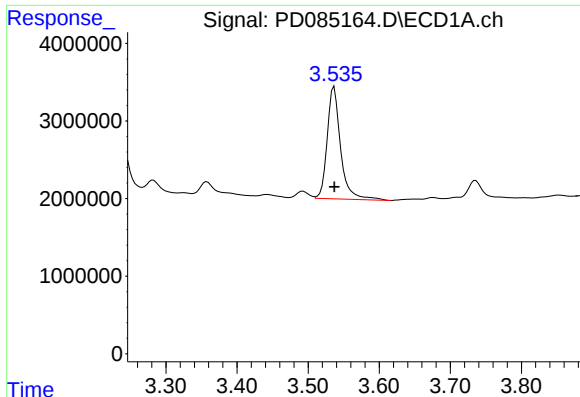


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 18952873
Conc: 18.74 ng/ml

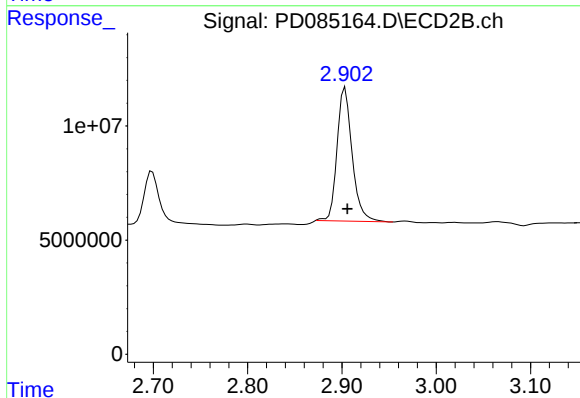


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.002 min
Response: 65004479
Conc: 18.37 ng/ml

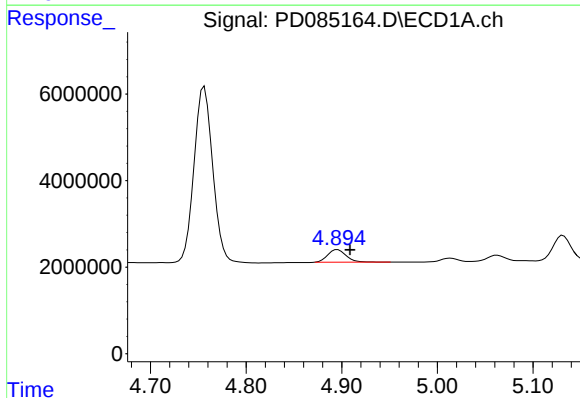


#4 Heptachlor

R.T.: 4.896 min
Delta R.T.: -0.013 min
Response: 3928768
Conc: 2.55 ng/ml

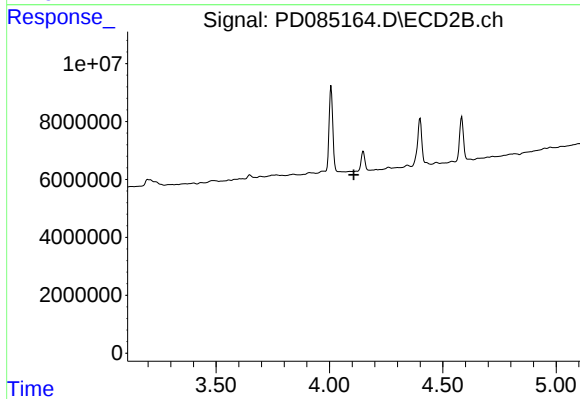


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.107 min
Response: 0
Conc: N.D.

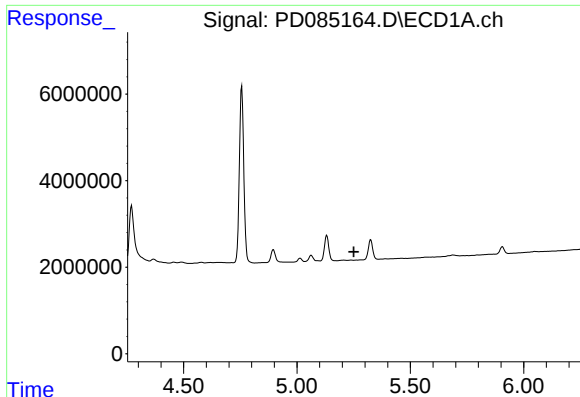


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.250 min
Response: 0
Conc: N.D.

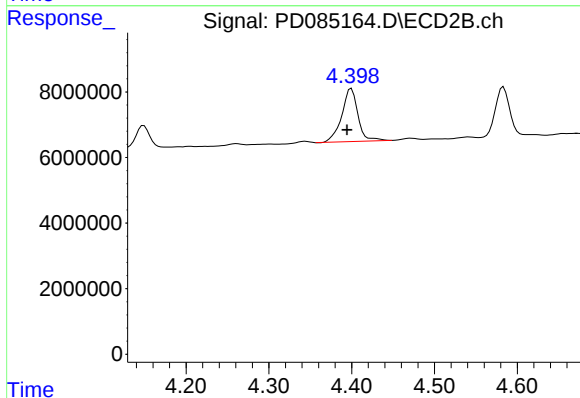


#5 Aldrin

R.T.: 4.400 min
Delta R.T.: 0.005 min
Response: 21922570
Conc: 4.94 ng/ml

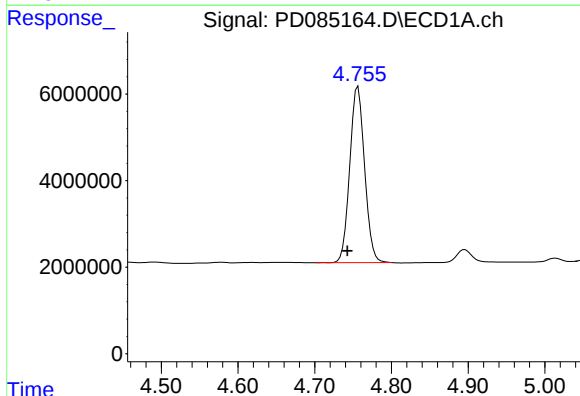


#7 delta-BHC

R.T.: 4.756 min
Delta R.T.: 0.014 min
Response: 55116014
Conc: 33.61 ng/ml

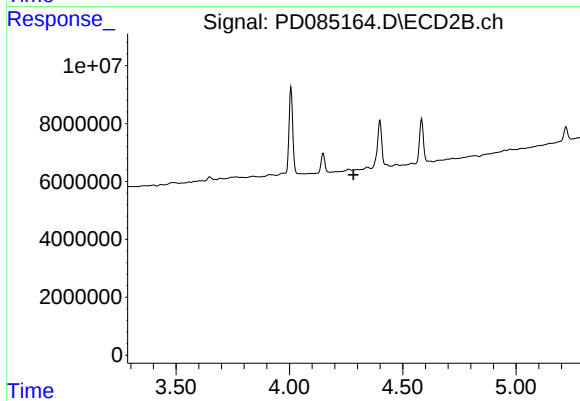


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

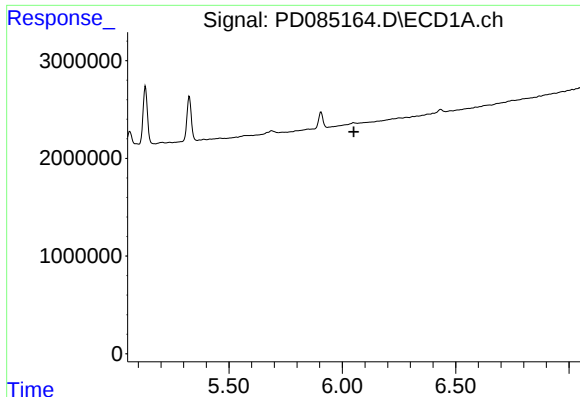


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

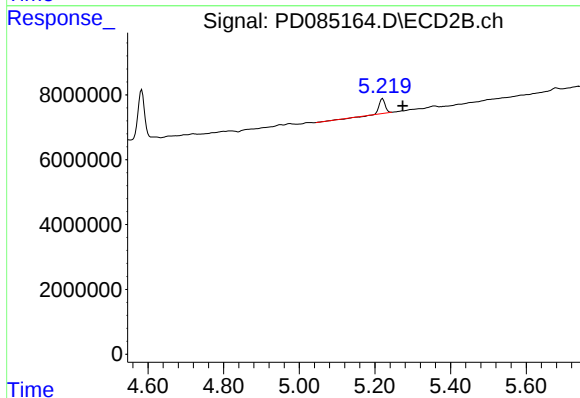


#9 Endosulfan I

R.T.: 5.220 min
Delta R.T.: -0.053 min
Response: 4629027
Conc: 1.21 ng/ml

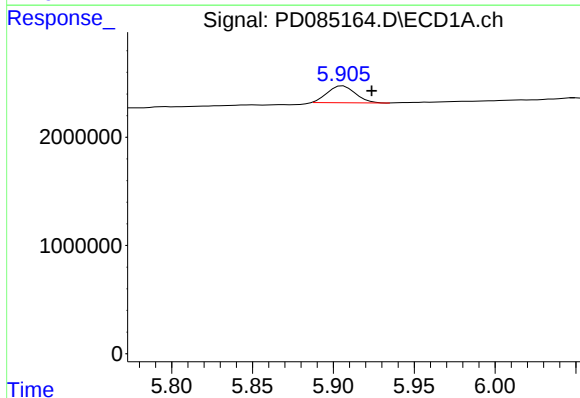


#10 trans-Chlordane

R.T.: 5.906 min
Delta R.T.: -0.018 min
Response: 1867356
Conc: 1.32 ng/ml

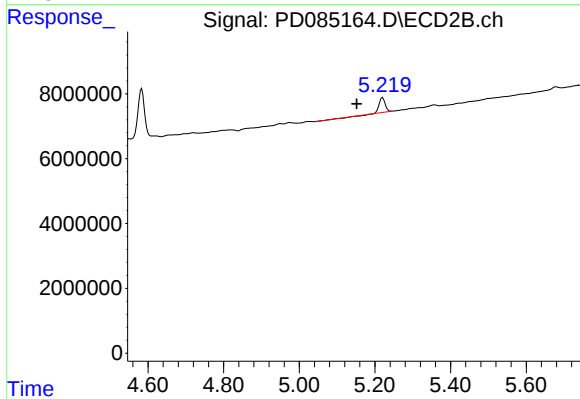


#10 trans-Chlordane

R.T.: 5.220 min
Delta R.T.: 0.068 min
Response: 4629027
Conc: 1.13 ng/ml

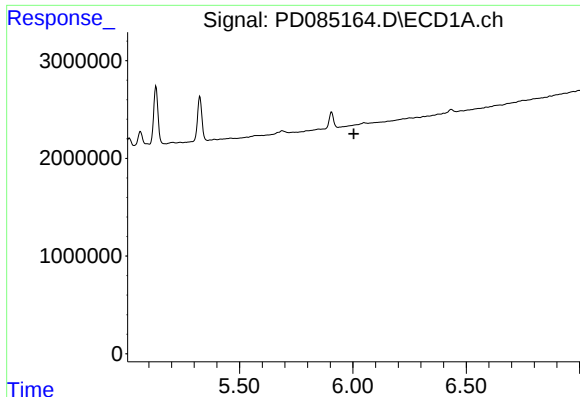


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.

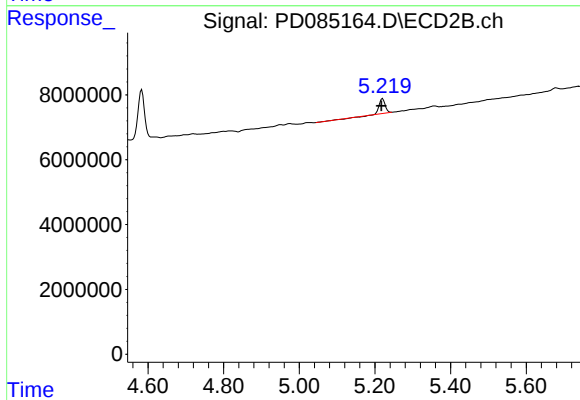


#11 cis-Chlordane

R.T.: 5.220 min
Delta R.T.: 0.003 min
Response: 4629027
Conc: 1.10 ng/ml

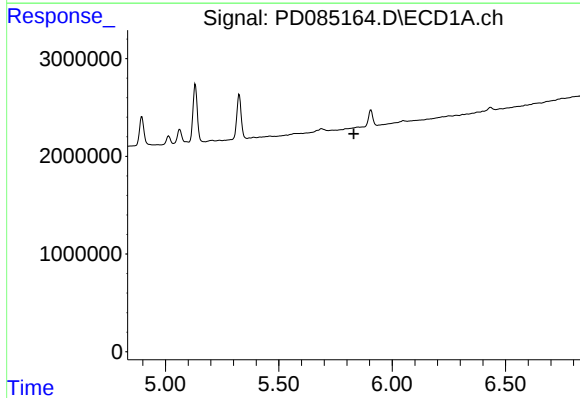


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.831 min
Response: 0
Conc: N.D.

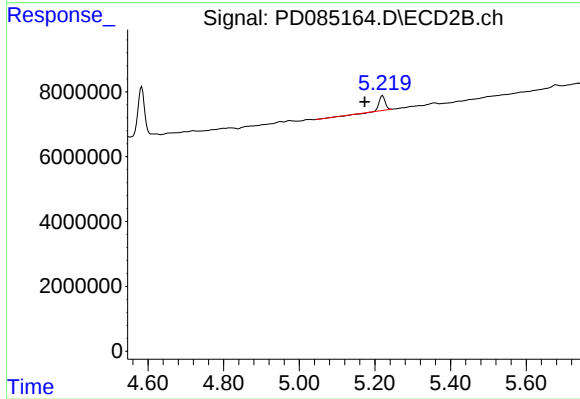


#22 Toxaphene-1

R.T.: 5.220 min
Delta R.T.: 0.047 min
Response: 4629027
Conc: 182.58 ng/ml

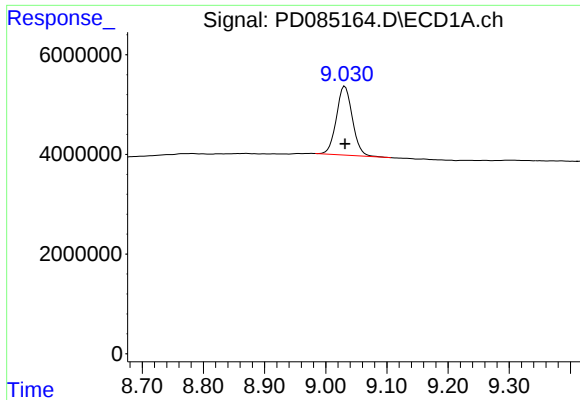

#27 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.000 min
Response: 25095927
Conc: 19.22 ng/ml

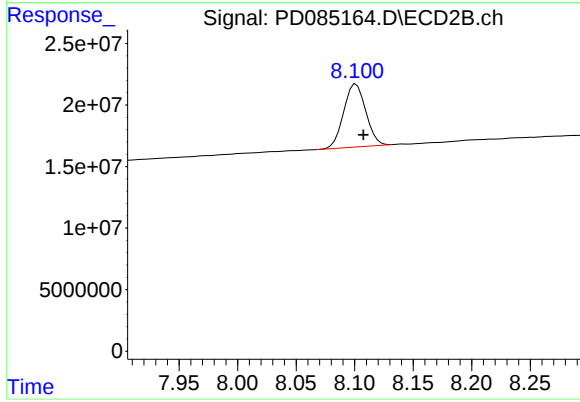

#27 Decachlorobiphenyl

R.T.: 8.101 min
Delta R.T.: -0.006 min
Response: 67366056
Conc: 19.37 ng/ml