

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 19:23
 Operator : AR\AJ
 Sample : P3899-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC00

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/18/2024
 Supervised By : Ankita Jodhani 09/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:10:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.915	141.0E6	18215.3E6	139.429m	5147.301 #
2)	SA Decachlor...	9.032	8.101	18200360	46939545	13.936	13.499
Target Compounds							
2)	A alpha-BHC	3.982	3.413	64655390	132.0E6	38.029	26.026 #
7)	B delta-BHC	4.740	4.279	87797101	218.8E6	53.535m	44.084
9)	A Endosulfan I	6.052	5.278	20666536	38293442	15.021m	9.990 #
16)	A 4,4'-DDD	6.682	5.953	14060802	25264709	14.241	7.445 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 19:23
Operator : AR\AJ
Sample : P3899-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:10:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

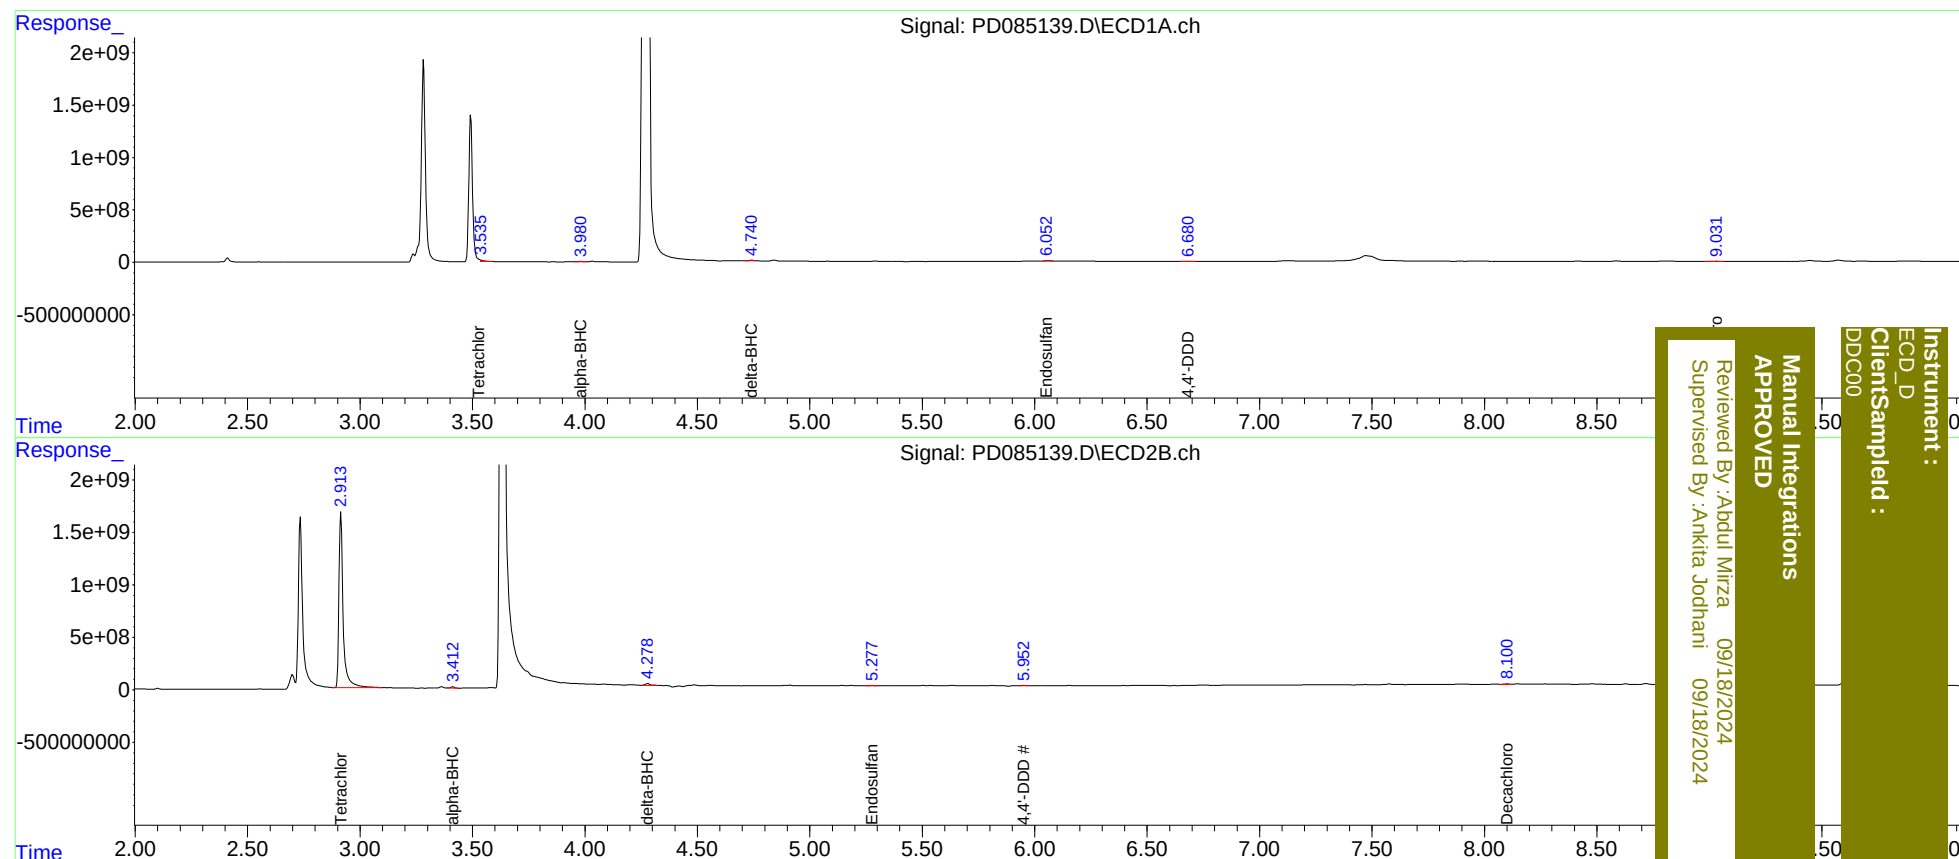

Instrument :
ECD_D
ClientSampled :
DDC00

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/18/2024
Supervised By : Ankita Jodhani 09/18/2024