

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 15:31
 Operator : AR\AJ
 Sample : P3993-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COUF3MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/16/2024
 Supervised By :Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:06:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.903	11476862	45997868	11.347m	12.998
27)	SA Decachlor...	9.053	8.103	13876535	36502526	10.625	10.498
Target Compounds							
2)	A alpha-BHC	4.001	3.414	74192563	224.3E6	43.639m	44.241
3)	MA gamma-BHC...	4.330	3.749	74655066	215.5E6	46.144m	44.478
4)	MA Heptachlor	4.928	4.103	66871496	205.9E6	43.463m	48.367
5)	MB Aldrin	5.270	4.390	67356886	193.7E6	42.115	43.605
6)	B beta-BHC	4.514	4.043	27998721	88381273	38.546	40.767
7)	B delta-BHC	4.760	4.280	75688827	213.8E6	46.152m	43.061
8)	B Heptachlo...	5.687	4.894	60009849	177.2E6	40.235m	41.838
9)	A Endosulfan I	6.069	5.270	56050875	168.0E6	40.741m	43.836
10)	B trans-Chl...	5.941	5.146	58743626	182.8E6	41.651m	44.434m
11)	B cis-Chlor...	6.022	5.212	59987062	180.9E6	40.571m	43.120
12)	B 4,4'-DDE	6.192	5.397	111.6E6	347.8E6	89.431	88.657
13)	MA Dieldrin	6.342	5.535	125.2E6	371.7E6	84.844m	86.509m
14)	MA Endrin	6.570	5.814	108.5E6	352.4E6	96.136	95.187
15)	B Endosulfa...	6.780	6.106	105.9E6	319.6E6	80.246m	86.186
16)	A 4,4'-DDD	6.700	5.953	85459163	274.6E6	86.554m	80.917
17)	MA 4,4'-DDT	7.015	6.209	87533090	303.8E6	97.788m	94.981
18)	B Endrin al...	6.908	6.285	79587924	247.2E6	88.127m	86.594
19)	B Endosulfa...	7.144	6.509	98634731	308.0E6	85.620	86.251
20)	A Methoxychlor	7.485	6.781	245.7E6	736.4E6	471.712m	445.165
21)	B Endrin ke...	7.622	7.020	108.0E6	361.8E6	88.372m	82.178

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 15:31
Operator : AR\AJ
Sample : P3993-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:06:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

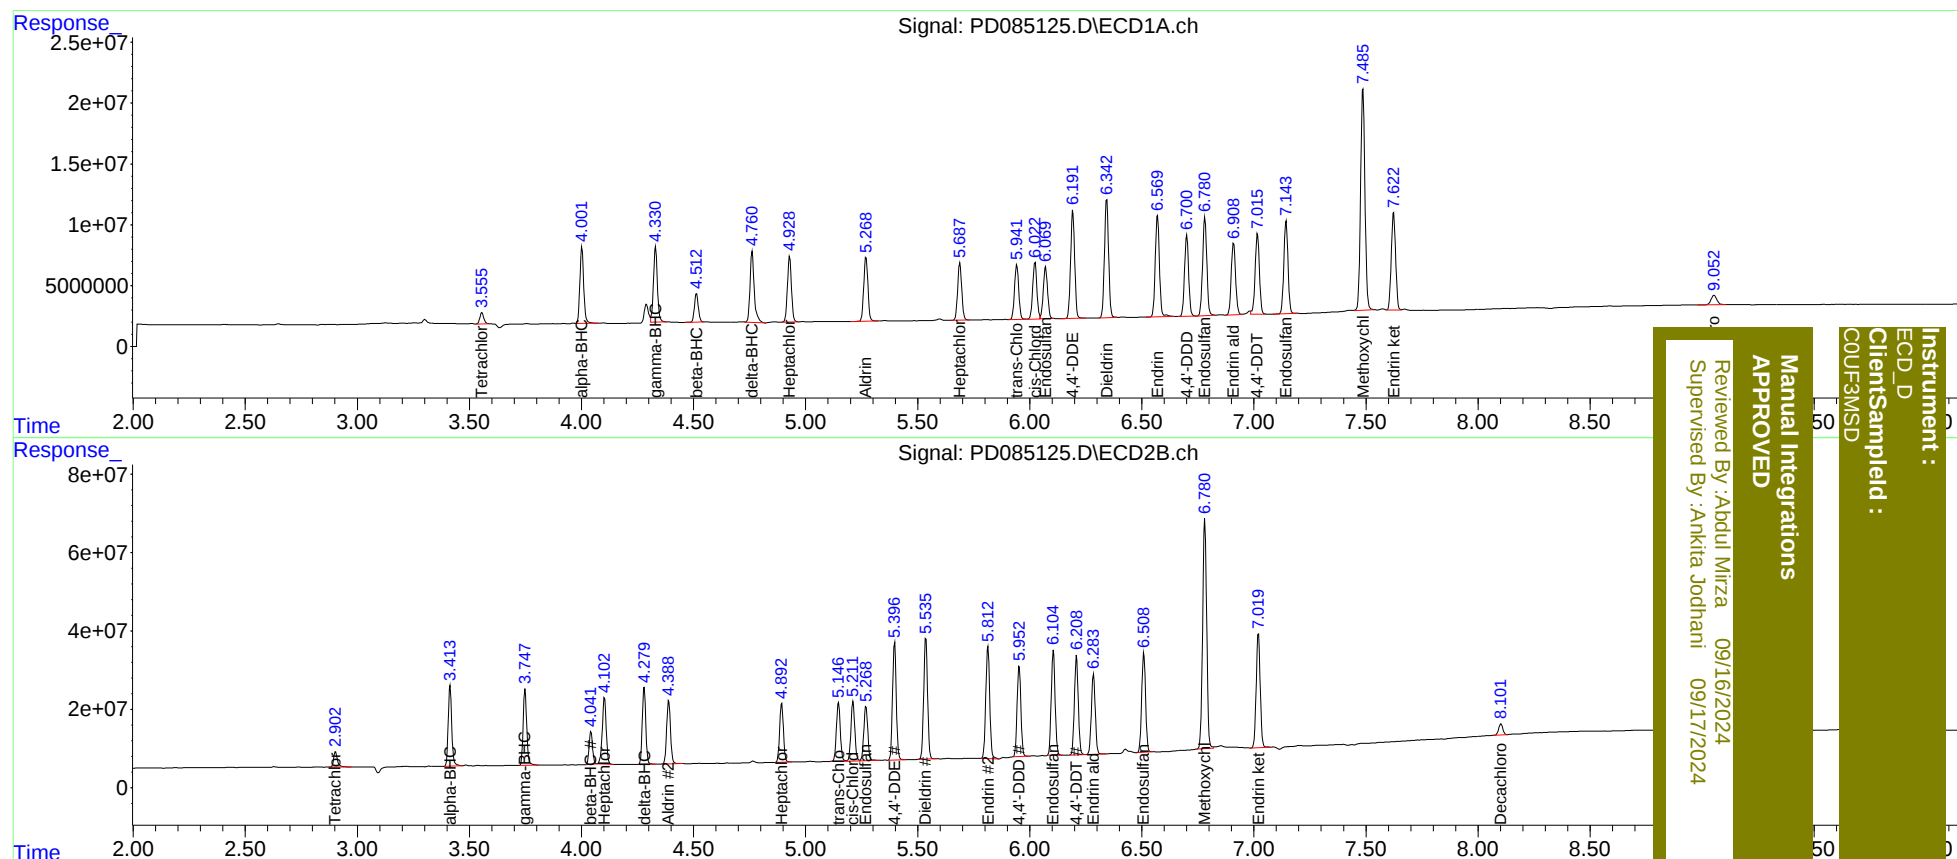

Instrument :
ECD_D
Client Sampled :
COU-F3MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 09/16/2024
Supervised By: Ankita Jodhani 09/17/2024