

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
 Data File : PD085168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2024 02:31
 Operator : AR\AJ
 Sample : P3922-03MSD
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN7MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/18/2024
 Supervised By :Ankita Jodhani 09/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:18:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.904	11379221	42612025	11.251	12.041
2) SA Decachlor...	9.032	8.100	17274536	45238777	13.227	13.010m
Target Compounds						
2) A alpha-BHC	3.983	3.414	53124917	168.8E6	31.247	33.286
3) MA gamma-BHC...	4.310	3.749	56350421	169.1E6	34.830m	34.892
4) MA Heptachlor	4.909	4.103	51935250	147.1E6	33.755	34.562
5) MB Aldrin	5.249	4.390	49416259	131.0E6	30.898	29.502
6) B beta-BHC	4.494	4.042	22085863	68770934	30.406	31.722
7) B delta-BHC	4.740	4.281	45018935	164.2E6	27.450m	33.074
8) B Heptachlo...	5.668	4.893	44129572	154.4E6	29.588	36.456
9) A Endosulfan I	6.049	5.269	42745342	138.5E6	31.069m	36.138
10) B trans-Chl...	5.922	5.145	42803337	135.3E6	30.349	32.896m
11) B cis-Chlor...	6.002	5.212	45511540	142.2E6	30.781m	33.897
12) B 4,4'-DDE	6.172	5.395	83591274	271.4E6	67.010	69.177m
13) MA Dieldrin	6.323	5.536	94346222	280.4E6	63.959	65.264
14) MA Endrin	6.550	5.814	83169296	267.4E6	73.709	72.231
15) B Endosulfa...	6.761	6.106	80329551	245.6E6	60.854	66.235
16) A 4,4'-DDD	6.679	5.952	70507094	277.7E6	71.410m	81.839m
17) MA 4,4'-DDT	6.994	6.209	84276575	217.6E6	94.150m	68.038 #
18) B Endrin al...	6.890	6.280	56325112	683.4E6	62.368	239.342m#
19) B Endosulfa...	7.123	6.509	77181332	237.7E6	66.997	66.546
20) A Methoxychlor	7.467	6.781	190.5E6	573.8E6	365.775	346.862
21) B Endrin ke...	7.603	7.020	81980949	279.3E6	67.052	63.439

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091424\
Data File : PD085168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2024 02:31
Operator : AR\AJ
Sample : P3922-03MSD
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:18:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

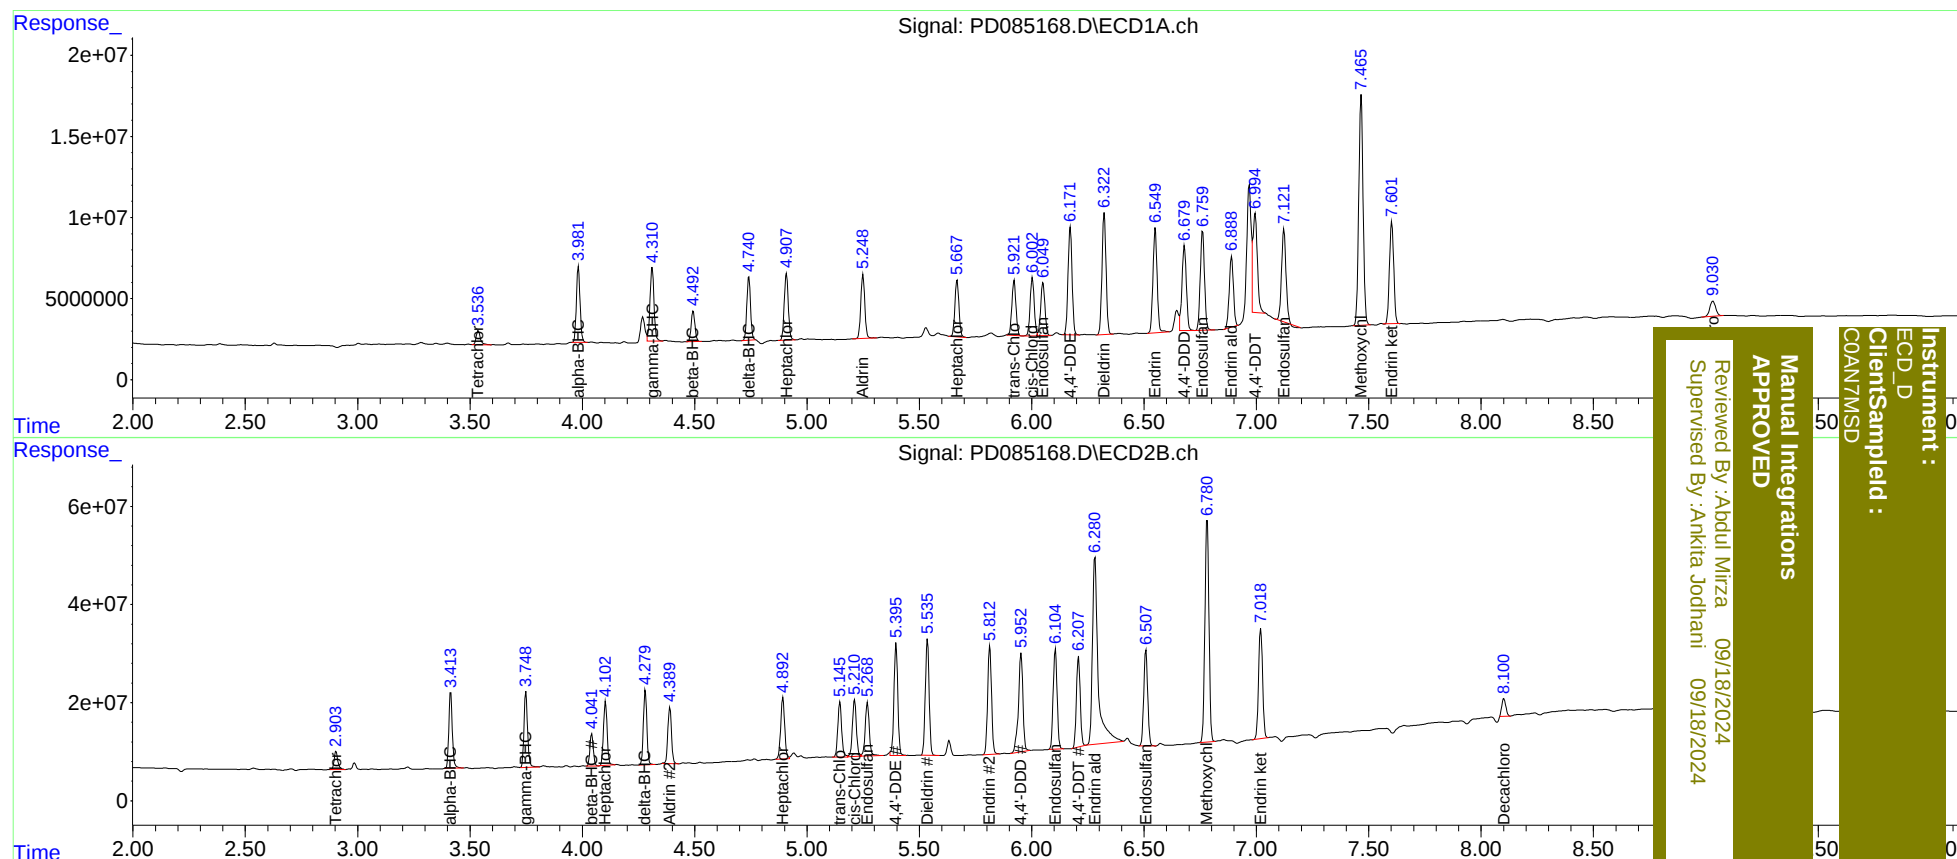

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 09/18/2024
Supervised By: Ankita Jodhani 09/18/2024

Instrument :
ECD_D
Client Sampled :
COANTMSD