

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 10:44
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:51:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 01:50:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.014	100.4E6	652.3E6	99.854	94.184
28)	SA Decachlor...	8.236	9.086	117.9E6	358.5E6	93.610	93.756
Target Compounds							
23)	Chlordane-1	4.364	5.009	32339244	236.9E6	975.036	922.895
24)	Chlordane-2	4.864	5.479	39582836	225.1E6	924.333	915.425
25)	Chlordane-3	5.430	6.127	122.9E6	867.2E6	1016.026	961.106
26)	Chlordane-4	5.488	6.200	101.7E6	999.6E6	992.928	954.282
27)	Chlordane-5	6.325	7.010	47627347	200.9E6	973.726	958.310


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 10:44
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:51:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 01:50:44 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

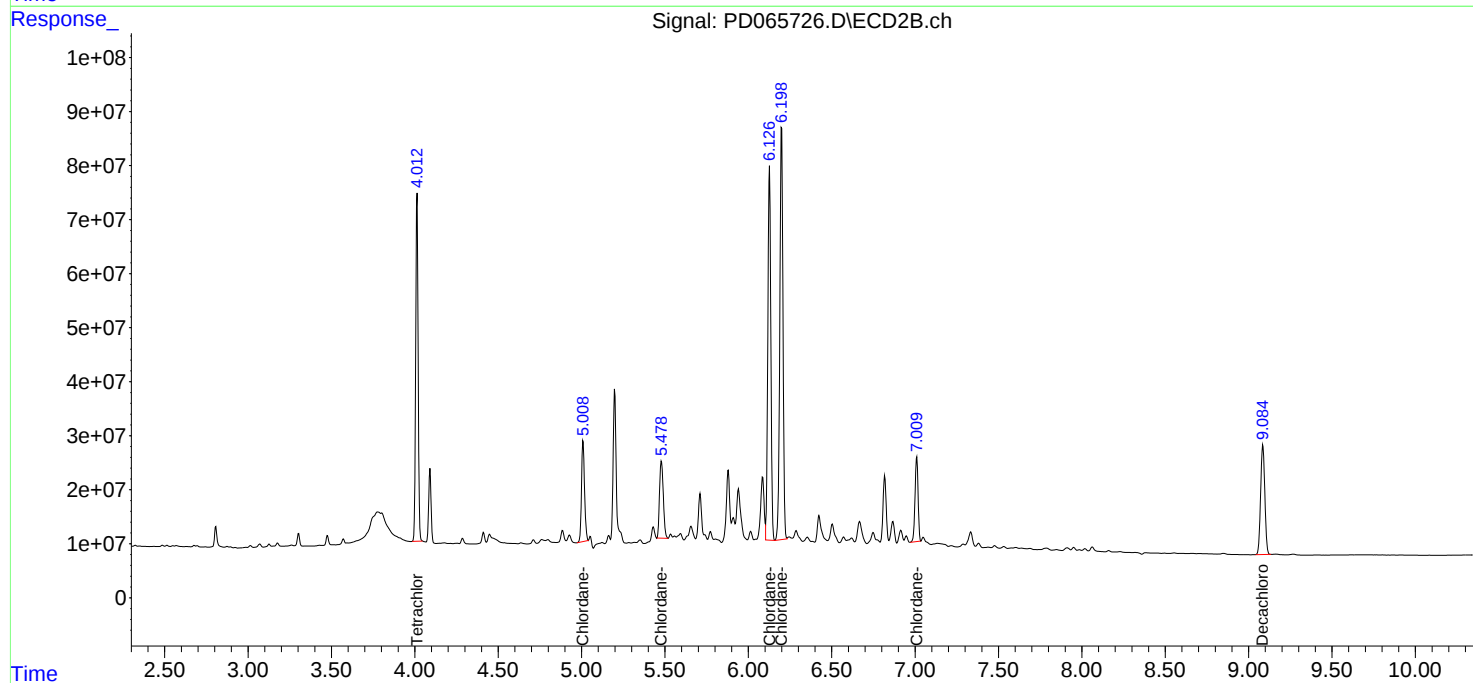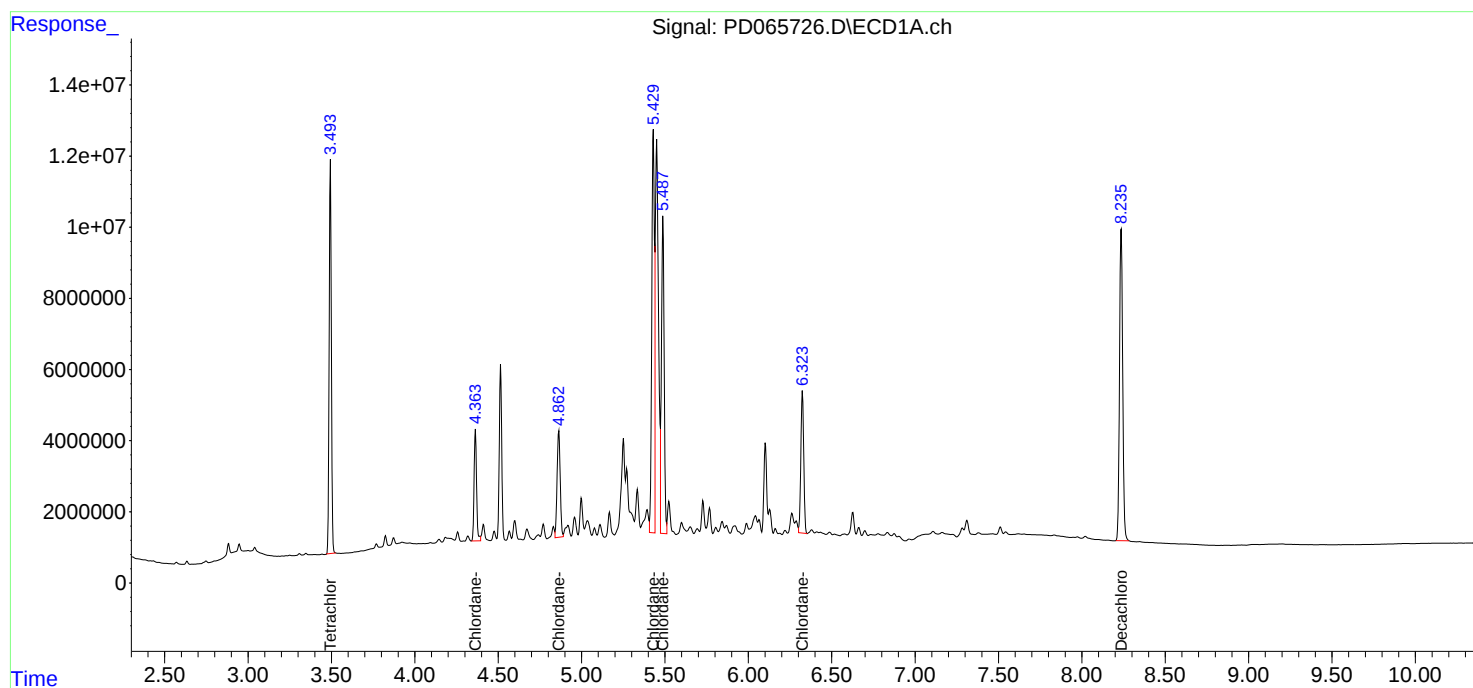

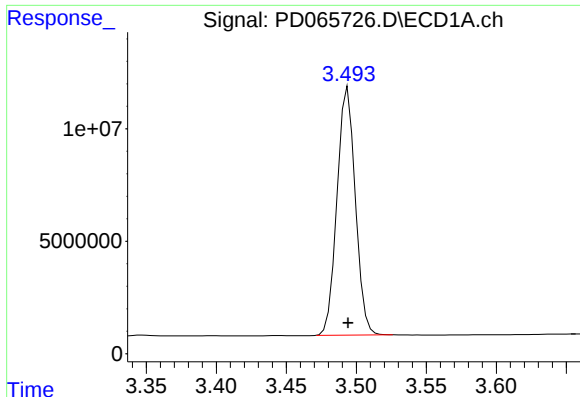


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 100424793
Conc: 99.85 ng/ml

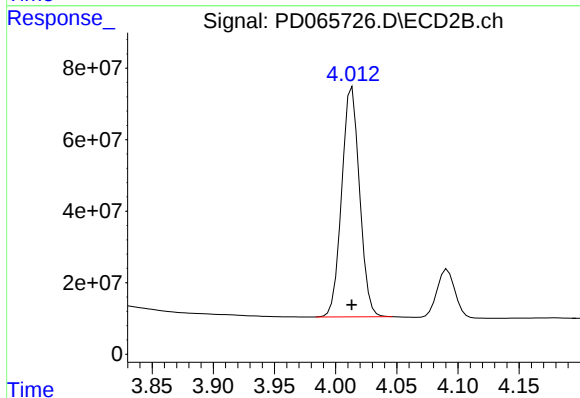


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 652305058
Conc: 94.18 ng/ml

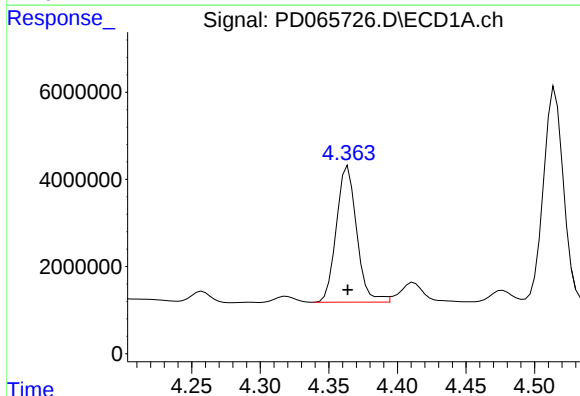


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 32339244
Conc: 975.04 ng/ml

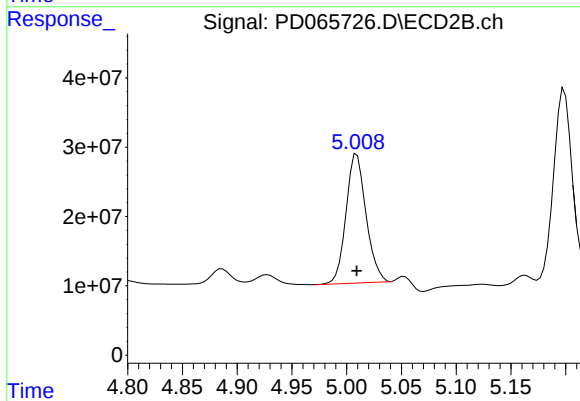


#23 Chlordane-1

R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 236854590
Conc: 922.89 ng/ml

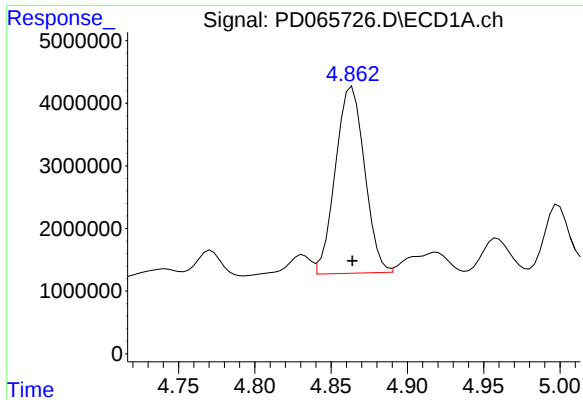


#24 Chlordane-2

R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 39582836
Conc: 924.33 ng/ml

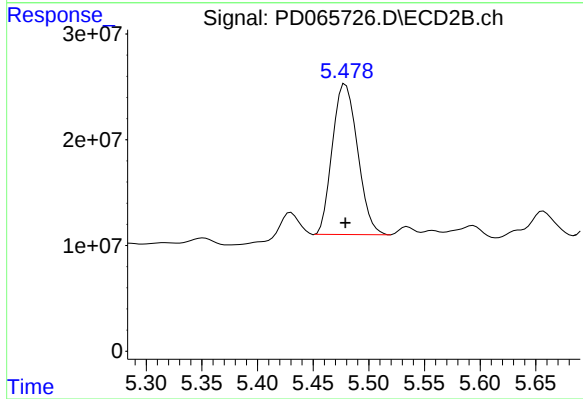


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 225133107
Conc: 915.43 ng/ml

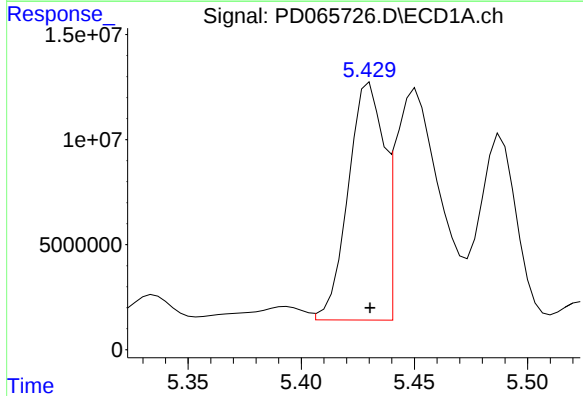


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 122931520
Conc: 1016.03 ng/ml

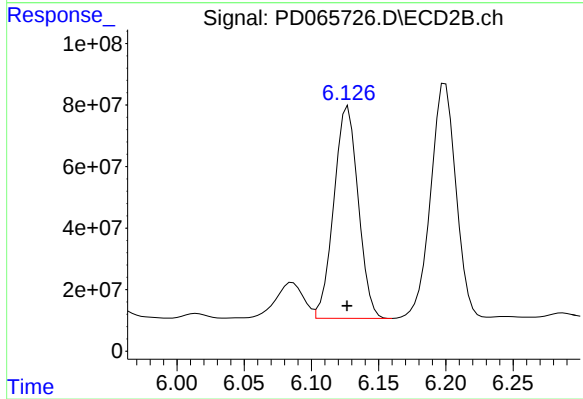


#25 Chlordane-3

R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 867198435
Conc: 961.11 ng/ml

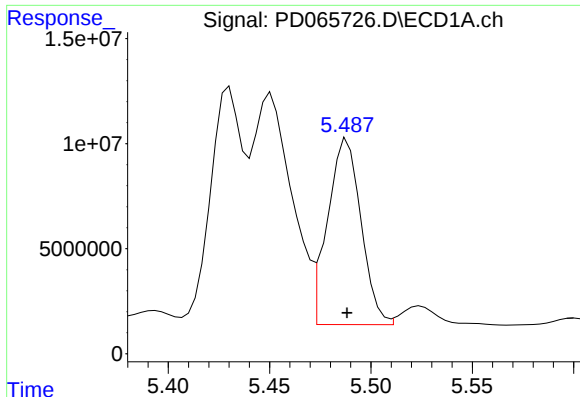


#26 Chlordane-4

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 101730339
Conc: 992.93 ng/ml

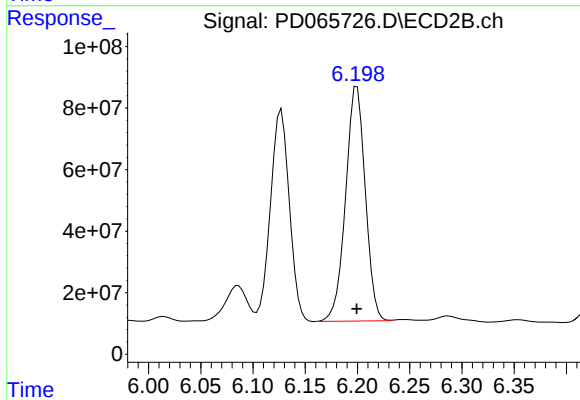


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 999631793
Conc: 954.28 ng/ml

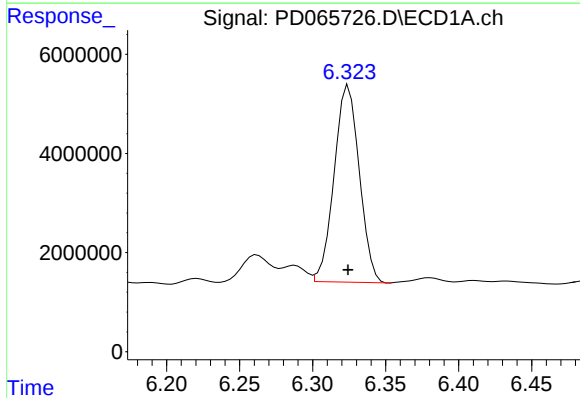


#27 Chlordane-5

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 47627347
Conc: 973.73 ng/ml

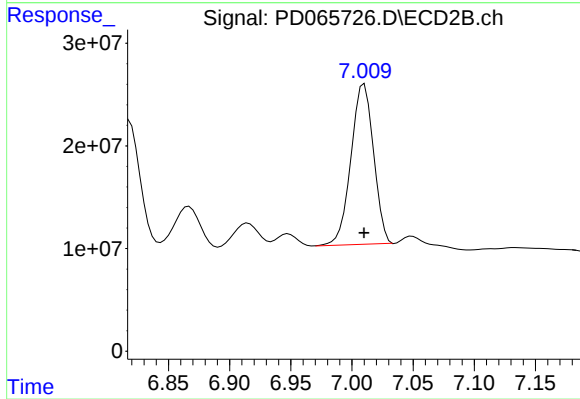


#27 Chlordane-5

R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 200886147
Conc: 958.31 ng/ml

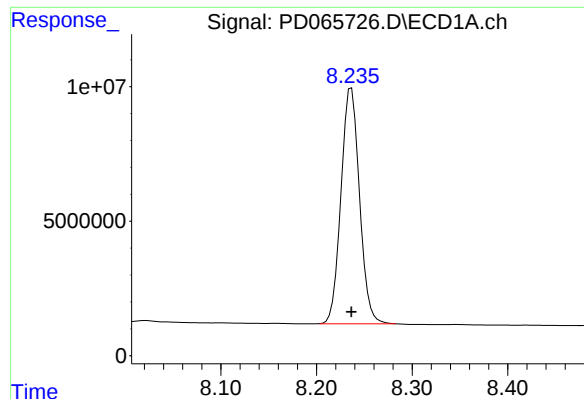

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 117901839
Conc: 93.61 ng/ml

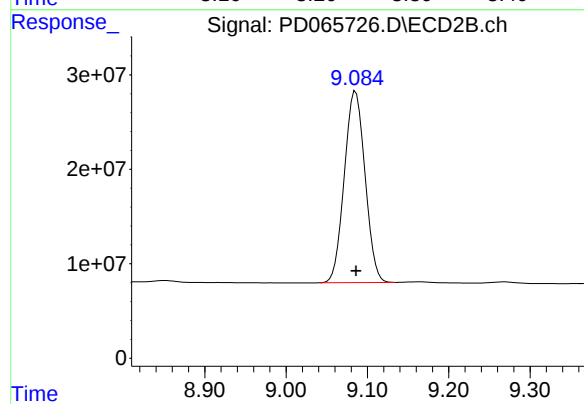

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 358457933
Conc: 93.76 ng/ml