

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 11:12
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:51:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 01:50:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	50285834	346.3E6	50.000	50.000
28)	SA Decachlor...	8.236	9.086	62974782	191.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.364	5.009	16583616	128.3E6	500.000	500.000
24)	Chlordane-2	4.864	5.479	21411575	123.0E6	500.000	500.000
25)	Chlordane-3	5.430	6.127	60496249	451.1E6	500.000	500.000
26)	Chlordane-4	5.488	6.199	51227455	523.8E6	500.000	500.000
27)	Chlordane-5	6.324	7.010	24456229	104.8E6	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 11:12
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:51:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 01:50:44 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

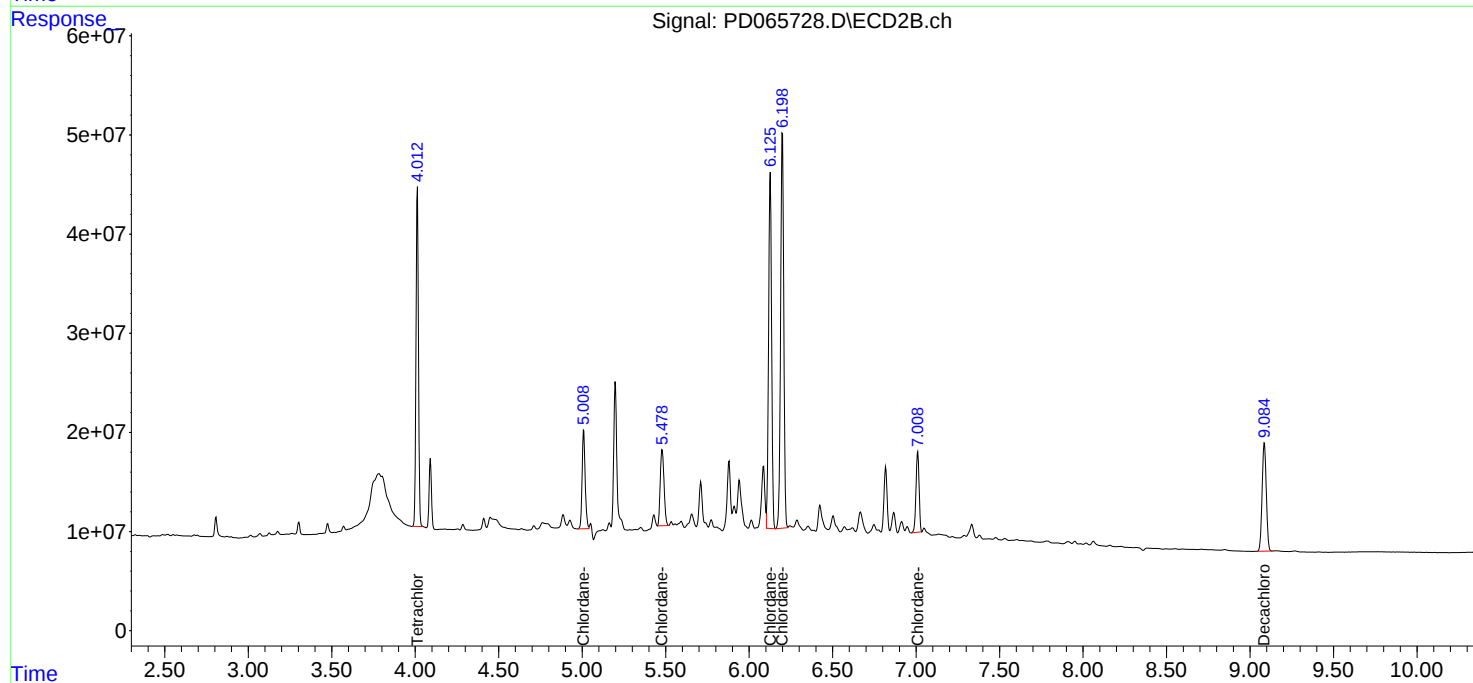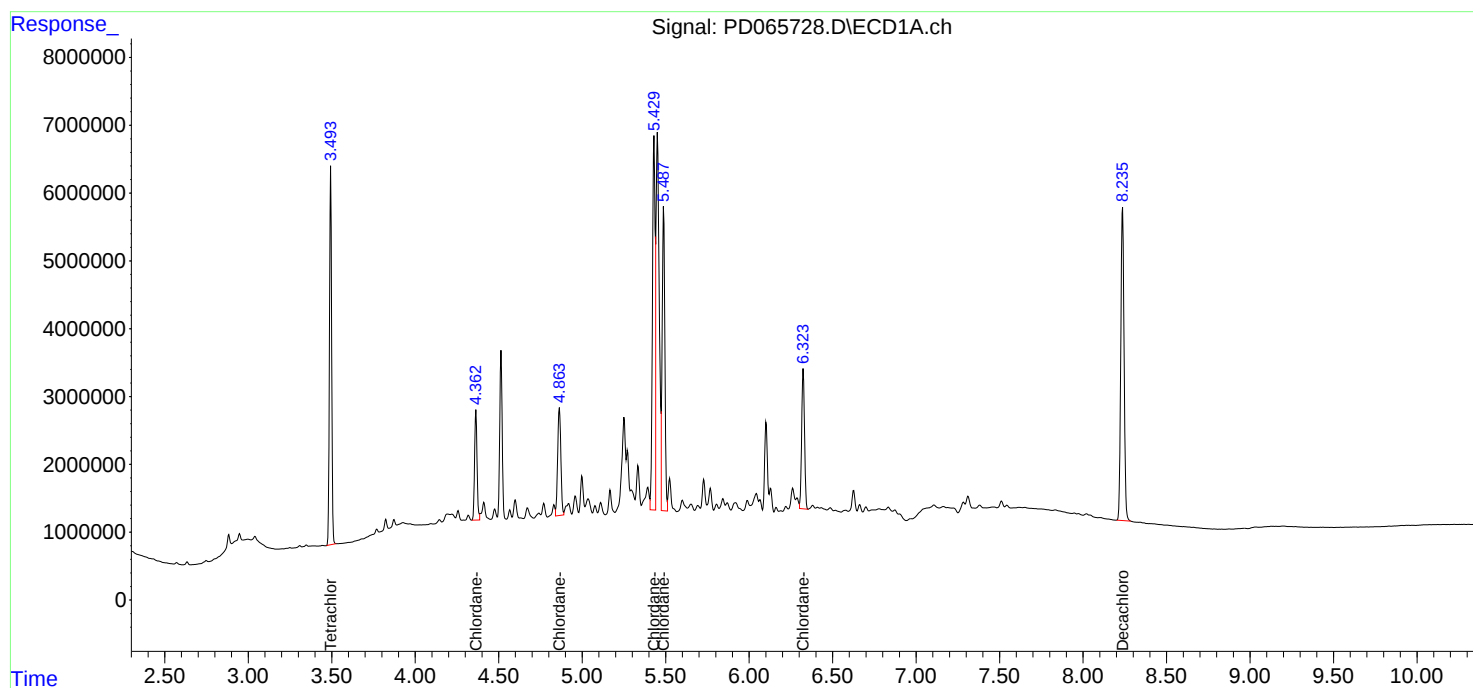

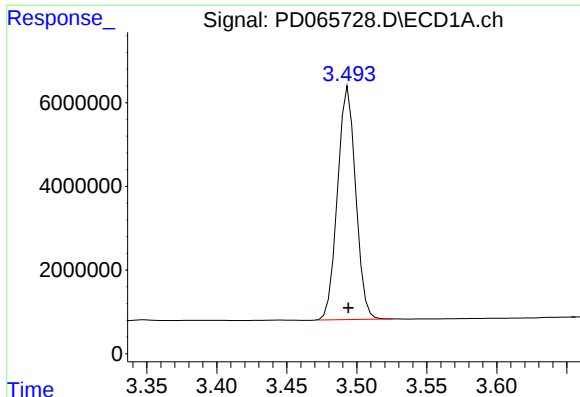


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 50285834
Conc: 50.00 ng/ml

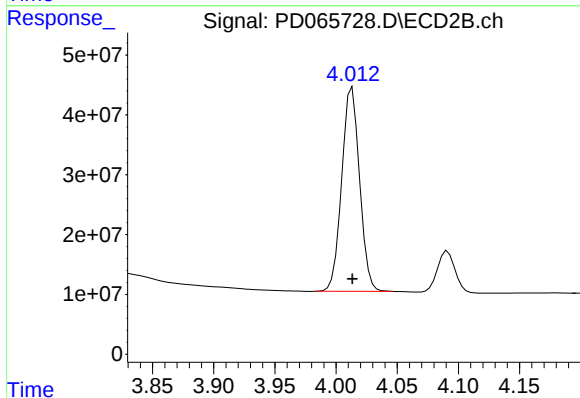


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 346292741
Conc: 50.00 ng/ml

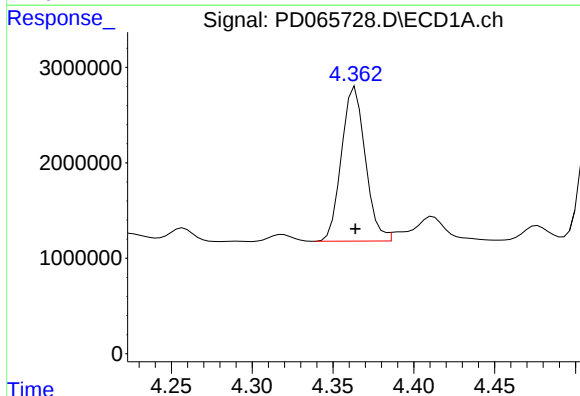


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 16583616
Conc: 500.00 ng/ml

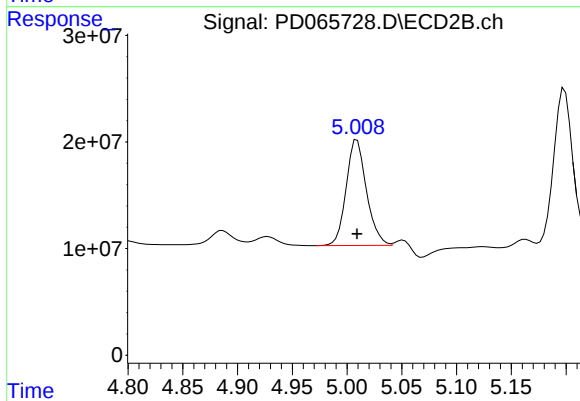


#23 Chlordane-1

R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 128321527
Conc: 500.00 ng/ml

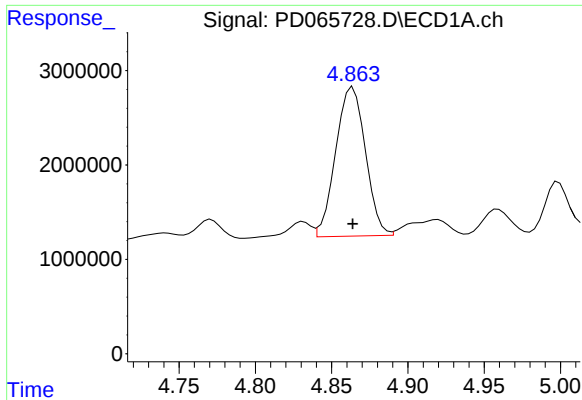


#24 Chlordane-2

R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 21411575
Conc: 500.00 ng/ml

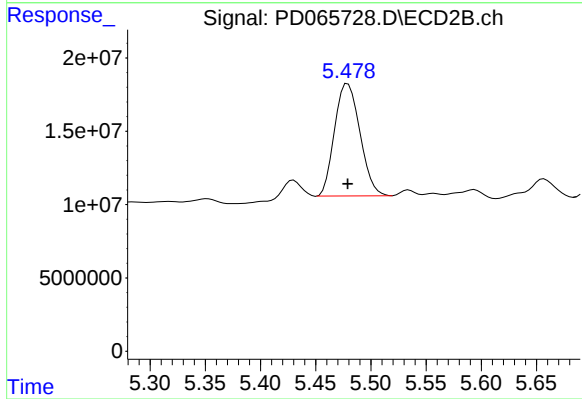


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 122966390
Conc: 500.00 ng/ml

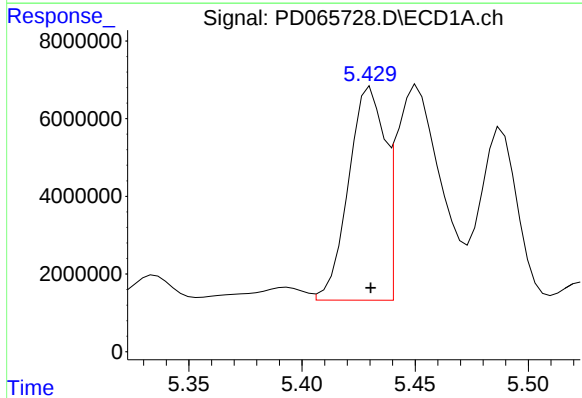


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 60496249
Conc: 500.00 ng/ml

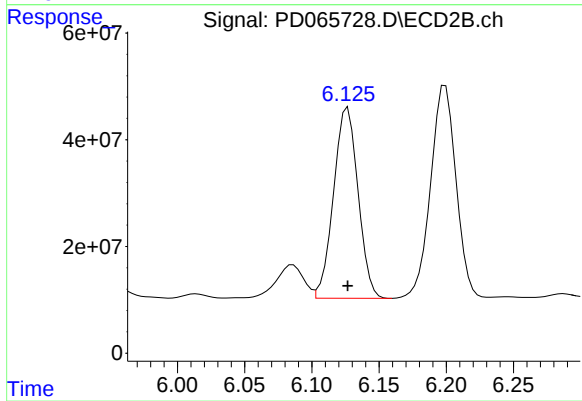


#25 Chlordane-3

R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 451145861
Conc: 500.00 ng/ml

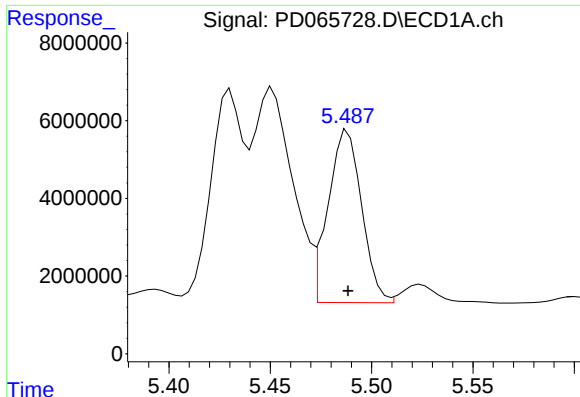


#26 Chlordane-4

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 51227455
Conc: 500.00 ng/ml

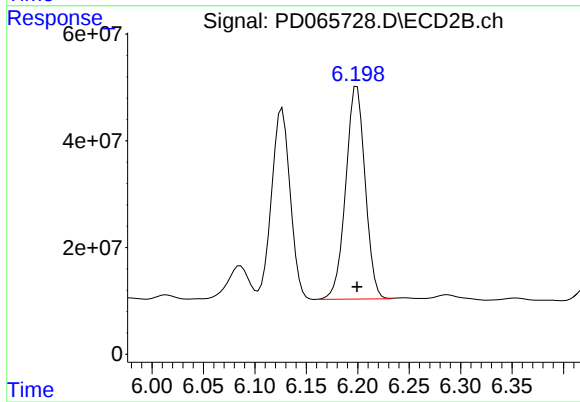


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 523760990
Conc: 500.00 ng/ml

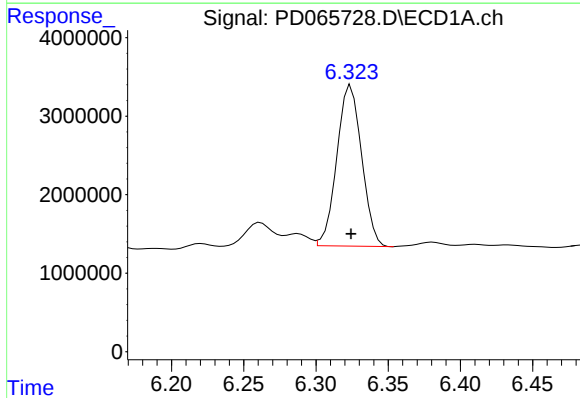


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 24456229
Conc: 500.00 ng/ml

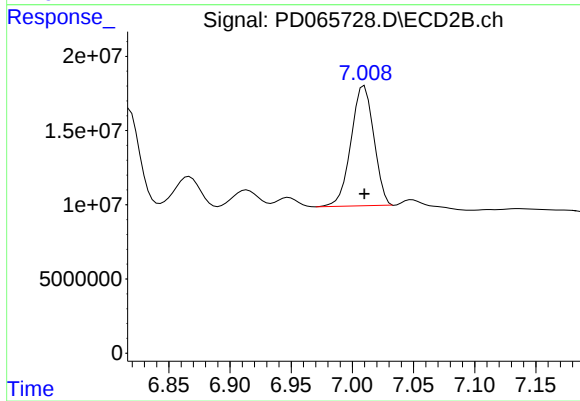


#27 Chlordane-5

R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 104812744
Conc: 500.00 ng/ml

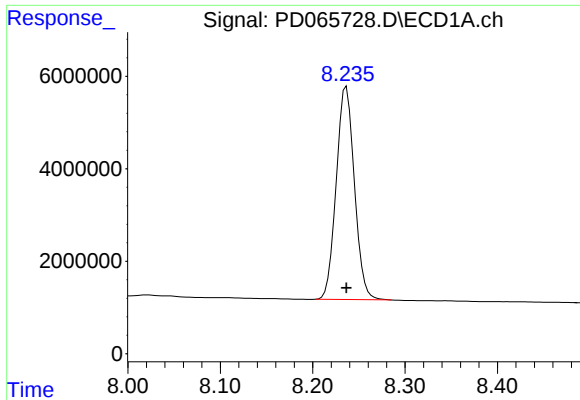

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 62974782
Conc: 50.00 ng/ml

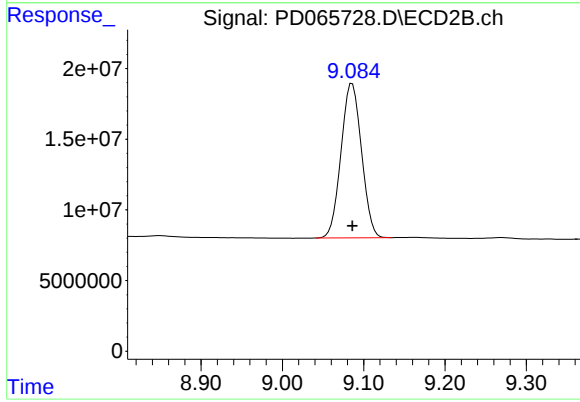

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 191165000
Conc: 50.00 ng/ml