

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 11:26
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:51:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 01:50:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.014	23820410	172.0E6	23.685	24.839
28)	SA Decachlor...	8.237	9.086	31904943	97375975	25.332	25.469
Target Compounds							
23)	Chlordane-1	4.364	5.009	8155977	65911037	245.905	256.820
24)	Chlordane-2	4.864	5.479	10837099	63648092	253.066	258.803
25)	Chlordane-3	5.430	6.127	28789675	223.4E6	237.946	247.644
26)	Chlordane-4	5.488	6.199	24838560	260.5E6	242.434	248.708
27)	Chlordane-5	6.325	7.010	11930469	50505375	243.915	240.931


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 11:26
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:51:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 01:50:44 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

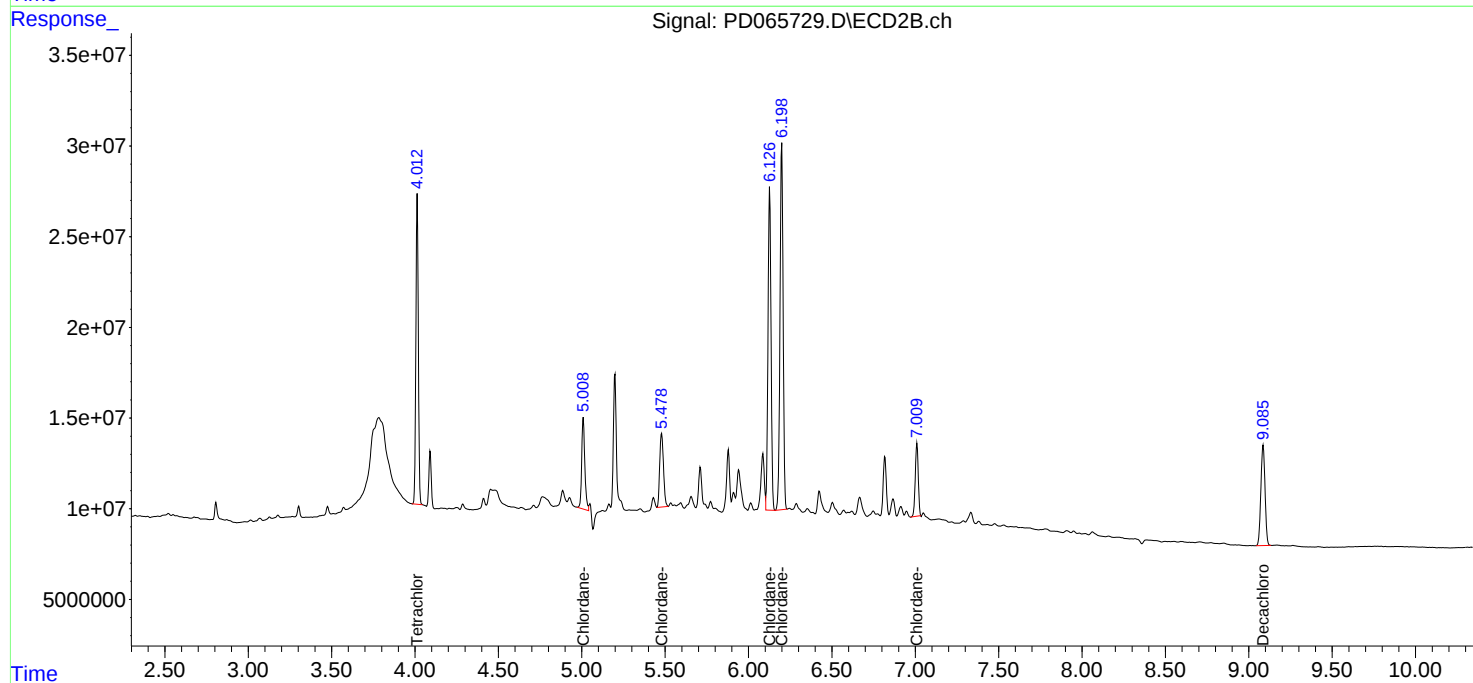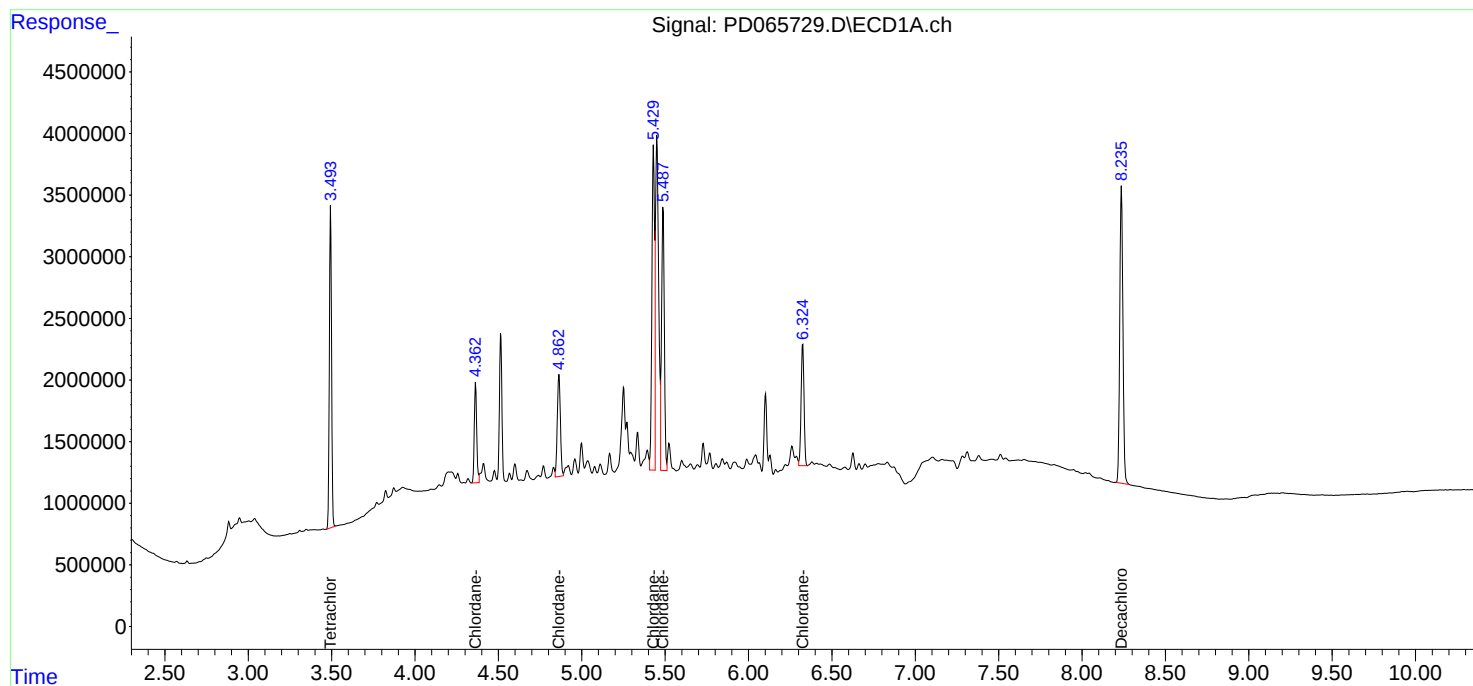

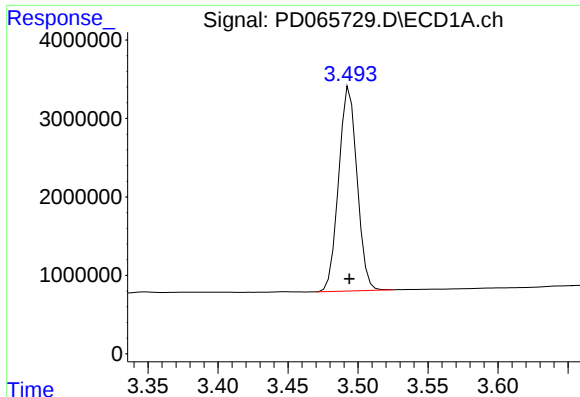


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 23820410
Conc: 23.69 ng/ml

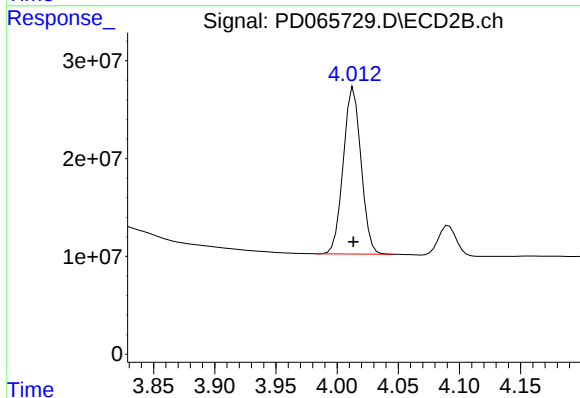


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 172030651
Conc: 24.84 ng/ml

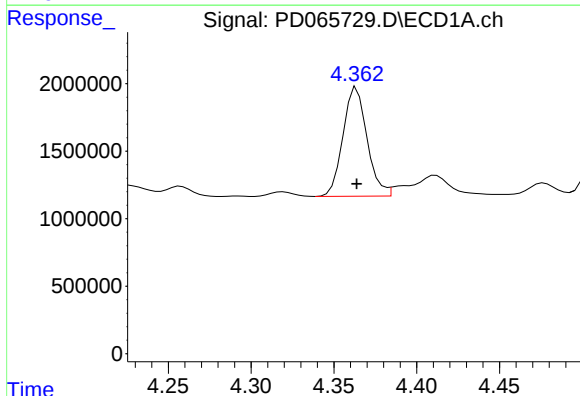


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 8155977
Conc: 245.90 ng/ml

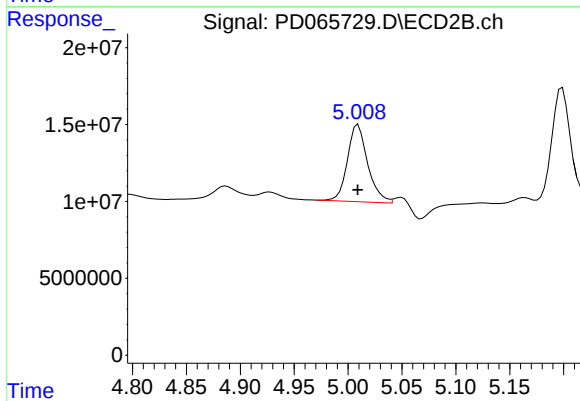


#23 Chlordane-1

R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 65911037
Conc: 256.82 ng/ml

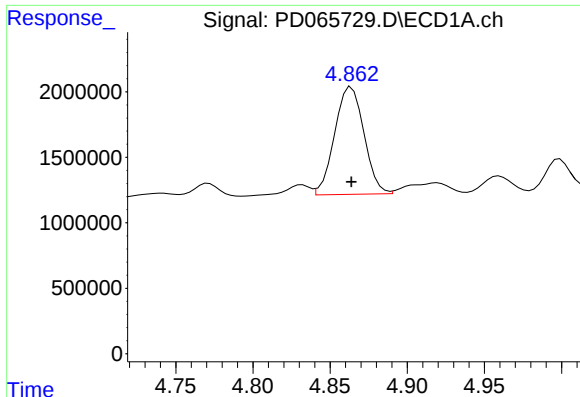


#24 Chlordane-2

R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 10837099
Conc: 253.07 ng/ml

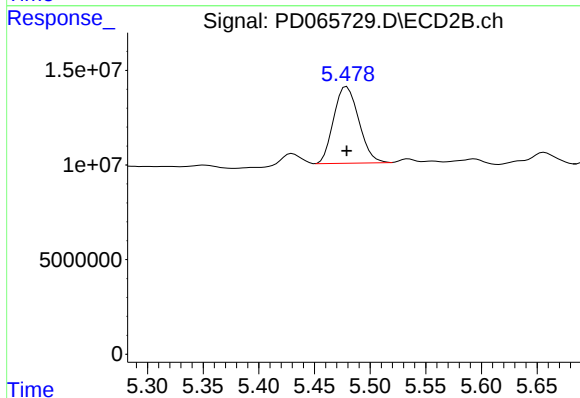


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 63648092
Conc: 258.80 ng/ml

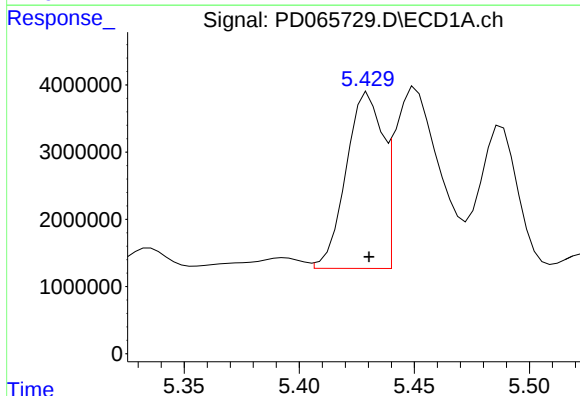


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 28789675
Conc: 237.95 ng/ml

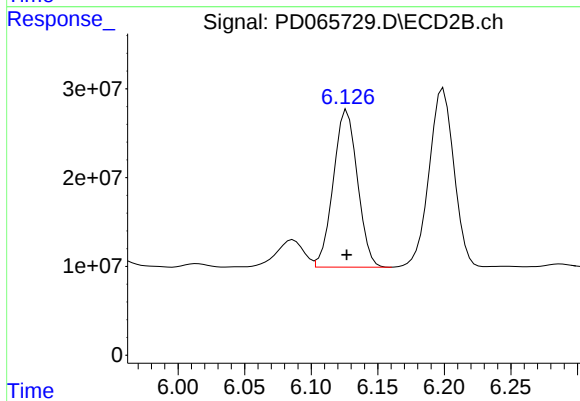


#25 Chlordane-3

R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 223446932
Conc: 247.64 ng/ml

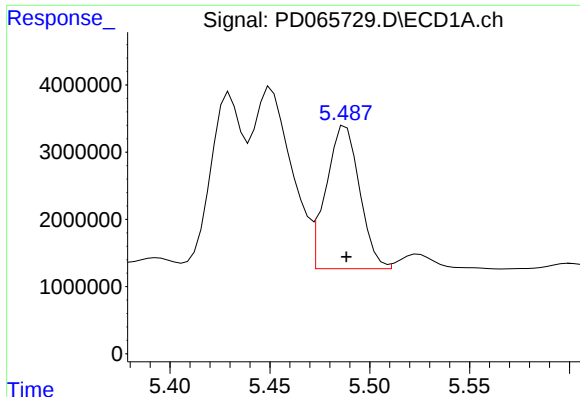


#26 Chlordane-4

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 24838560
Conc: 242.43 ng/ml

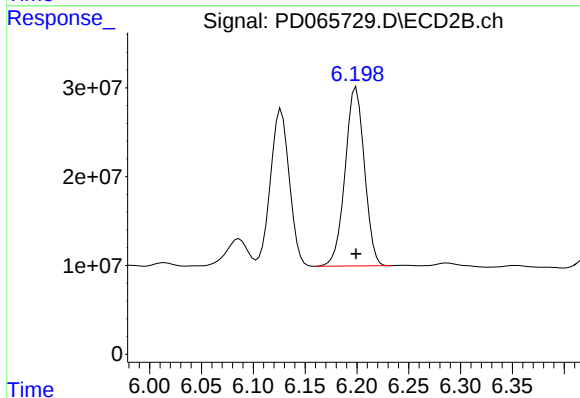


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 260526655
Conc: 248.71 ng/ml

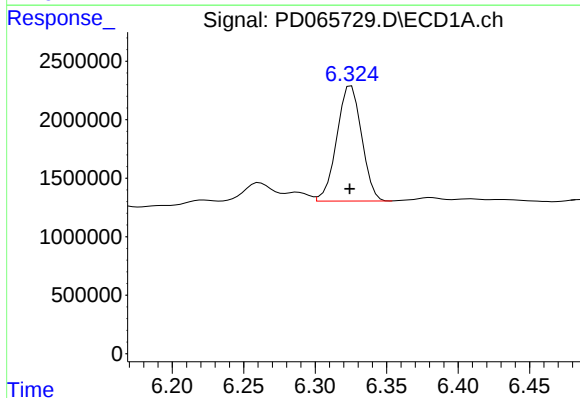


#27 Chlordane-5

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 11930469
Conc: 243.91 ng/ml

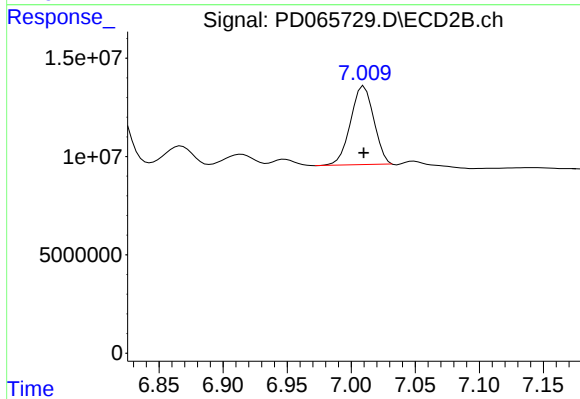


#27 Chlordane-5

R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 50505375
Conc: 240.93 ng/ml

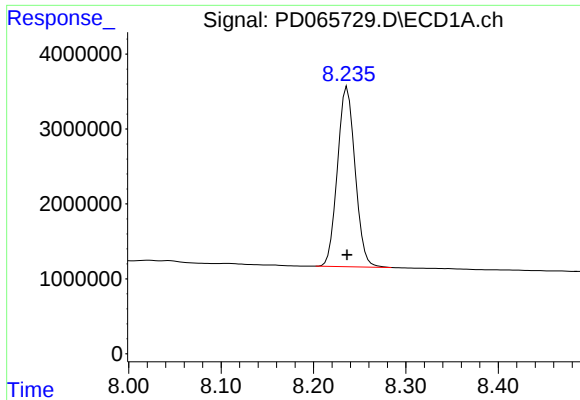

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 31904943
Conc: 25.33 ng/ml

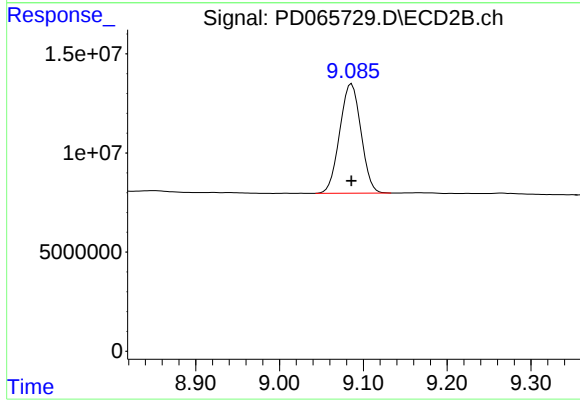

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 97375975
Conc: 25.47 ng/ml