

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2021 06:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 07:52:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 02:05:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	18828734	155.4E6	24.114	24.534
28)	SA Decachlor...	8.235	9.084	31567783	91172814	28.347	26.251
Target Compounds							
6)	B beta-BHC	4.476	4.891f	1489402	2389765	2.331	0.564 #
15)	B Endosulfa...	0.000	6.934	0	1063262	N.D.	0.200 #
22)	Mirex	7.383	0.000	906192	0	0.775	N.D. #
23)	Chlordane-1	4.391f	0.000	1783541	0	53.635	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2021 06:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 07:52:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 02:05:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

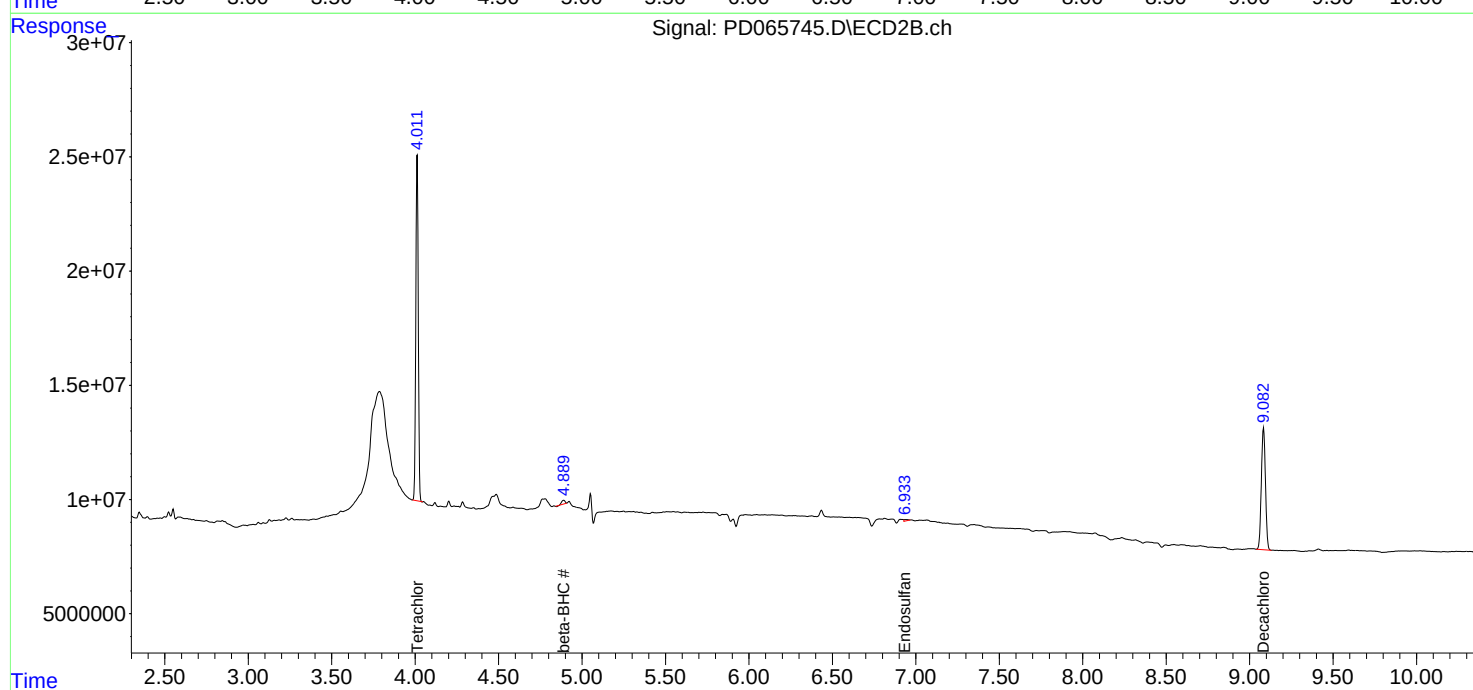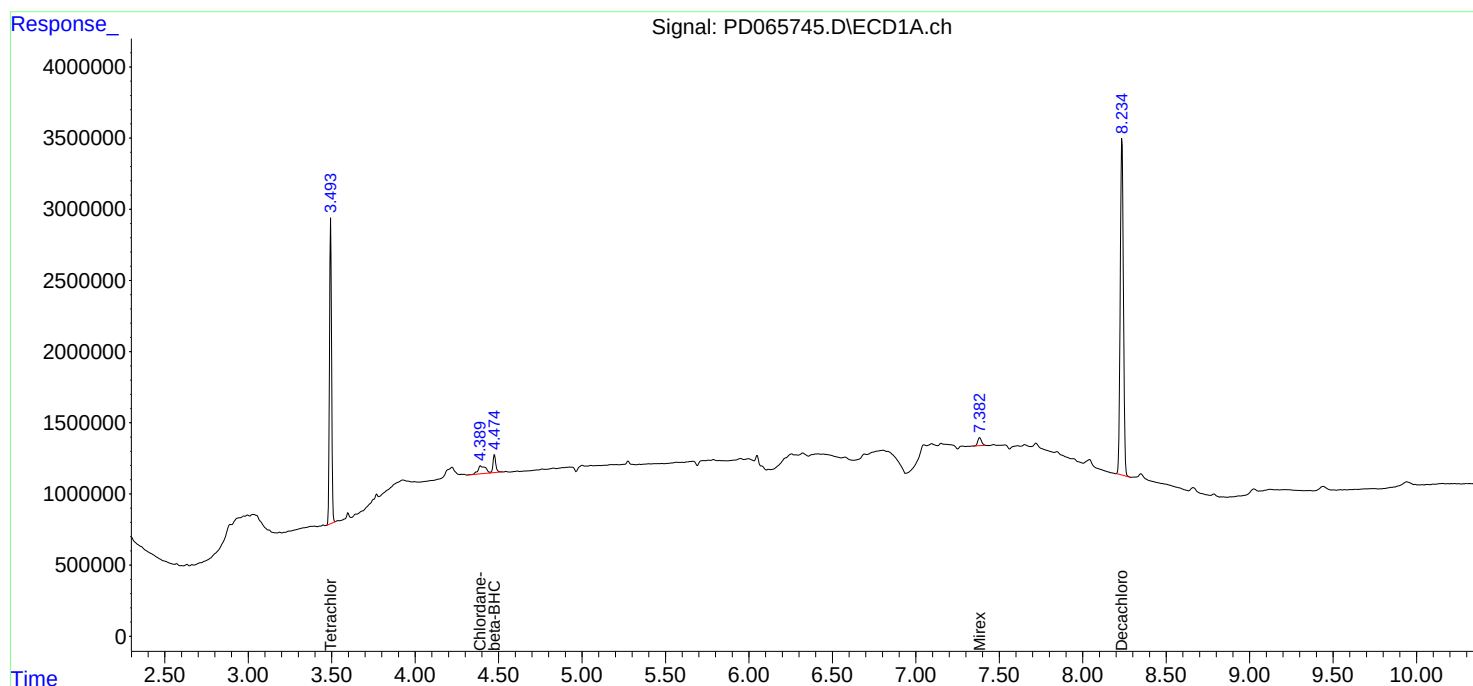

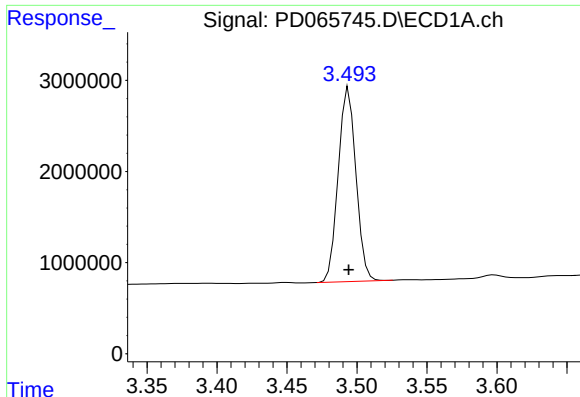


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 18828734
Conc: 24.11 ng/ml

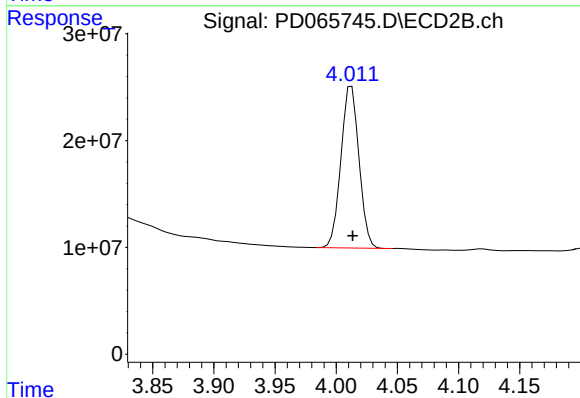


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 155413207
Conc: 24.53 ng/ml

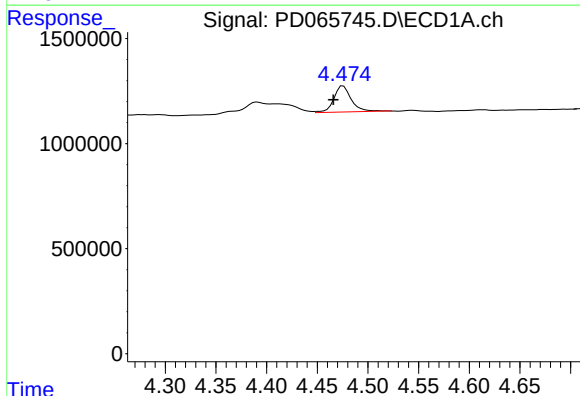


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.010 min
Response: 1489402
Conc: 2.33 ng/ml

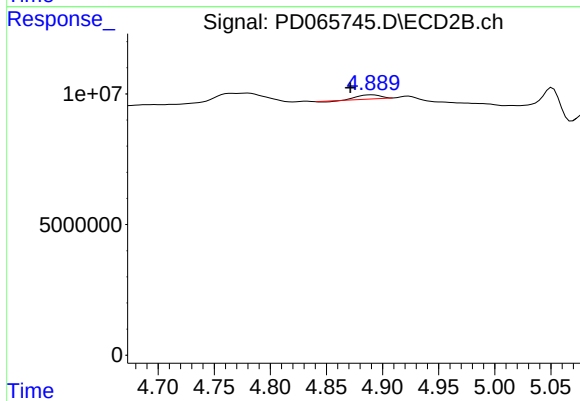


#6 beta-BHC

R.T.: 4.891 min
Delta R.T.: 0.019 min
Response: 2389765
Conc: 0.56 ng/ml

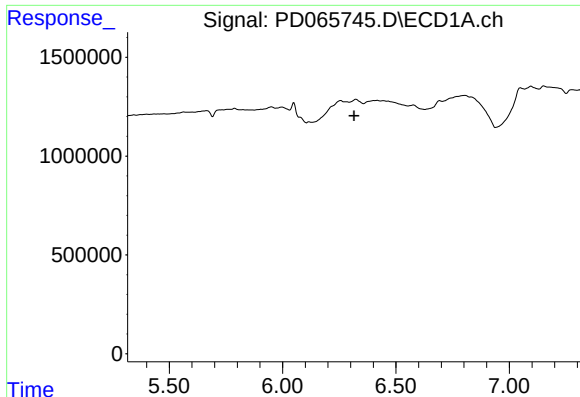


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

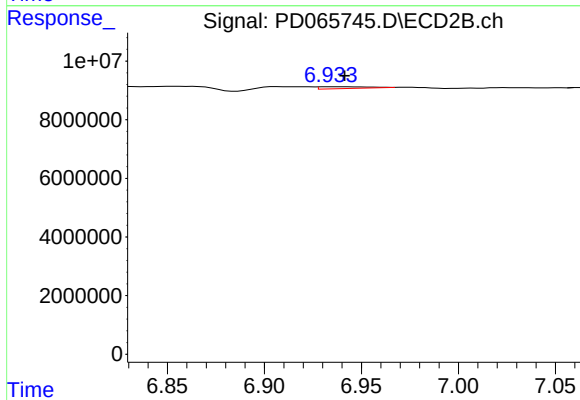


#15 Endosulfan II

R.T.: 6.934 min
Delta R.T.: -0.007 min
Response: 1063262
Conc: 0.20 ng/ml

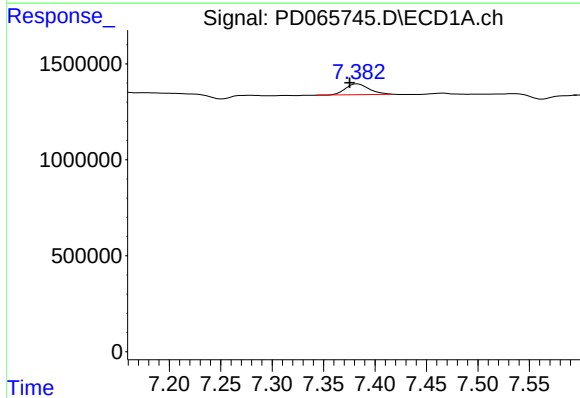


#22 Mirex

R.T.: 7.383 min
Delta R.T.: 0.008 min
Response: 906192
Conc: 0.78 ng/ml

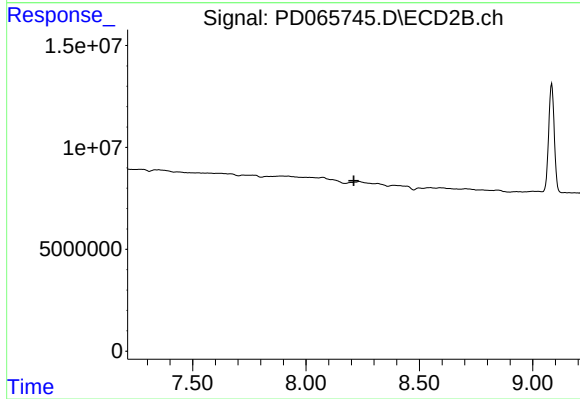


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.211 min
Response: 0
Conc: N.D.

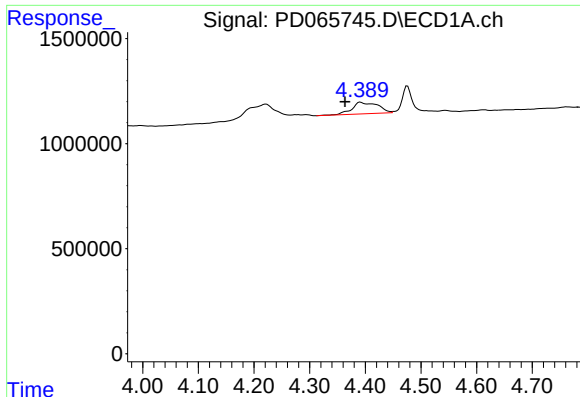


#23 Chlordane-1

R.T.: 4.391 min
Delta R.T.: 0.027 min
Response: 1783541
Conc: 53.64 ng/ml

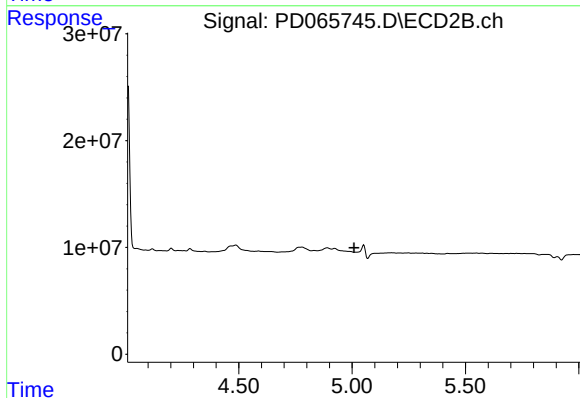


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

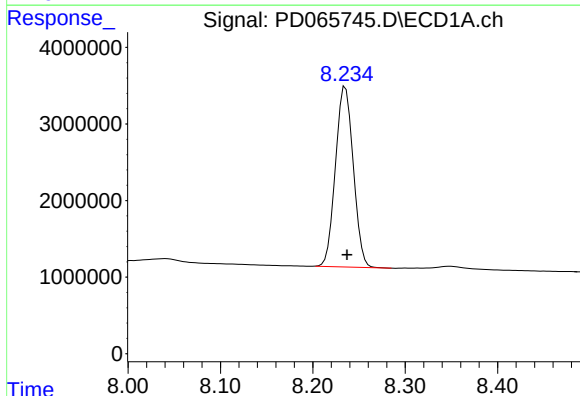

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: -0.002 min
Response: 31567783
Conc: 28.35 ng/ml

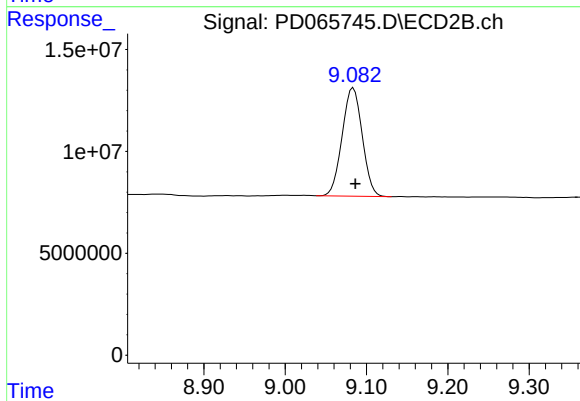

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 91172814
Conc: 26.25 ng/ml