

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2021 07:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 07:53:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 02:05:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	19216854	156.5E6	24.612	24.707
28)	SA Decachlor...	8.235	9.083	28555460	86404945	25.642	24.879
Target Compounds							
6)	B beta-BHC	4.476	4.890f	1449183	2088821	2.268	0.493 #
14)	MA Endrin	6.050	0.000	998646	0	0.901	N.D. #
22)	Mirex	0.000	8.237f	0	1000388	N.D.	0.283 #
23)	Chlordane-1	4.391f	0.000	1605776	0	48.289	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2021 07:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 07:53:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 02:05:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

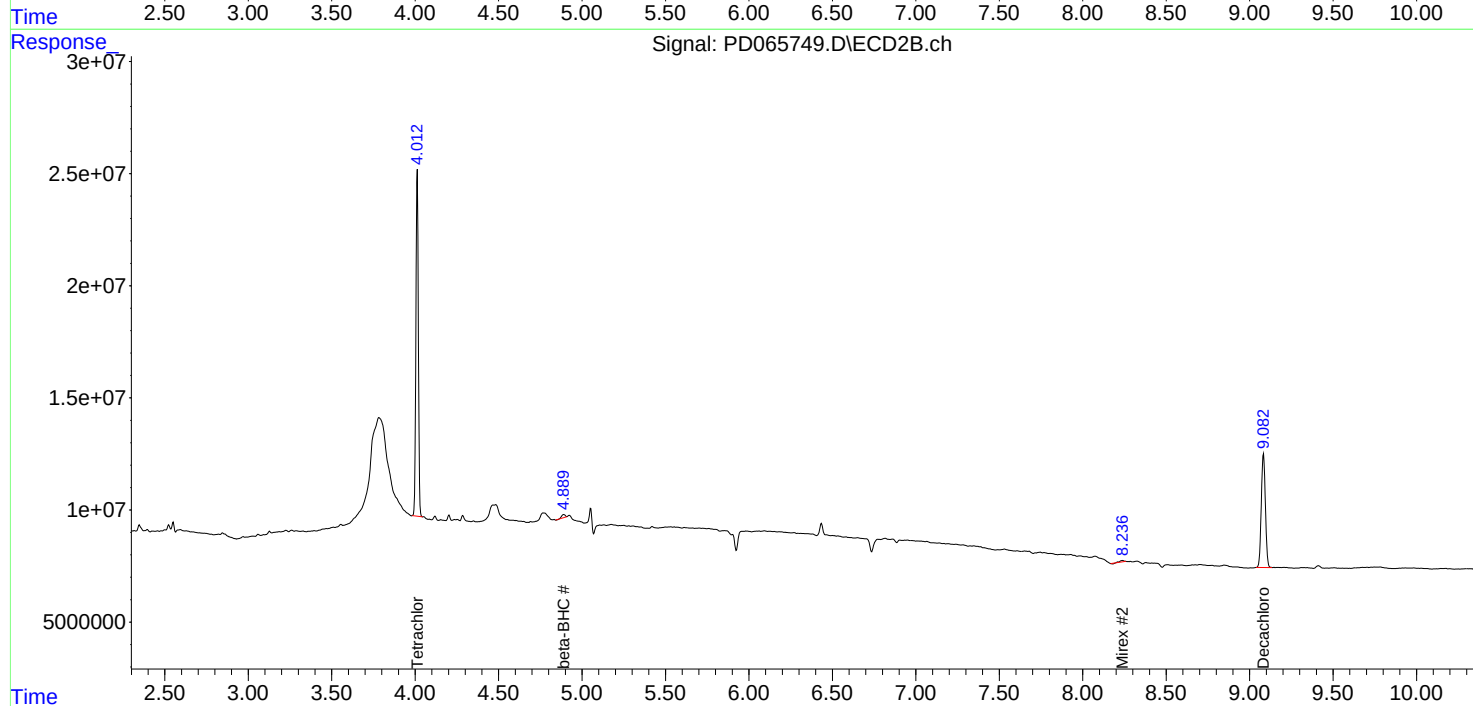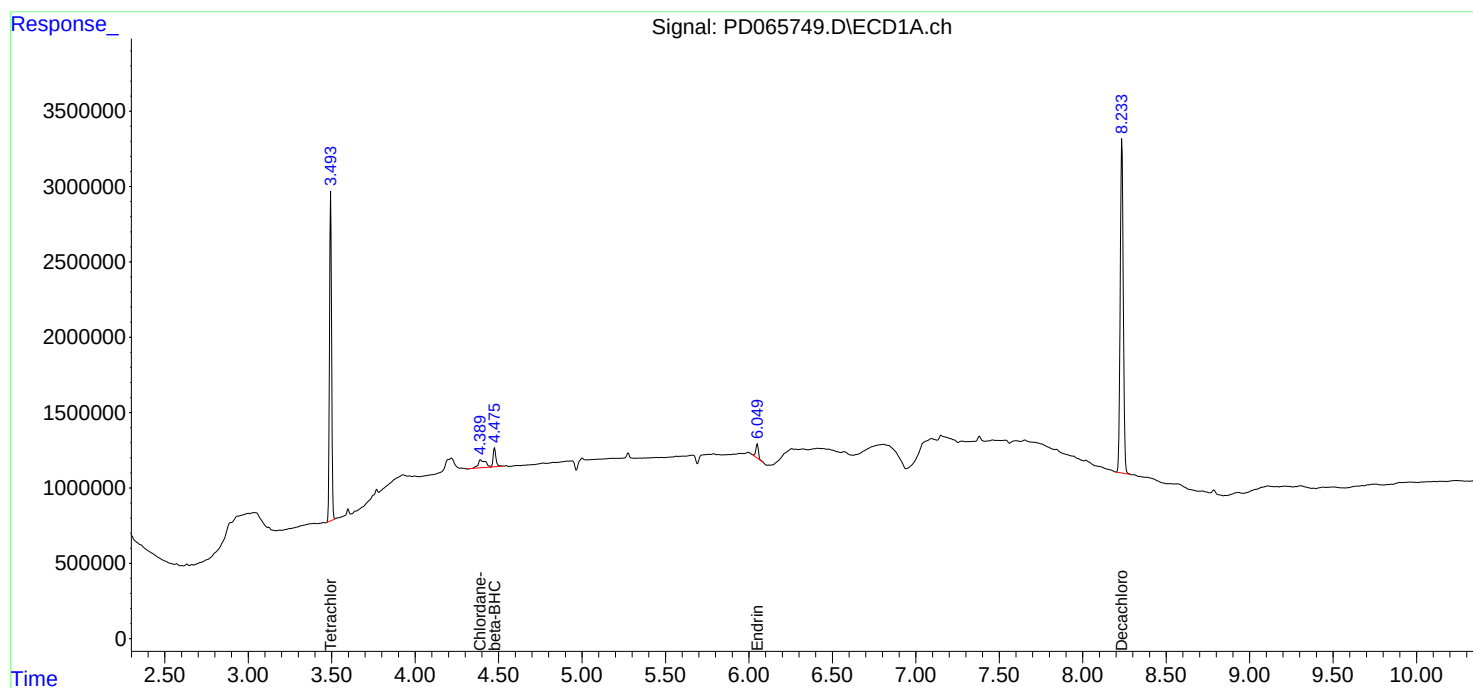

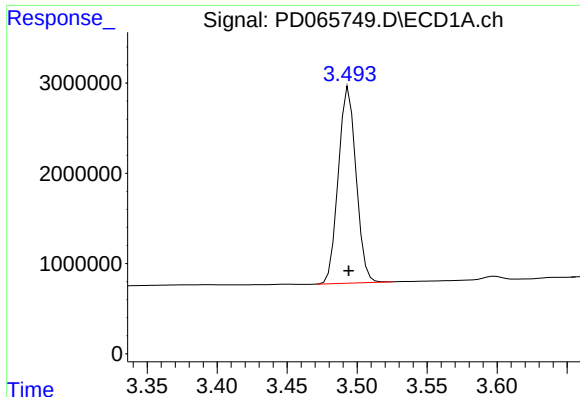


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 19216854
Conc: 24.61 ng/ml

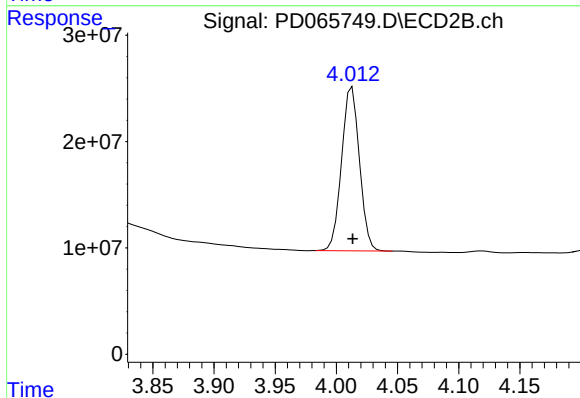


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 156509619
Conc: 24.71 ng/ml

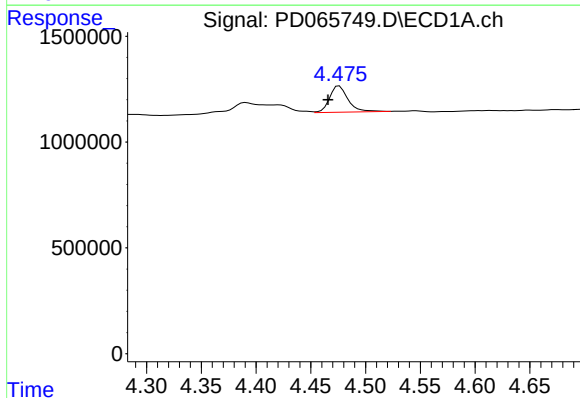


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.010 min
Response: 1449183
Conc: 2.27 ng/ml

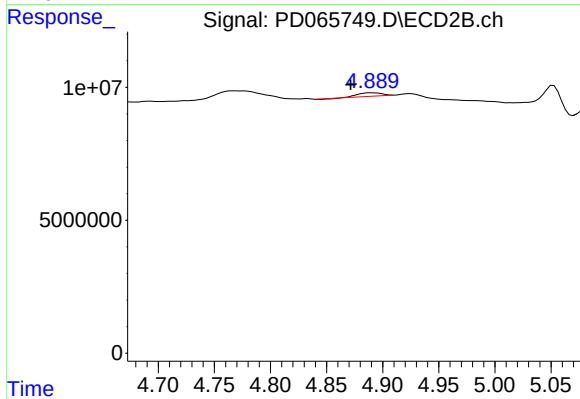


#6 beta-BHC

R.T.: 4.890 min
Delta R.T.: 0.019 min
Response: 2088821
Conc: 0.49 ng/ml

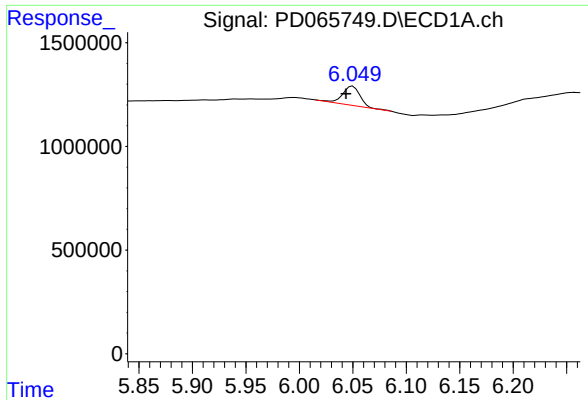


#14 Endrin

R.T.: 6.050 min
Delta R.T.: 0.006 min
Response: 998646
Conc: 0.90 ng/ml

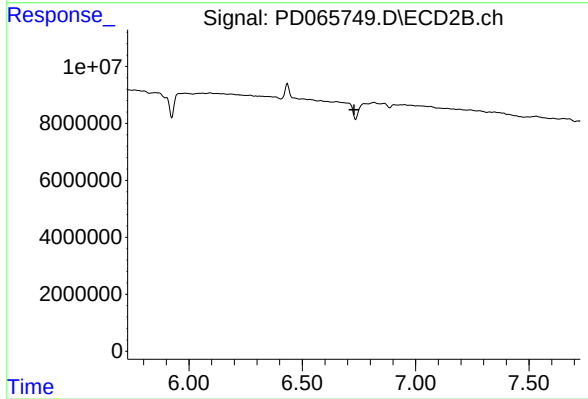


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

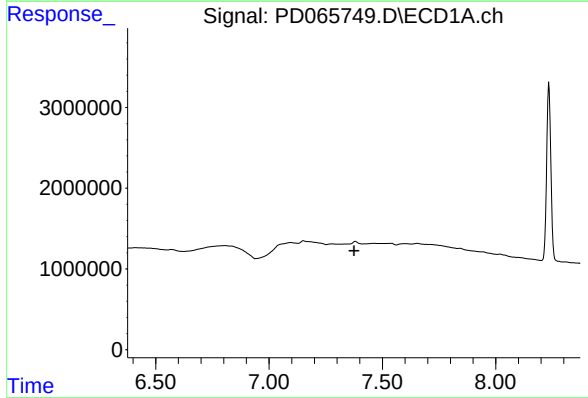


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.375 min
Response: 0
Conc: N.D.

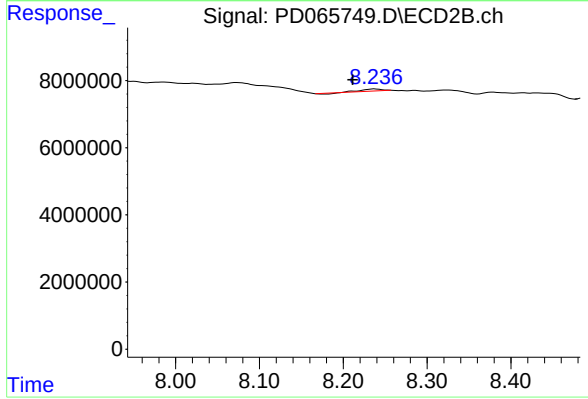


#22 Mirex

R.T.: 8.237 min
Delta R.T.: 0.026 min
Response: 1000388
Conc: 0.28 ng/ml

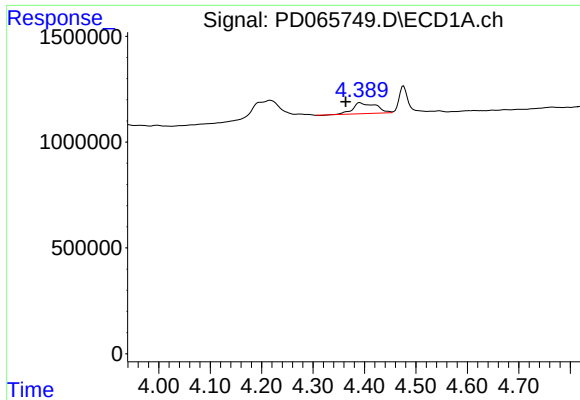


#23 Chlordane-1

R.T.: 4.391 min
Delta R.T.: 0.027 min
Response: 1605776
Conc: 48.29 ng/ml

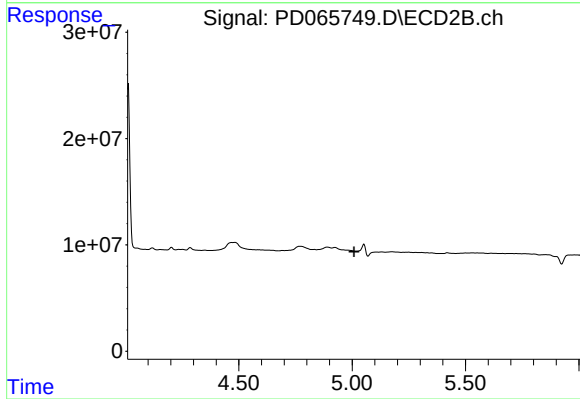


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

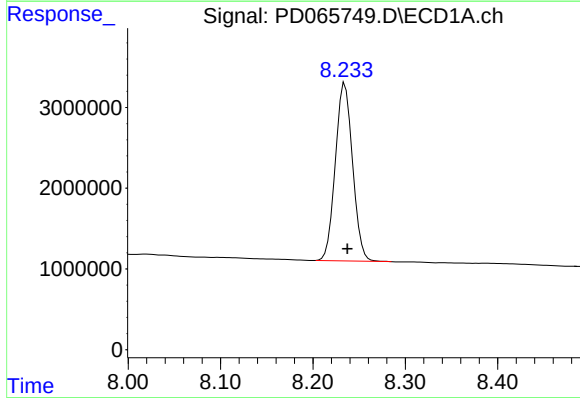

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: -0.003 min
Response: 28555460
Conc: 25.64 ng/ml

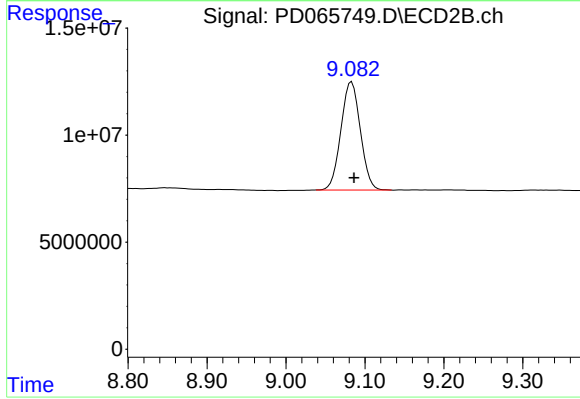

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.003 min
Response: 86404945
Conc: 24.88 ng/ml