

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 10:58
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:51:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 01:50:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.014	75064896	498.0E6	74.638	71.900
28)	SA Decachlor...	8.236	9.086	90084441	277.5E6	71.524	72.583
Target Compounds							
23)	Chlordane-1	4.364	5.009	23975475	180.6E6	722.866	703.840
24)	Chlordane-2	4.864	5.479	30279130	176.3E6	707.074	717.033
25)	Chlordane-3	5.430	6.127	91009364	660.5E6	752.190	732.070
26)	Chlordane-4	5.488	6.200	75688979	763.2E6	738.754	728.622
27)	Chlordane-5	6.325	7.010	35929383	150.4E6	734.565	717.274



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 10:58
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:51:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 01:50:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

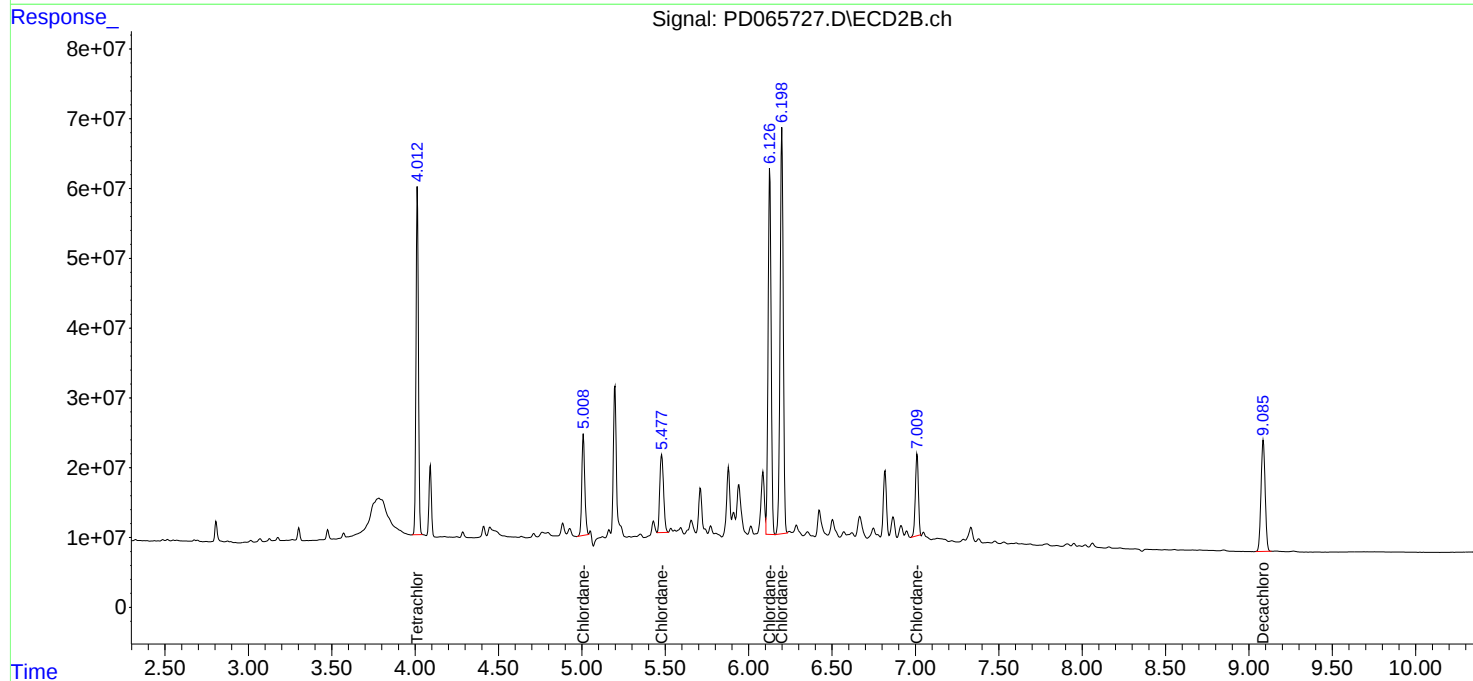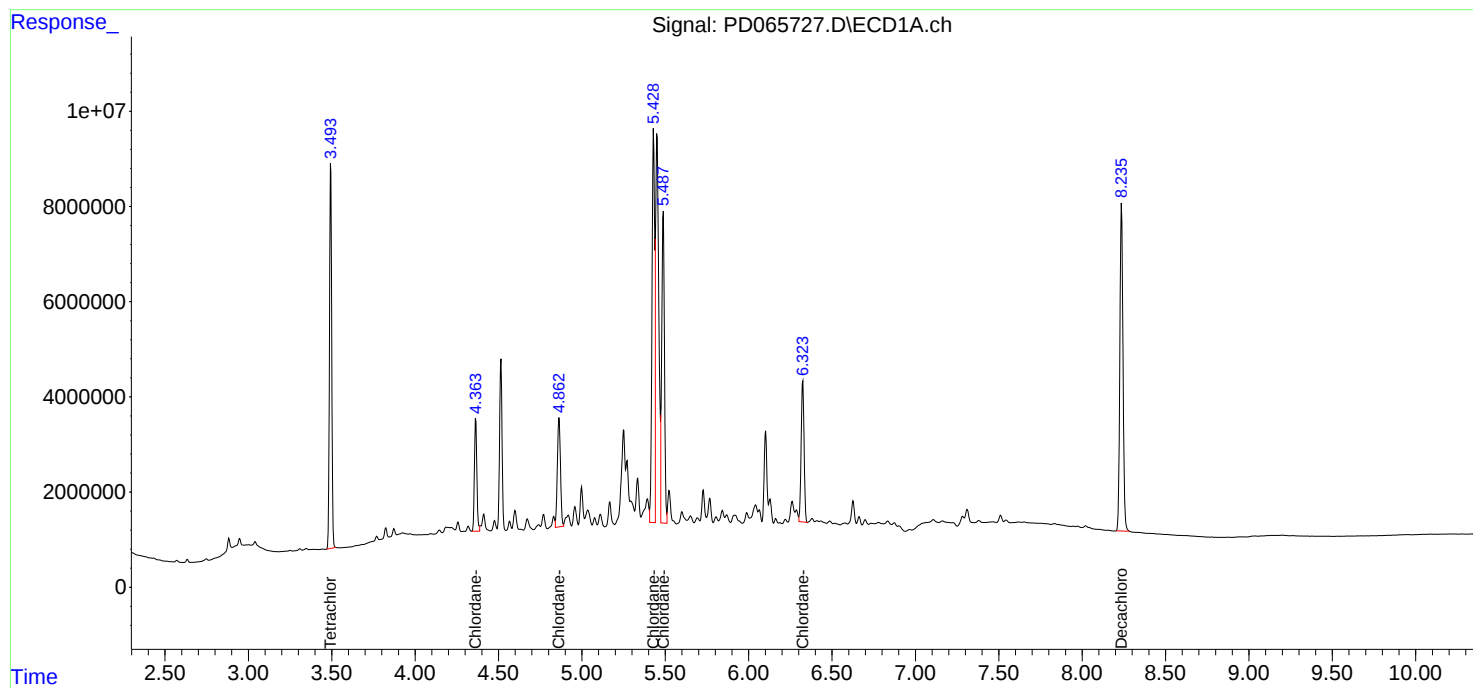


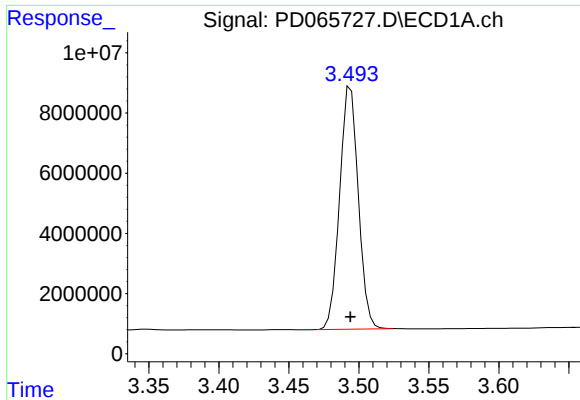

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 75064896
Conc: 74.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

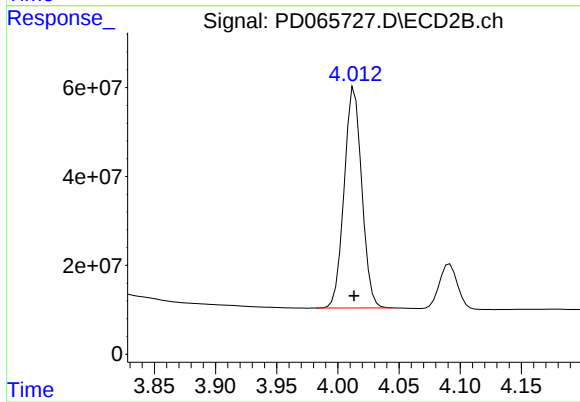


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 497965911
Conc: 71.90 ng/ml

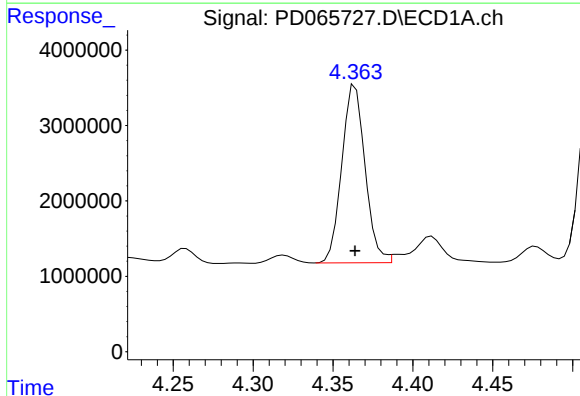


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 23975475
Conc: 722.87 ng/ml

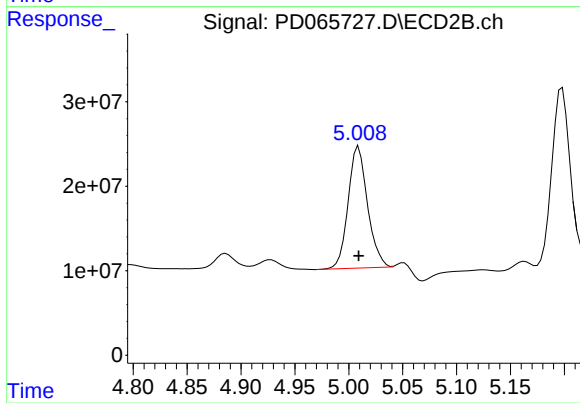

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 180635557
Conc: 703.84 ng/ml

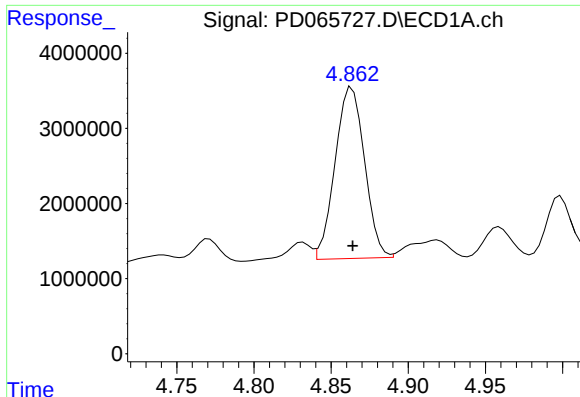

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 30279130
Conc: 707.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

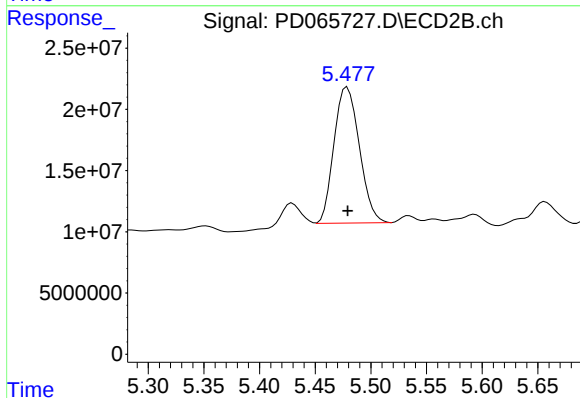


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 176341877
Conc: 717.03 ng/ml

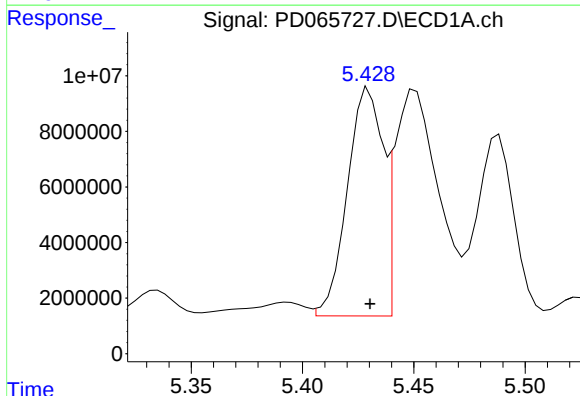


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 91009364
Conc: 752.19 ng/ml

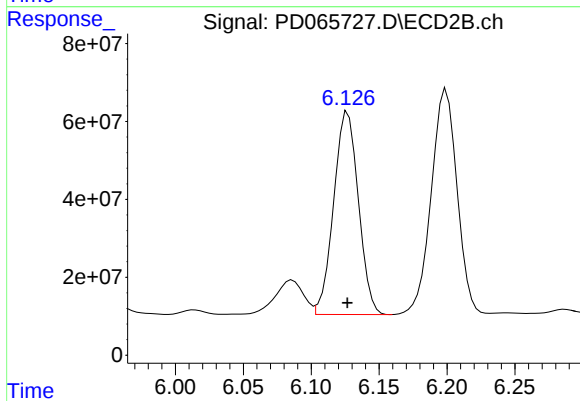

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 660540877
Conc: 732.07 ng/ml

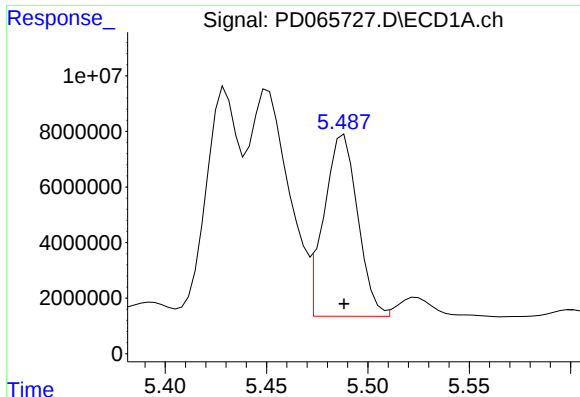

#26 Chlordane-4


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 75688979
Conc: 738.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

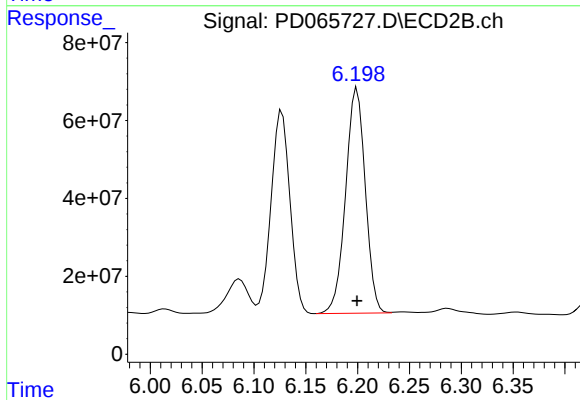


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 763247647
Conc: 728.62 ng/ml

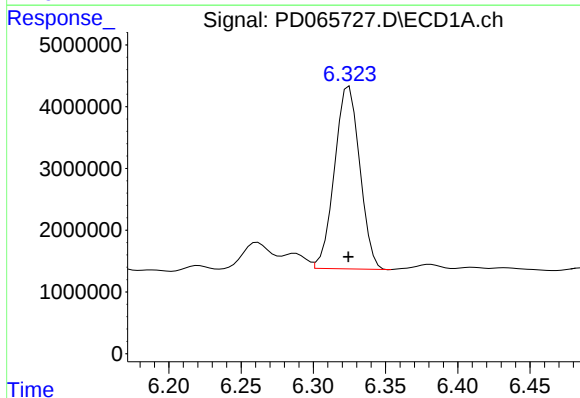


#27 Chlordane-5

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 35929383
Conc: 734.57 ng/ml

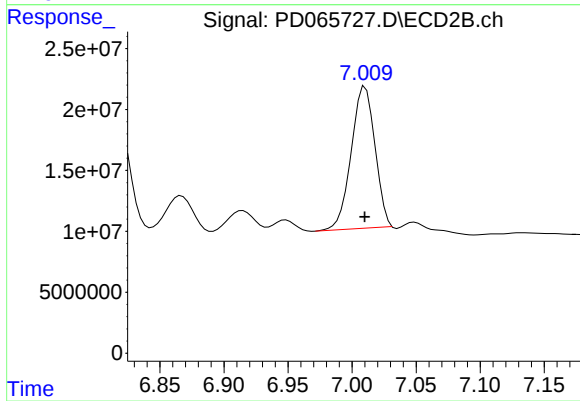

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 150358903
Conc: 717.27 ng/ml

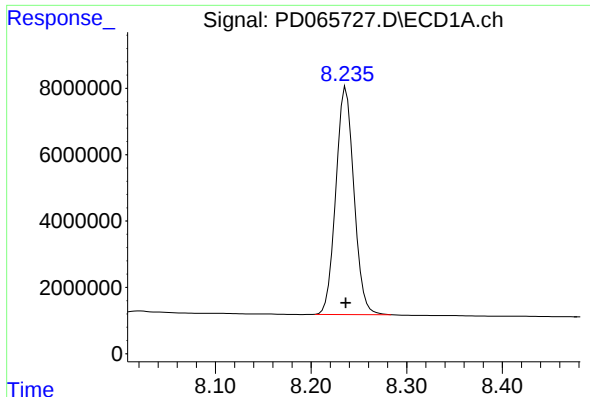

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 90084441
Conc: 71.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

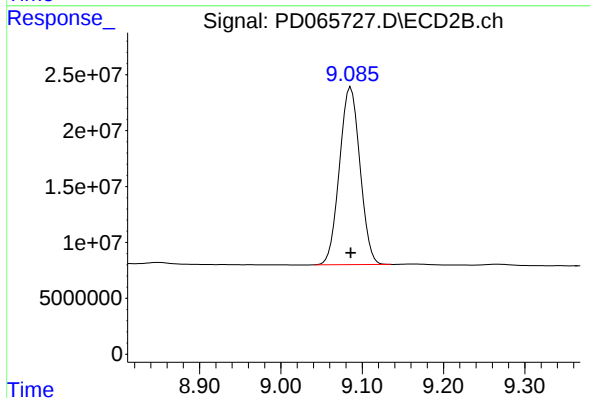

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 277507414
Conc: 72.58 ng/ml