

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 11:40
 Operator : AR\AJ
 Sample : PCHLORICC50
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:52:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 01:50:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	4808230	37606285	4.781	5.430
28)	SA Decachlor...	8.236	9.086	7437170	21038777	5.905	5.503
Target Compounds							
23)	Chlordane-1	4.364	5.009	1808403	10787787	54.524	42.034
24)	Chlordane-2	4.864	5.479	2190335	14079870	51.148	57.251
25)	Chlordane-3	5.430	6.127	5918445	49204110	48.916	54.532
26)	Chlordane-4	5.488	6.199	4952831	58307857	48.342	55.663
27)	Chlordane-5	6.324	7.010	2478698	10368628	50.676	49.463



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 11:40
Operator : AR\AJ
Sample : PCHLORICC50
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:52:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 01:50:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

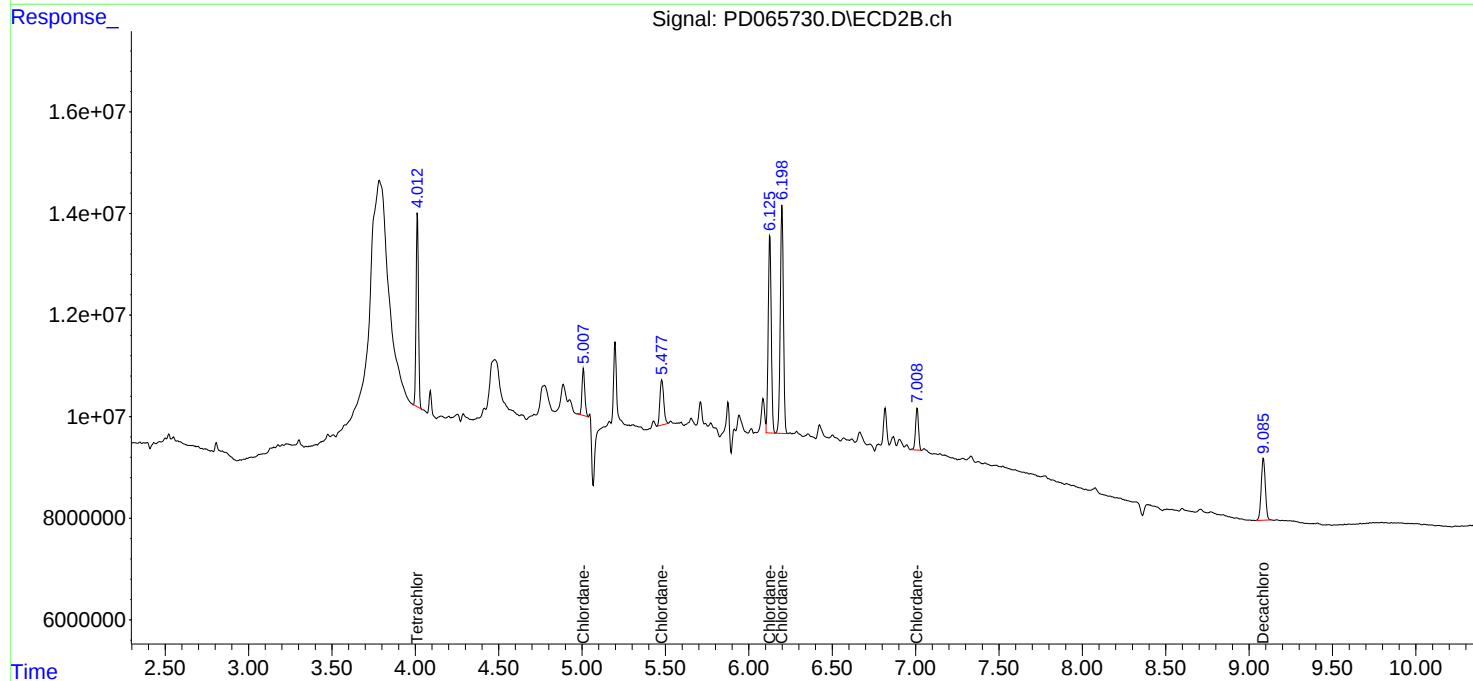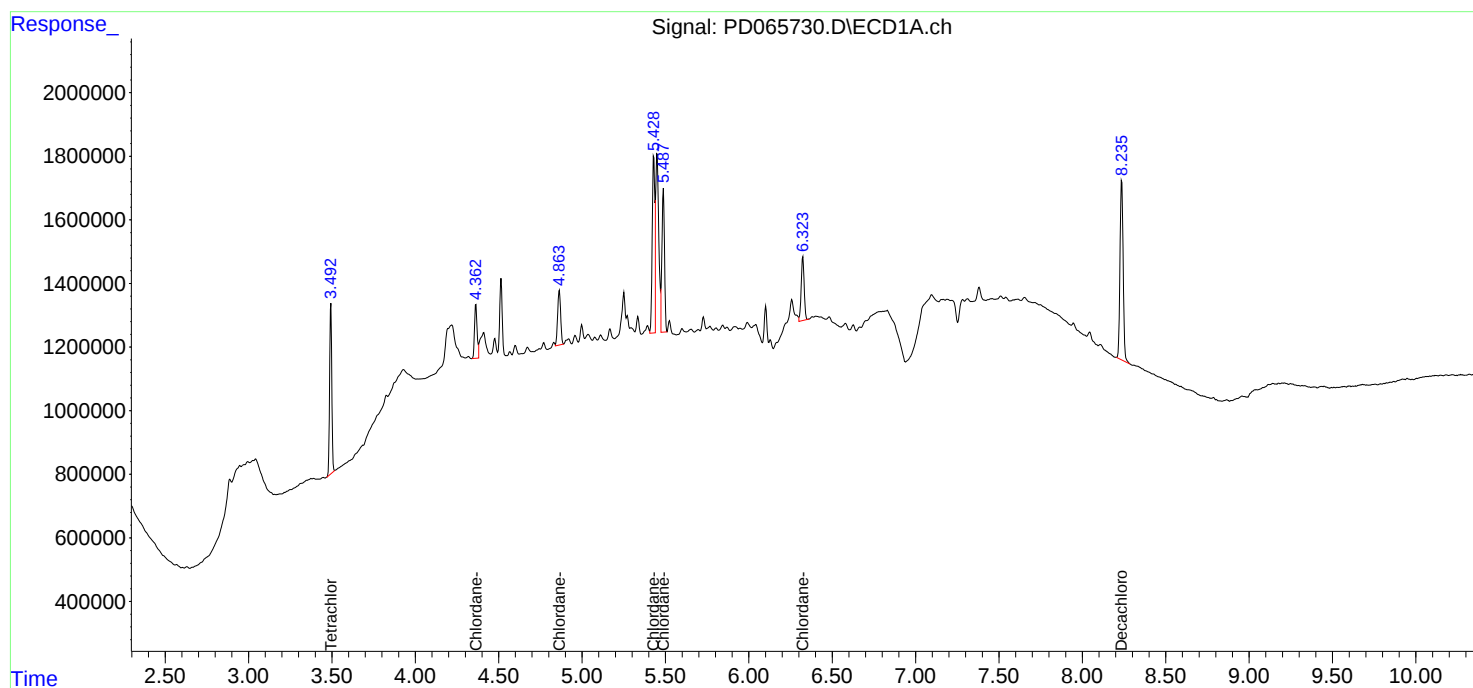


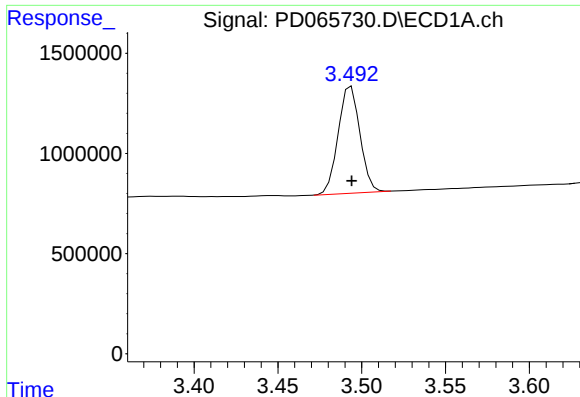

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 4808230
Conc: 4.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

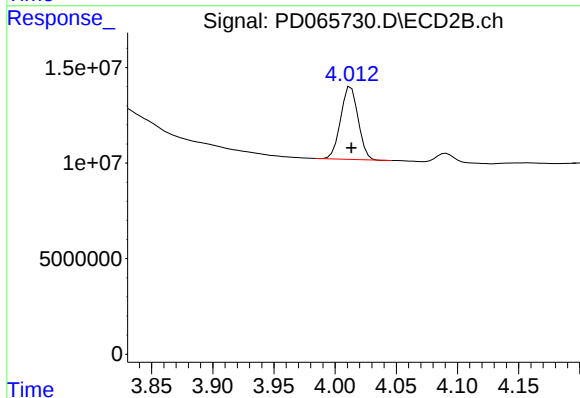


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 37606285
Conc: 5.43 ng/ml

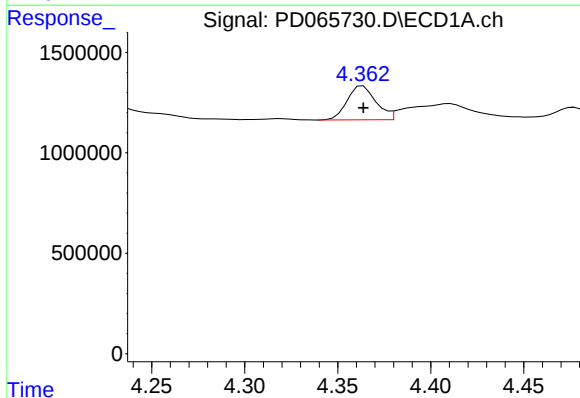


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 1808403
Conc: 54.52 ng/ml

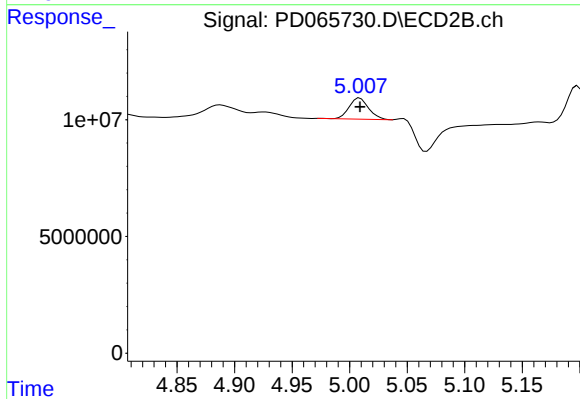

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 10787787
Conc: 42.03 ng/ml

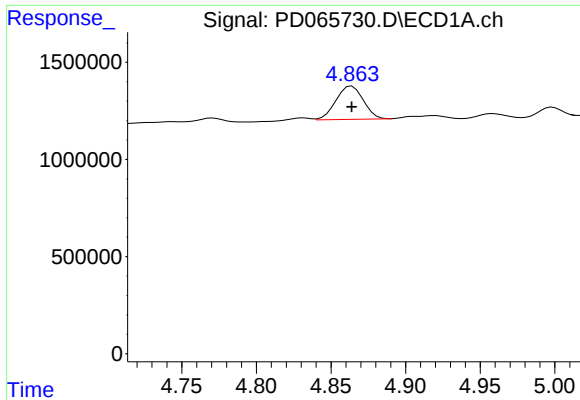

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 2190335
Conc: 51.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

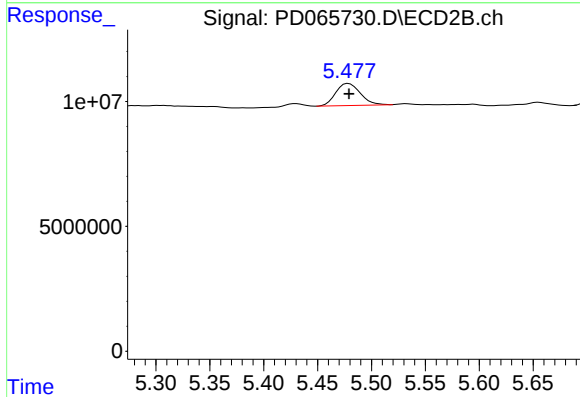


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 14079870
Conc: 57.25 ng/ml

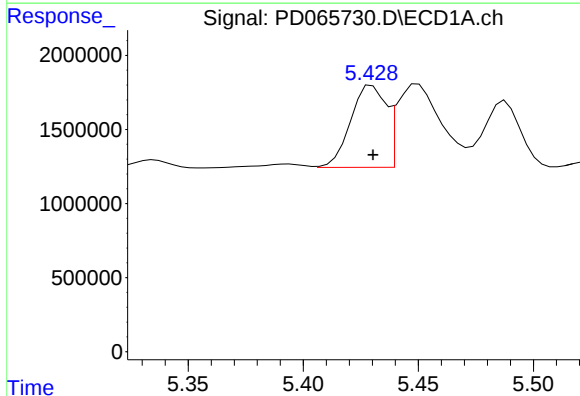


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 5918445
Conc: 48.92 ng/ml

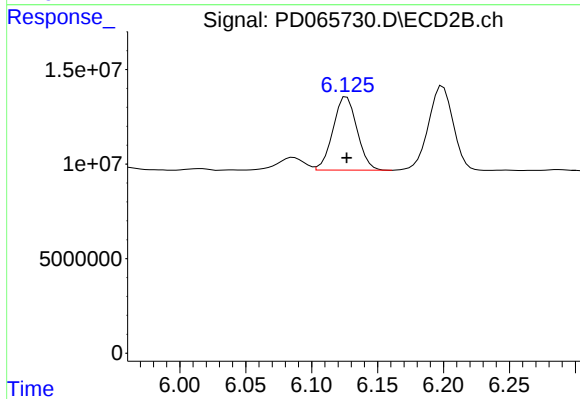

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 49204110
Conc: 54.53 ng/ml

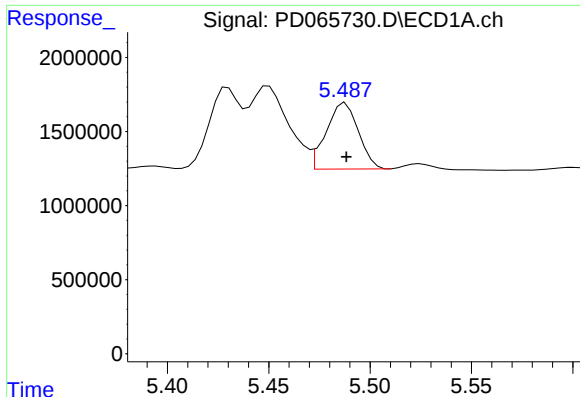

#26 Chlordane-4


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 4952831
Conc: 48.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

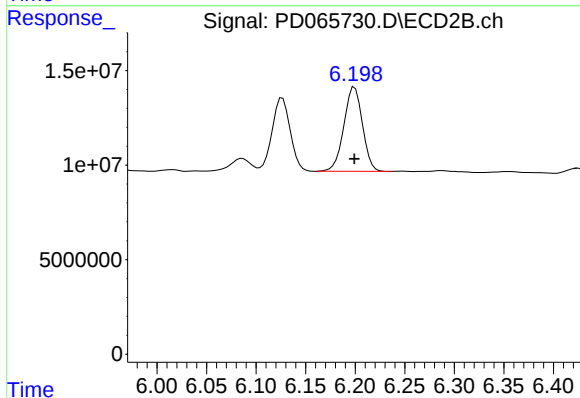


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 58307857
Conc: 55.66 ng/ml

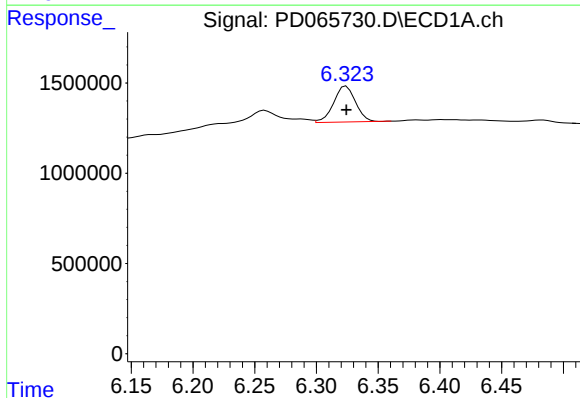


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 2478698
Conc: 50.68 ng/ml

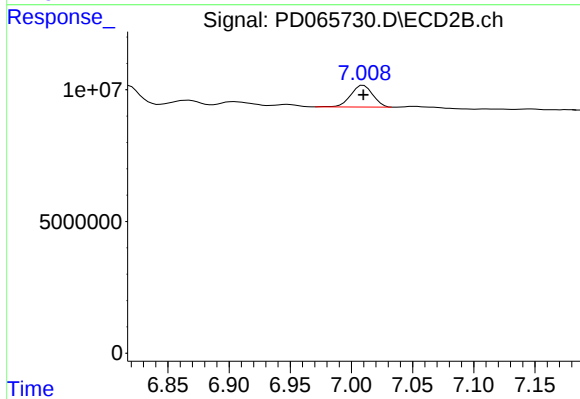

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 10368628
Conc: 49.46 ng/ml

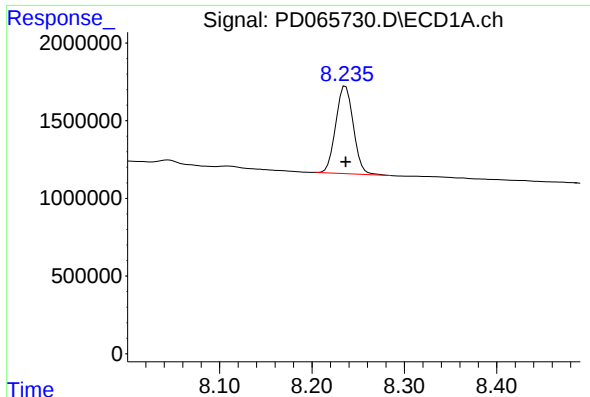

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 7437170
Conc: 5.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

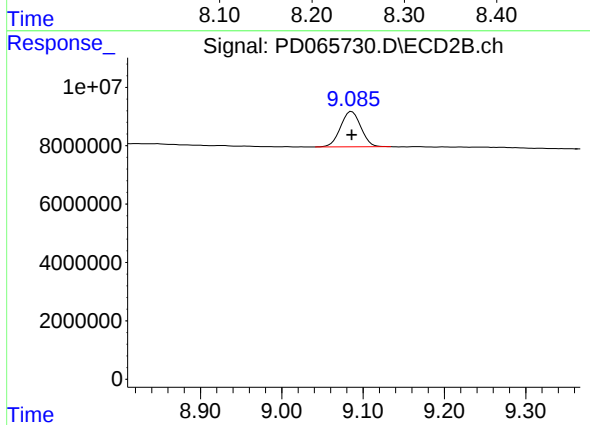

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 21038777
Conc: 5.50 ng/ml