

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
 Data File : PD065743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2021 05:41
 Operator : AR\AJ
 Sample : M3741-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 S-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 07:51:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 16 02:05:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.012	15510446	131.8E6	19.865	20.802
28)	SA Decachlor...	8.235	9.085	18967696	53444142	17.032	15.388
Target Compounds							
12)	B 4,4'-DDE	5.650	6.356	1017966	6788047	0.943	1.110
17)	MA 4,4'-DDT	6.405	7.148	855750	3783754	0.810	0.787



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091521\
Data File : PD065743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2021 05:41
Operator : AR\AJ
Sample : M3741-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
S-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 07:51:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 16 02:05:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

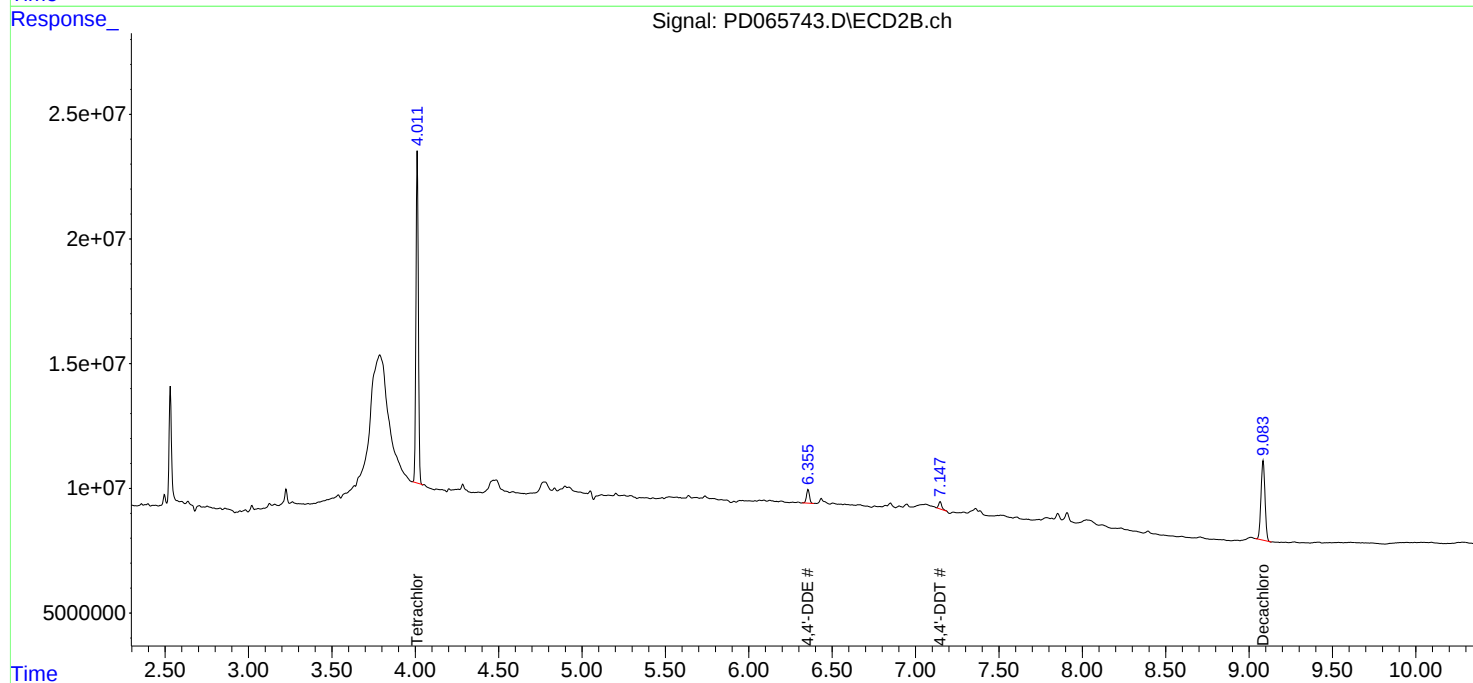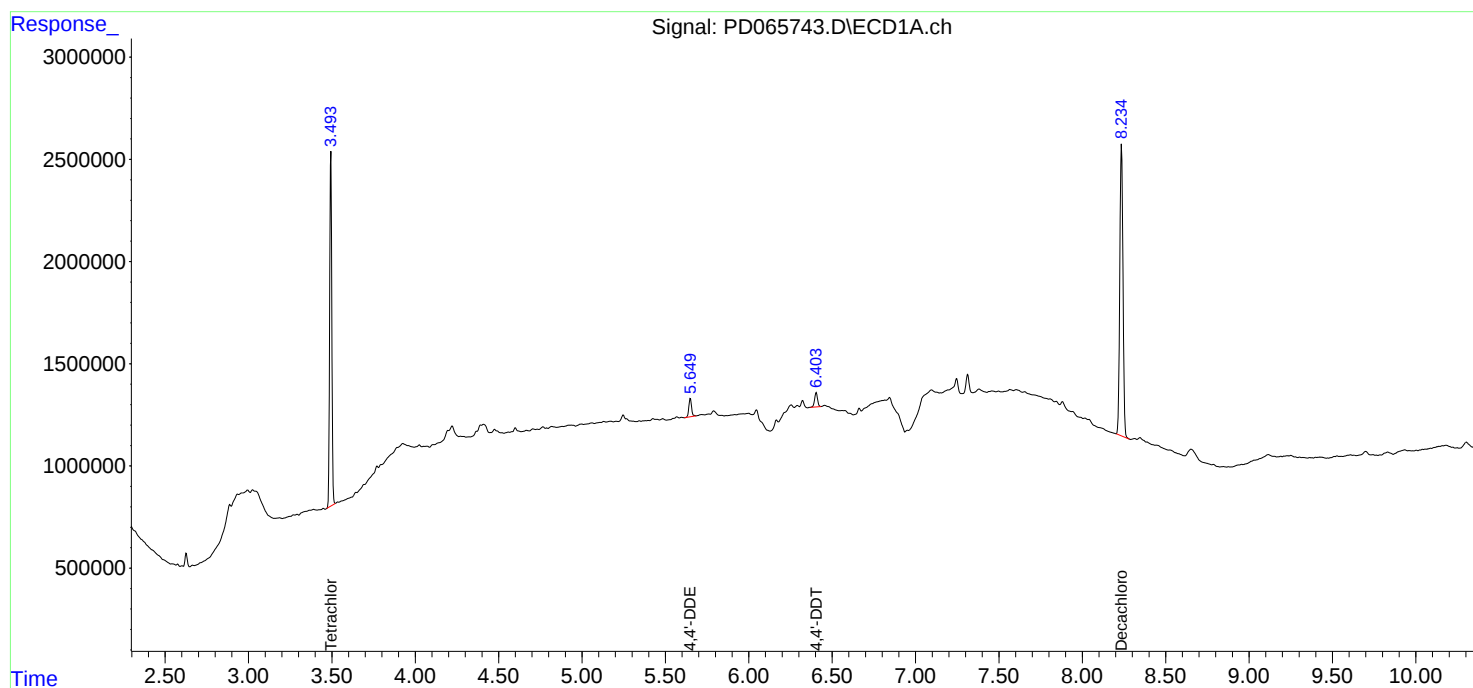


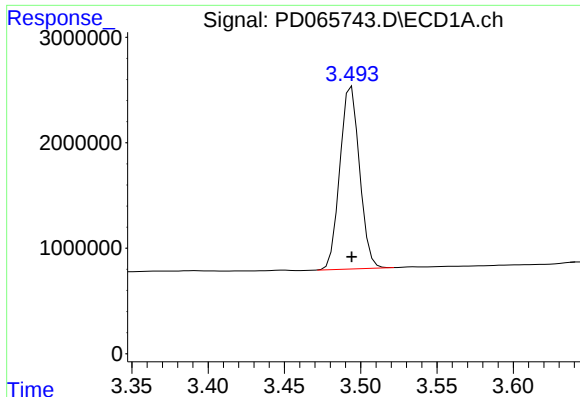

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 15510446
Conc: 19.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
S-4

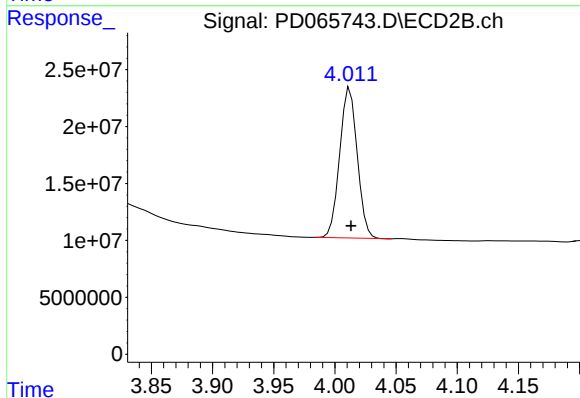


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: -0.001 min
Response: 131777553
Conc: 20.80 ng/ml

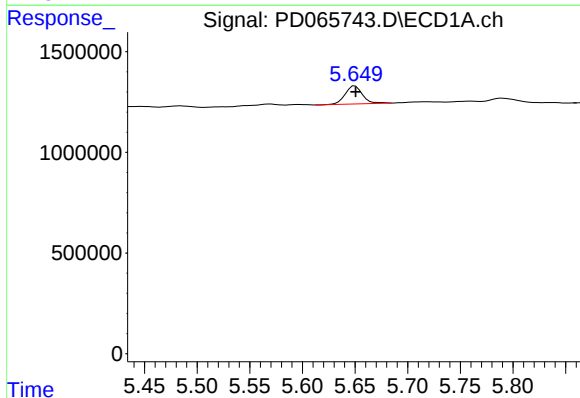


#12 4,4'-DDE

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 1017966
Conc: 0.94 ng/ml

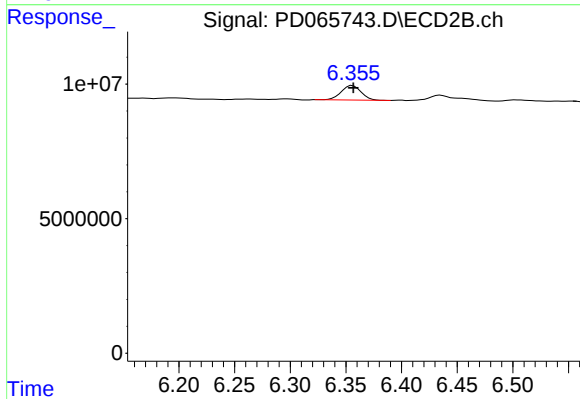

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 6788047
Conc: 1.11 ng/ml

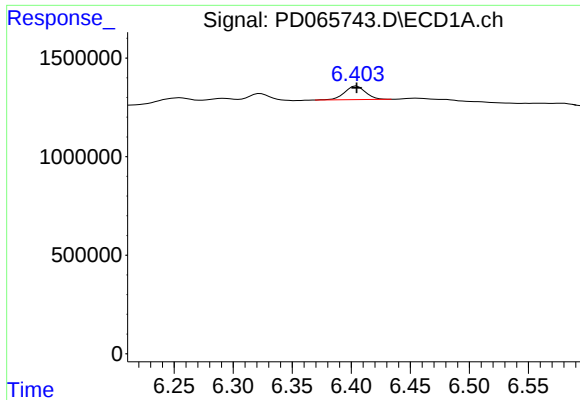

#17 4,4'-DDT


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 855750
Conc: 0.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
S-4

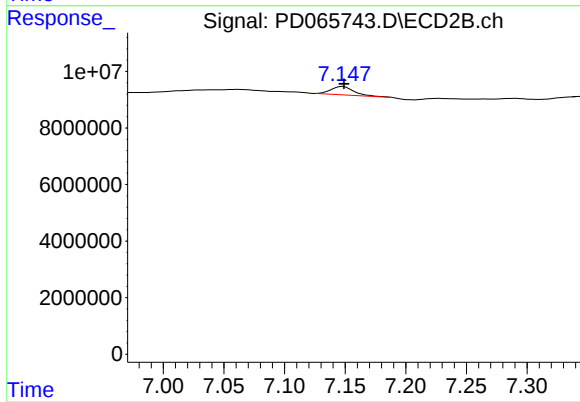


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 3783754
Conc: 0.79 ng/ml

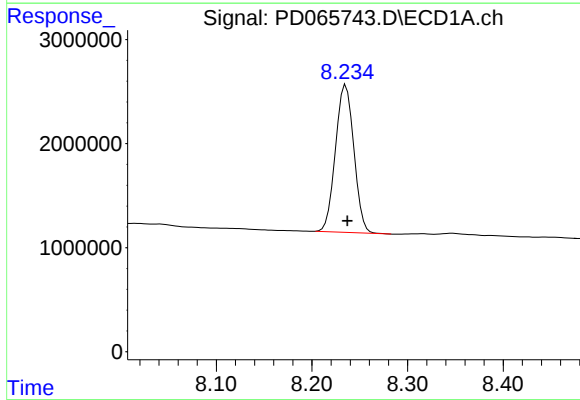

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: -0.002 min
Response: 18967696
Conc: 17.03 ng/ml

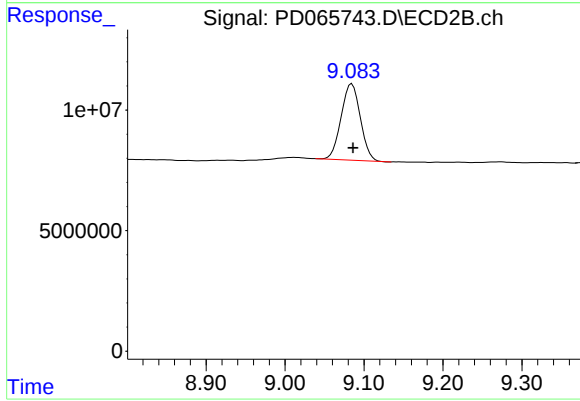

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.001 min
Response: 53444142
Conc: 15.39 ng/ml