

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091522\
 Data File : PD071886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 10:44
 Operator : AR\AJ
 Sample : N4578-41
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CHERRY-HILL-COMP-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:45:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.806	3.564	48682280	633.6E6	19.909	22.080
28) SA Decachlor...	7.996	9.090	35301896	155.8E6	14.013	16.761

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091522\
Data File : PD071886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 10:44
Operator : AR\AJ
Sample : N4578-41
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
CHERRY-HILL-COMP-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:45:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

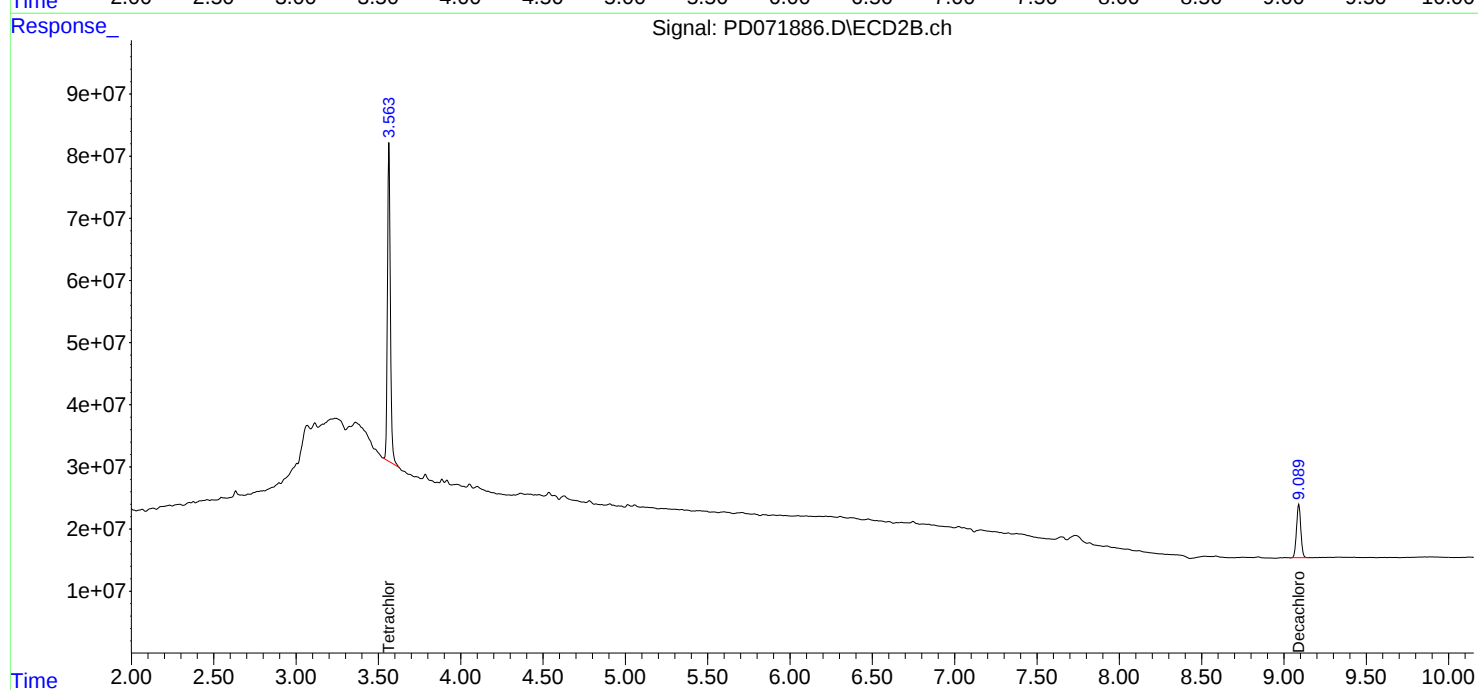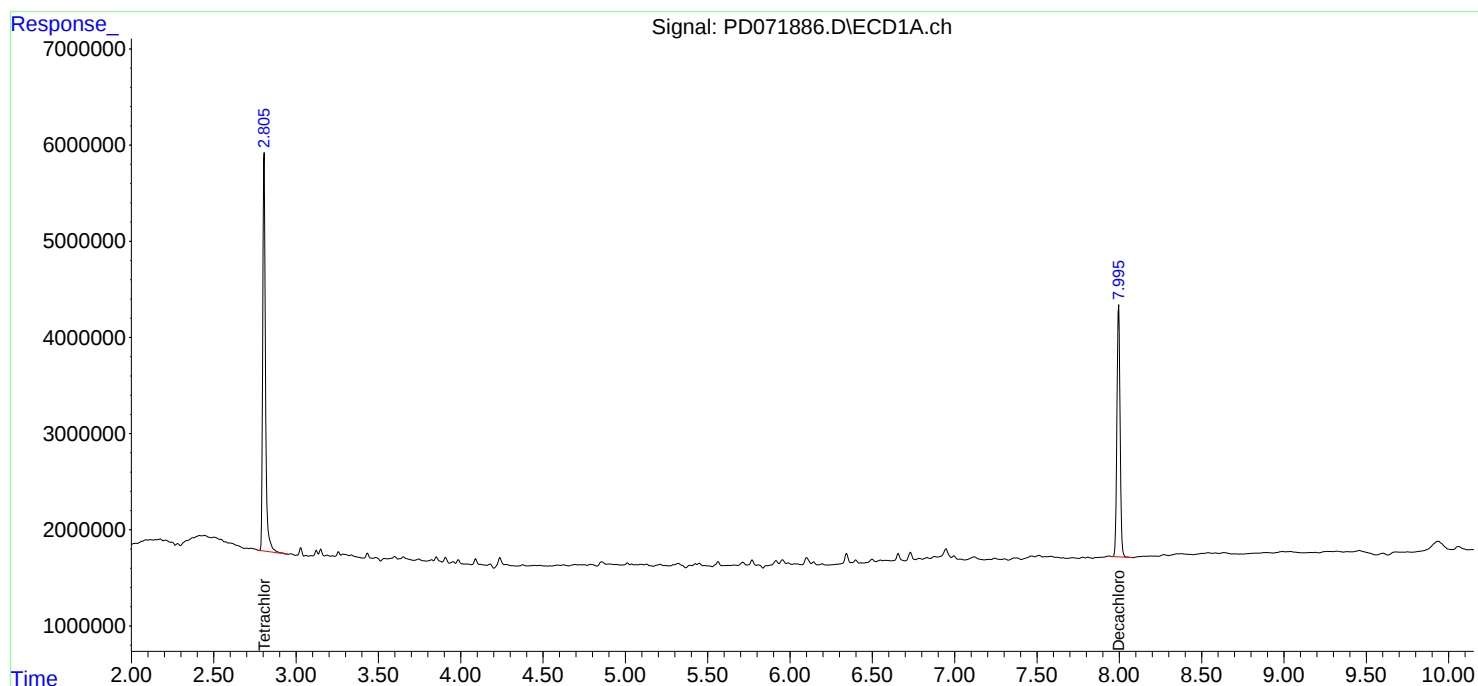


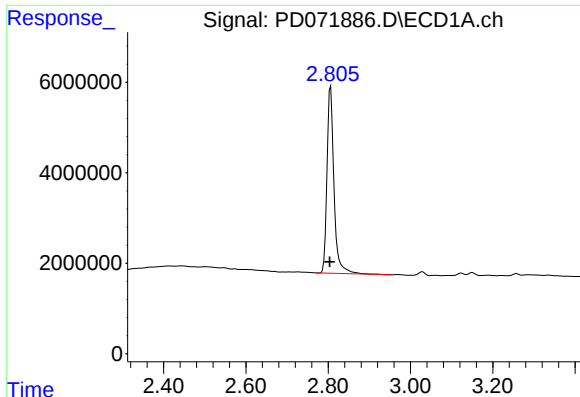

#1 Tetrachloro-m-xylene


R.T.: 2.806 min
Delta R.T.: 0.002 min
Response: 48682280
Conc: 19.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHERRY-HILL-COMP-10

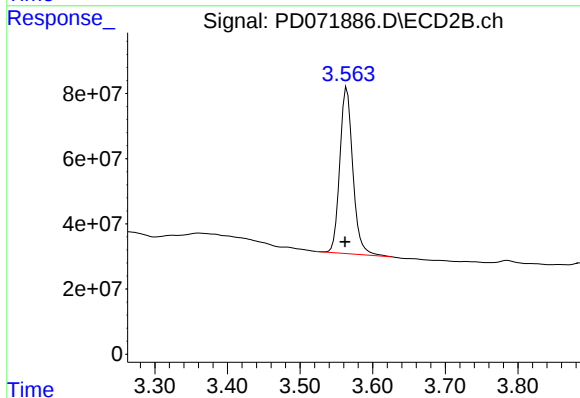


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 633586660
Conc: 22.08 ng/ml

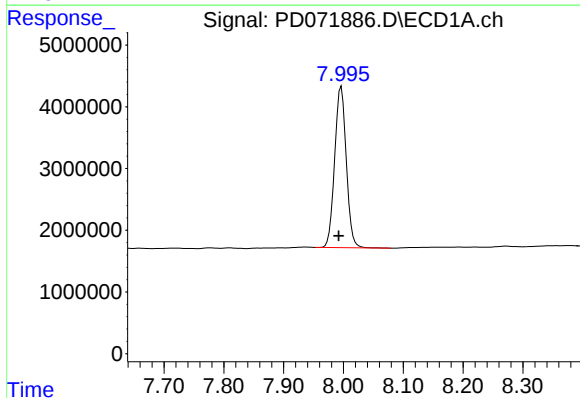

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.004 min
Response: 35301896
Conc: 14.01 ng/ml

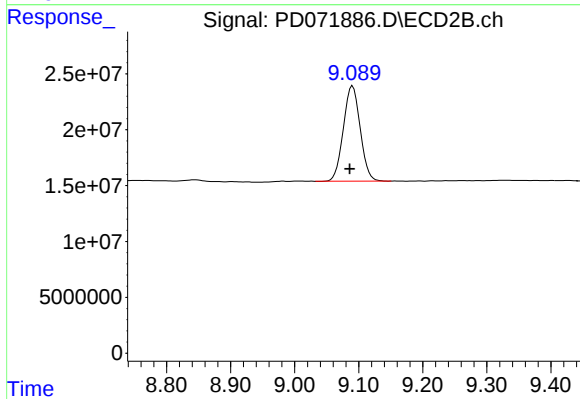

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.004 min
Response: 155826390
Conc: 16.76 ng/ml