

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091523\
 Data File : PD077977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 18:38
 Operator : AR\AJ
 Sample : 04380-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:30:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	48726788	30256510	19.201	20.473
27)	SA Decachlor...	9.081	7.898	64486504	34500502	20.643	21.303
Target Compounds							
3)	MA gamma-BHC...	0.000	3.592	0	4253600	N.D.	1.970
4)	MA Heptachlor	0.000	3.929	0	769123	N.D.	0.346
5)	MB Aldrin	5.276	4.225	13418690	357948	3.214	0.160 #
6)	B beta-BHC	0.000	3.929f	0	769123	N.D.	0.778
7)	B delta-BHC	0.000	4.125	0	843768	N.D.	0.379
8)	B Heptachlo...	0.000	4.775f	0	292441	N.D.	0.139
14)	MA Endrin	0.000	5.640	0	231062	N.D.	0.126
19)	B Endosulfa...	0.000	6.368f	0	198573	N.D.	0.120
20)	A Methoxychlor	0.000	6.599	0	352192	N.D.	0.451
23)	Toxaphene-2	0.000	5.640	0	231062	N.D.	19.161
25)	Toxaphene-4	0.000	6.599	0	352192	N.D.	9.126


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091523\
Data File : PD077977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 18:38
Operator : AR\AJ
Sample : 04380-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:30:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

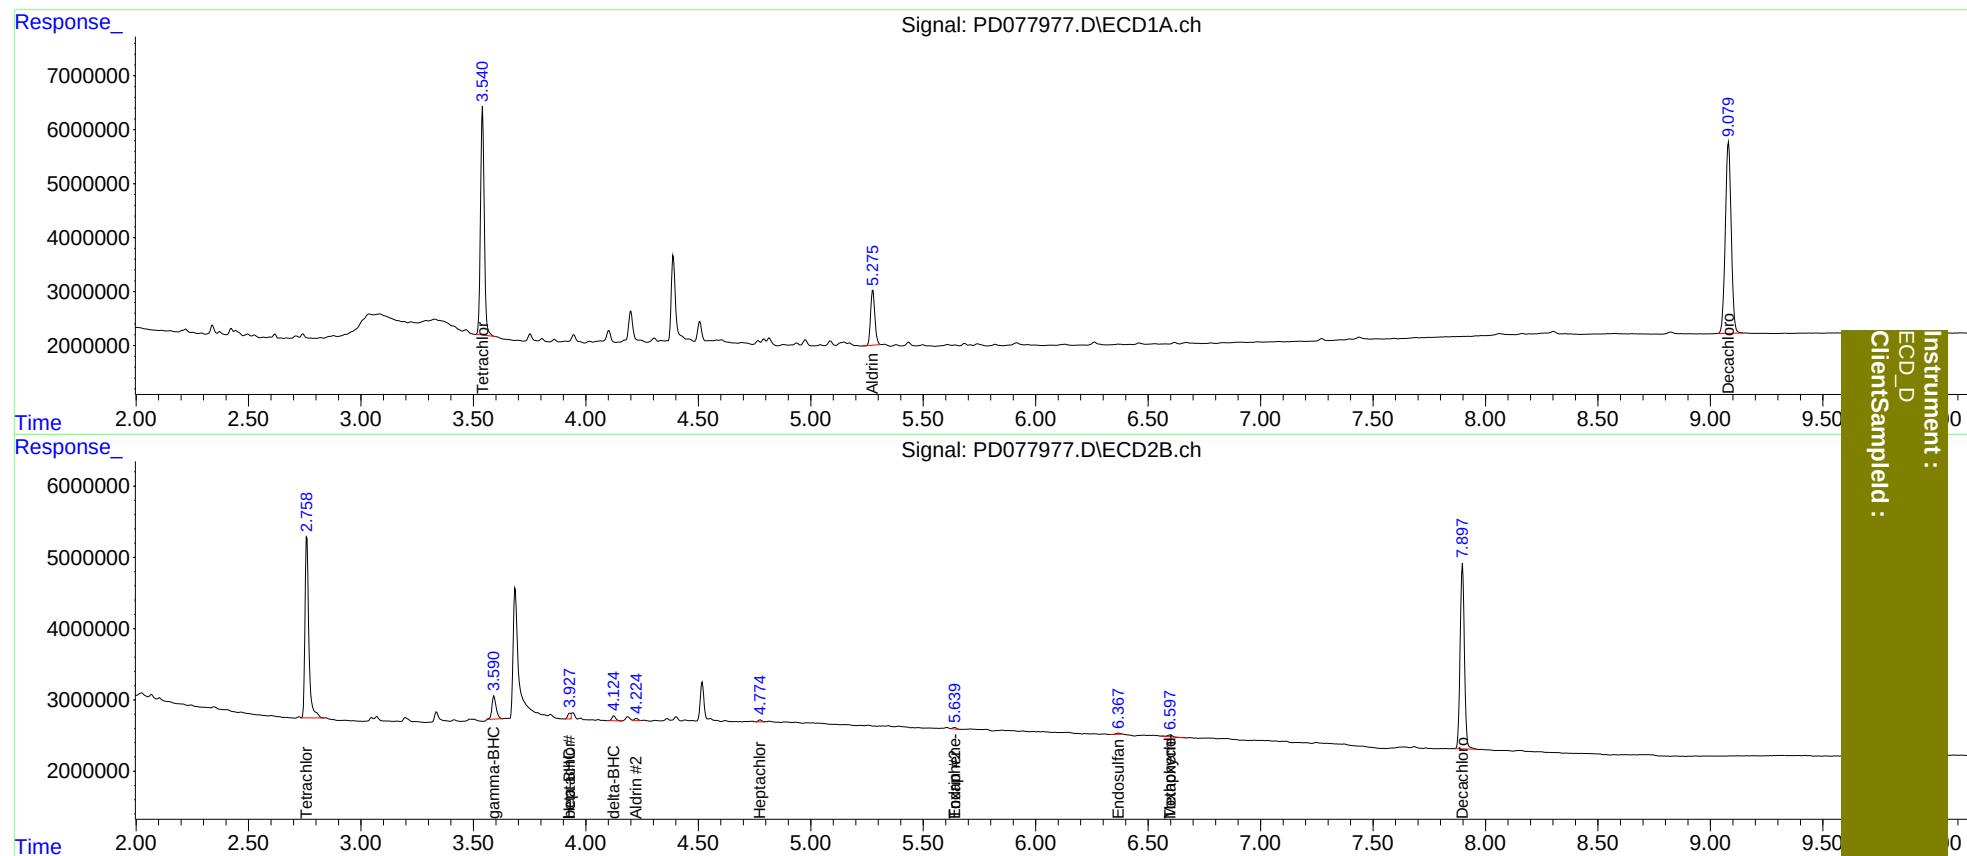


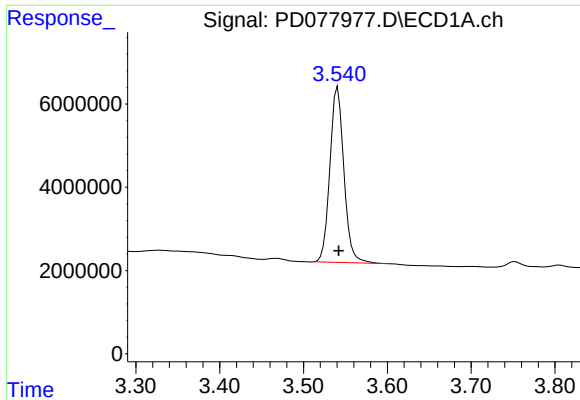

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.001 min
Response: 48726788
Conc: 19.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

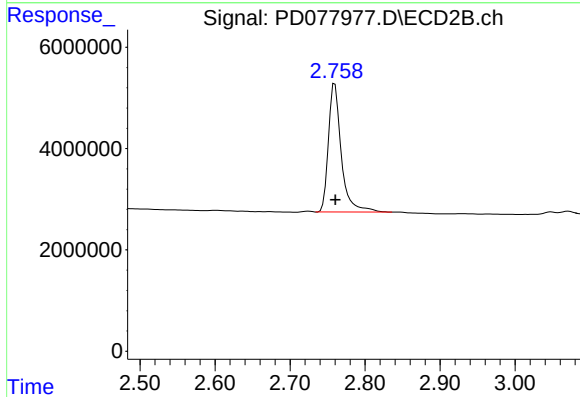


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 30256510
Conc: 20.47 ng/ml

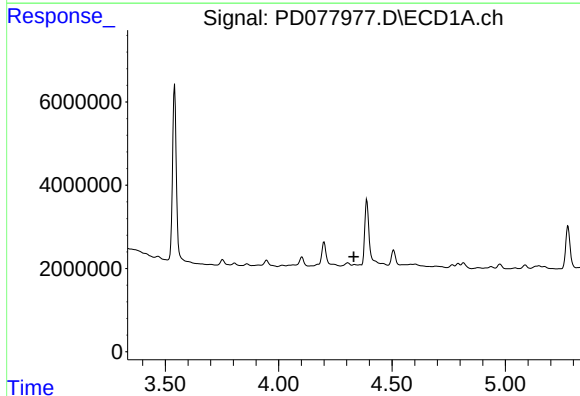


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.332 min
Response: 0
Conc: N.D.

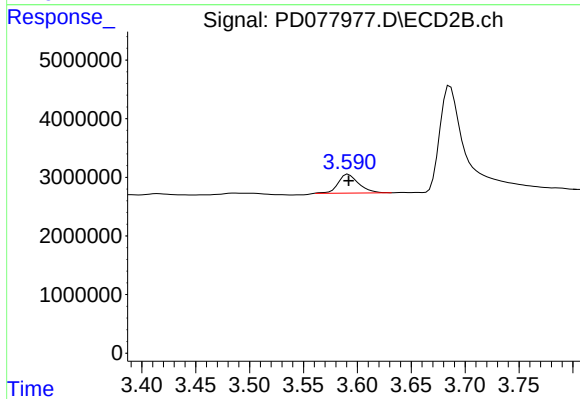

#3 gamma-BHC (Lindane)


R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 4253600
Conc: 1.97 ng/ml

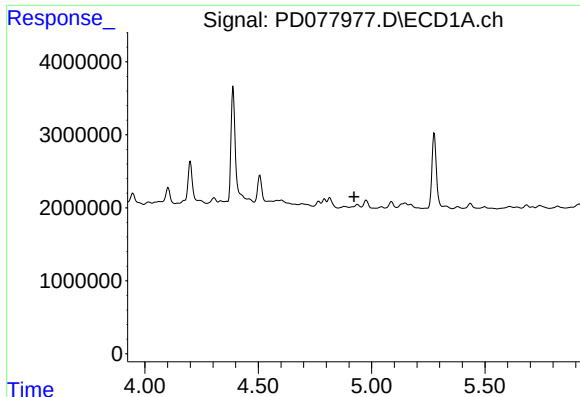

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.923 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

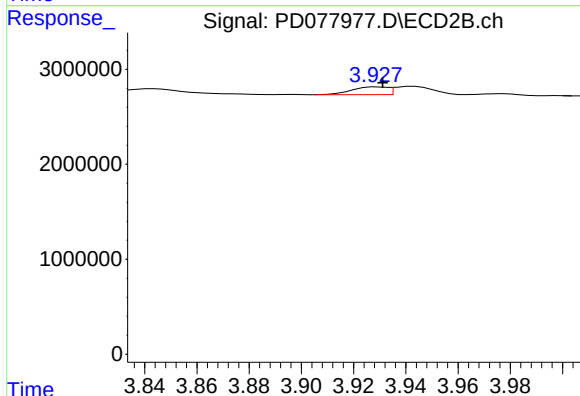


#4 Heptachlor

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 769123
Conc: 0.35 ng/ml

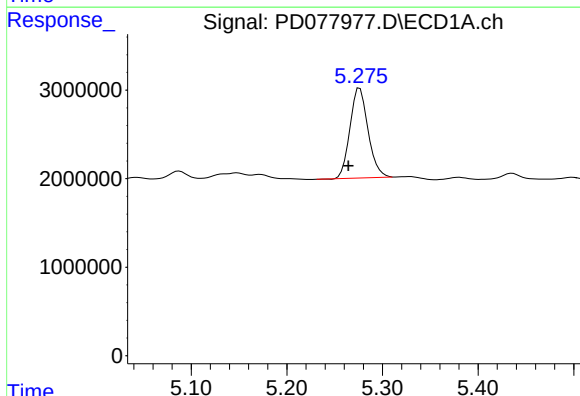


#5 Aldrin

R.T.: 5.276 min
Delta R.T.: 0.012 min
Response: 13418690
Conc: 3.21 ng/ml

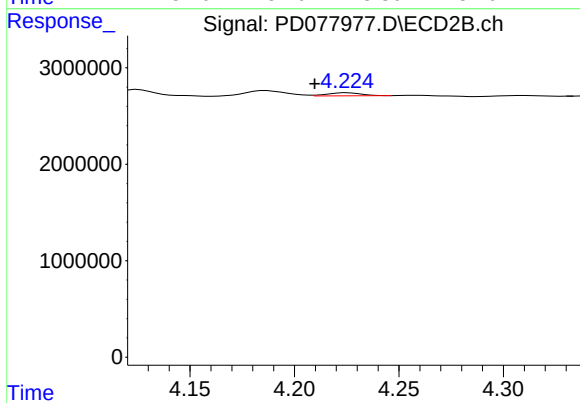

#5 Aldrin


R.T.: 4.225 min
Delta R.T.: 0.016 min
Response: 357948
Conc: 0.16 ng/ml

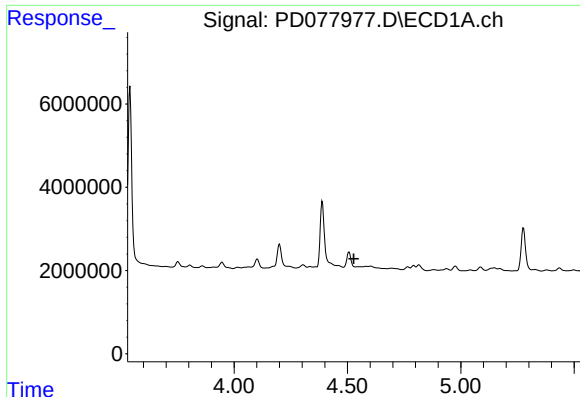

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

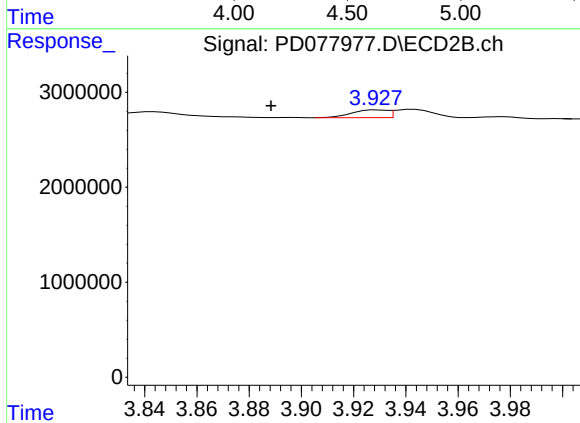


#6 beta-BHC

R.T.: 3.929 min
Delta R.T.: 0.041 min
Response: 769123
Conc: 0.78 ng/ml

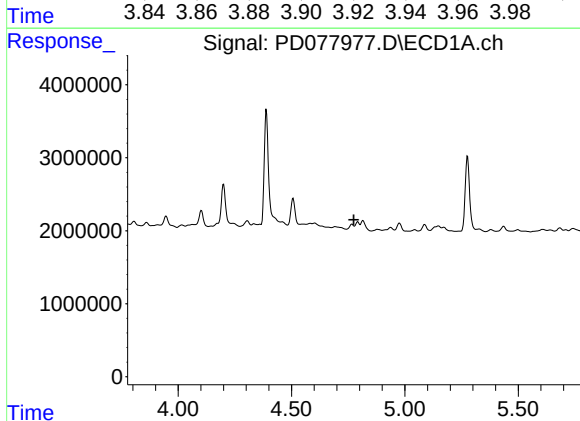


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.775 min
Response: 0
Conc: N.D.

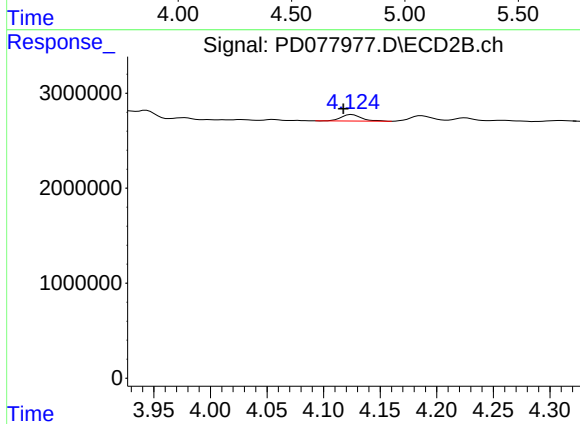

#7 delta-BHC


R.T.: 4.125 min
Delta R.T.: 0.008 min
Response: 843768
Conc: 0.38 ng/ml

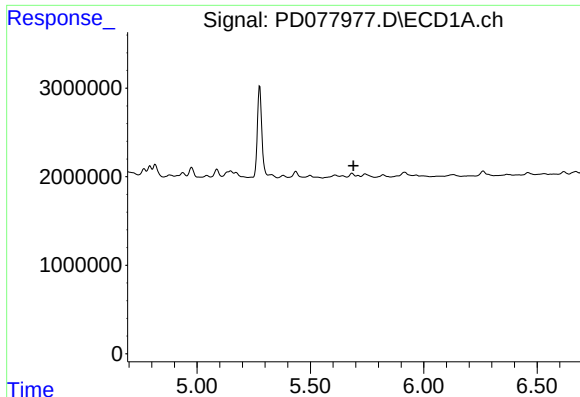

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.690 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

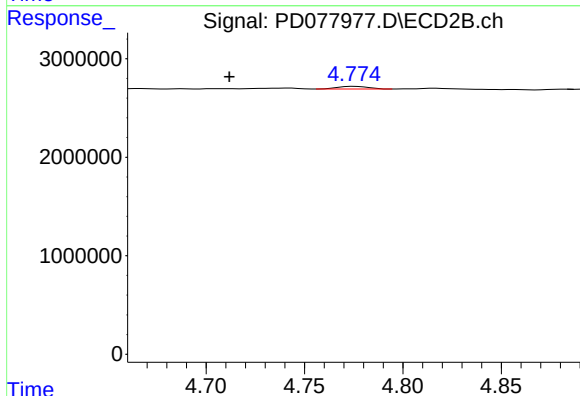


#8 Heptachlor epoxide

R.T.: 4.775 min
Delta R.T.: 0.063 min
Response: 292441
Conc: 0.14 ng/ml

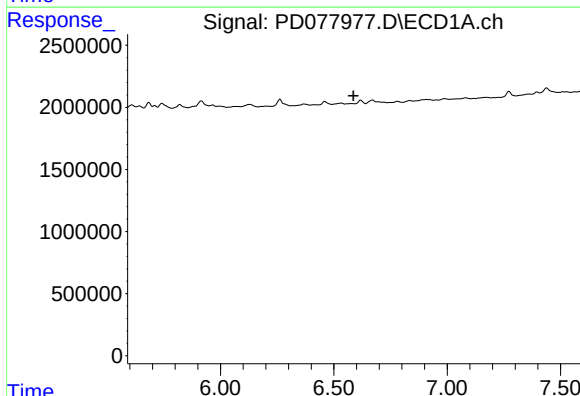


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

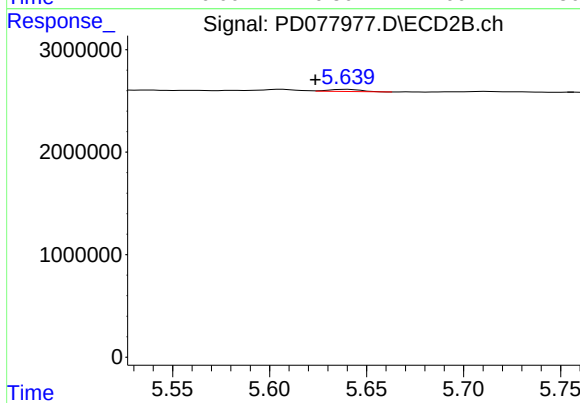

#14 Endrin


R.T.: 5.640 min
Delta R.T.: 0.017 min
Response: 231062
Conc: 0.13 ng/ml

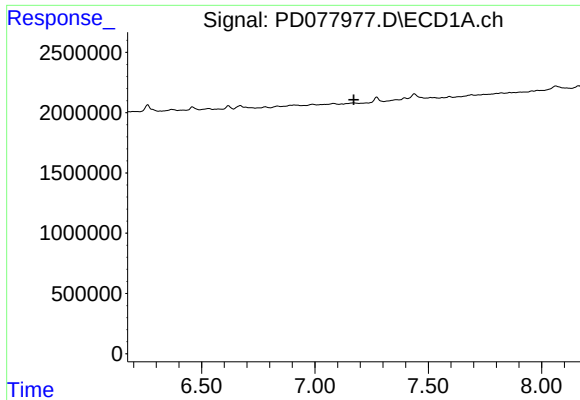

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

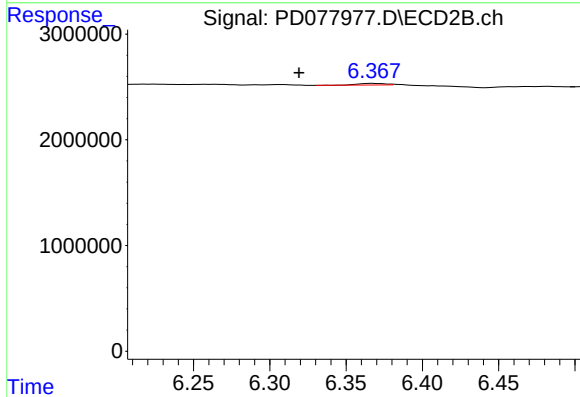


#19 Endosulfan Sulfate

R.T.: 6.368 min
Delta R.T.: 0.049 min
Response: 198573
Conc: 0.12 ng/ml

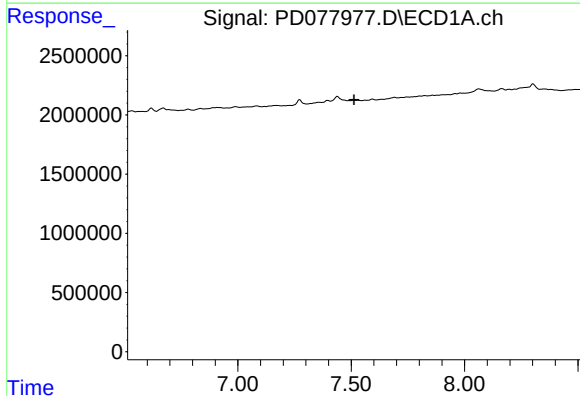


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.513 min
Response: 0
Conc: N.D.

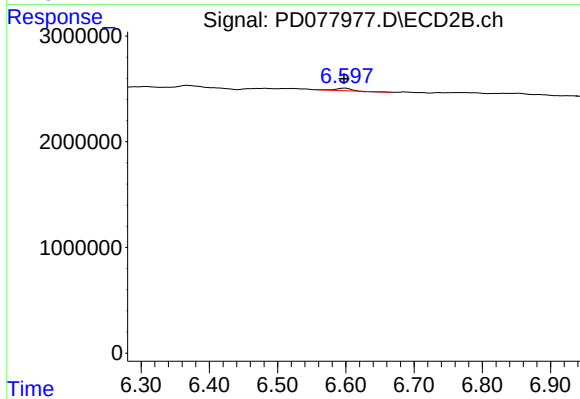

#20 Methoxychlor


R.T.: 6.599 min
Delta R.T.: 0.001 min
Response: 352192
Conc: 0.45 ng/ml

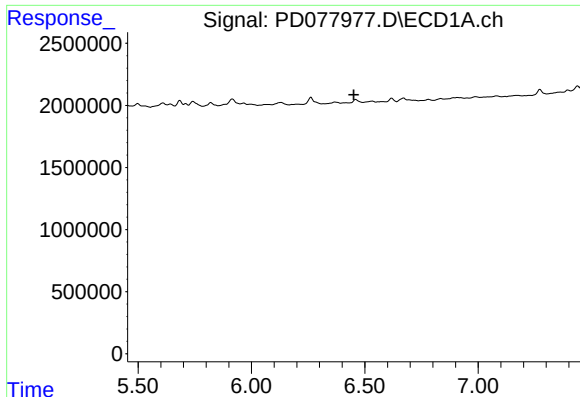

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

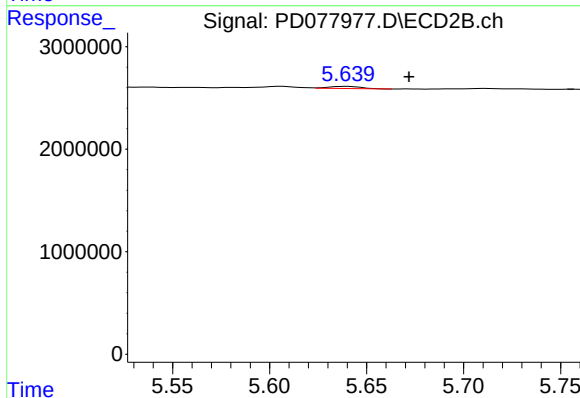


#23 Toxaphene-2

R.T.: 5.640 min
Delta R.T.: -0.032 min
Response: 231062
Conc: 19.16 ng/ml

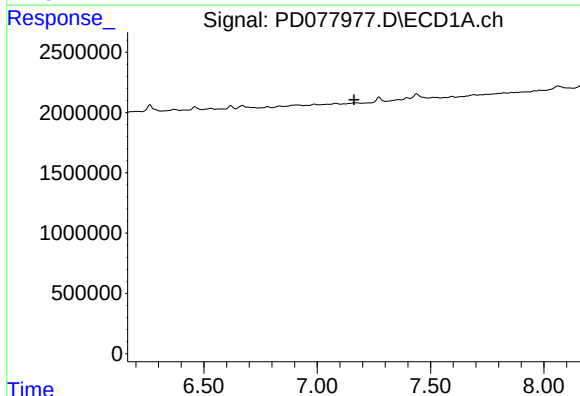


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.163 min
Response: 0
Conc: N.D.

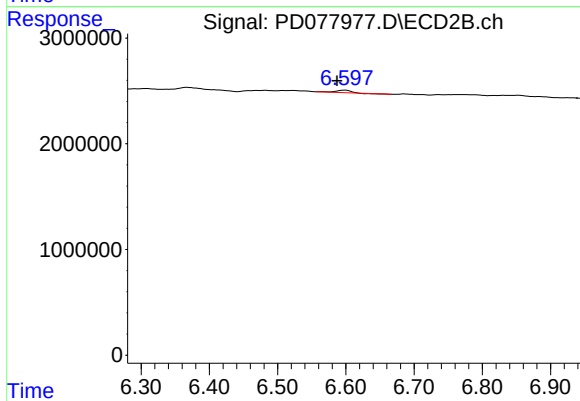

#25 Toxaphene-4


R.T.: 6.599 min
Delta R.T.: 0.012 min
Response: 352192
Conc: 9.13 ng/ml

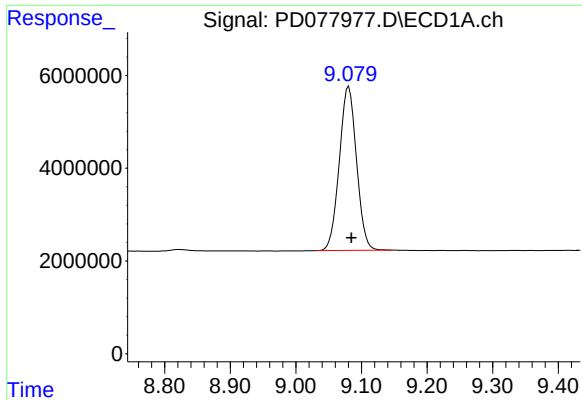

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.004 min
Response: 64486504
Conc: 20.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

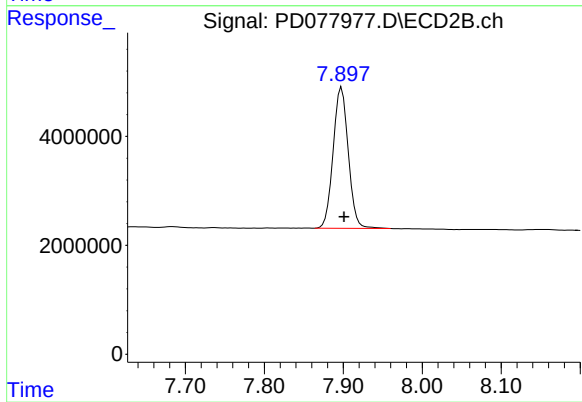

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 34500502
Conc: 21.30 ng/ml