

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091523\
 Data File : PD077963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 11:19
 Operator : AR\AJ
 Sample : 04344-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBHL8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/15/2023
 Supervised By : Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:27:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.759	40630193	27346204	16.011	18.504
2) SA Decachlor...	9.082	7.898	48423587	26106528	15.501	16.120
Target Compounds						
11) B cis-Chlor...	6.017	5.033	1812222	2456399	0.470m	1.201m#
16) A 4,4'-DDD	6.693	5.763	3926245	2421442	1.476m	1.799
17) MA 4,4'-DDT	7.065	6.031	4251122	2852089	1.552	2.018 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091523\
Data File : PD077963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 11:19
Operator : AR\AJ
Sample : 04344-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:27:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

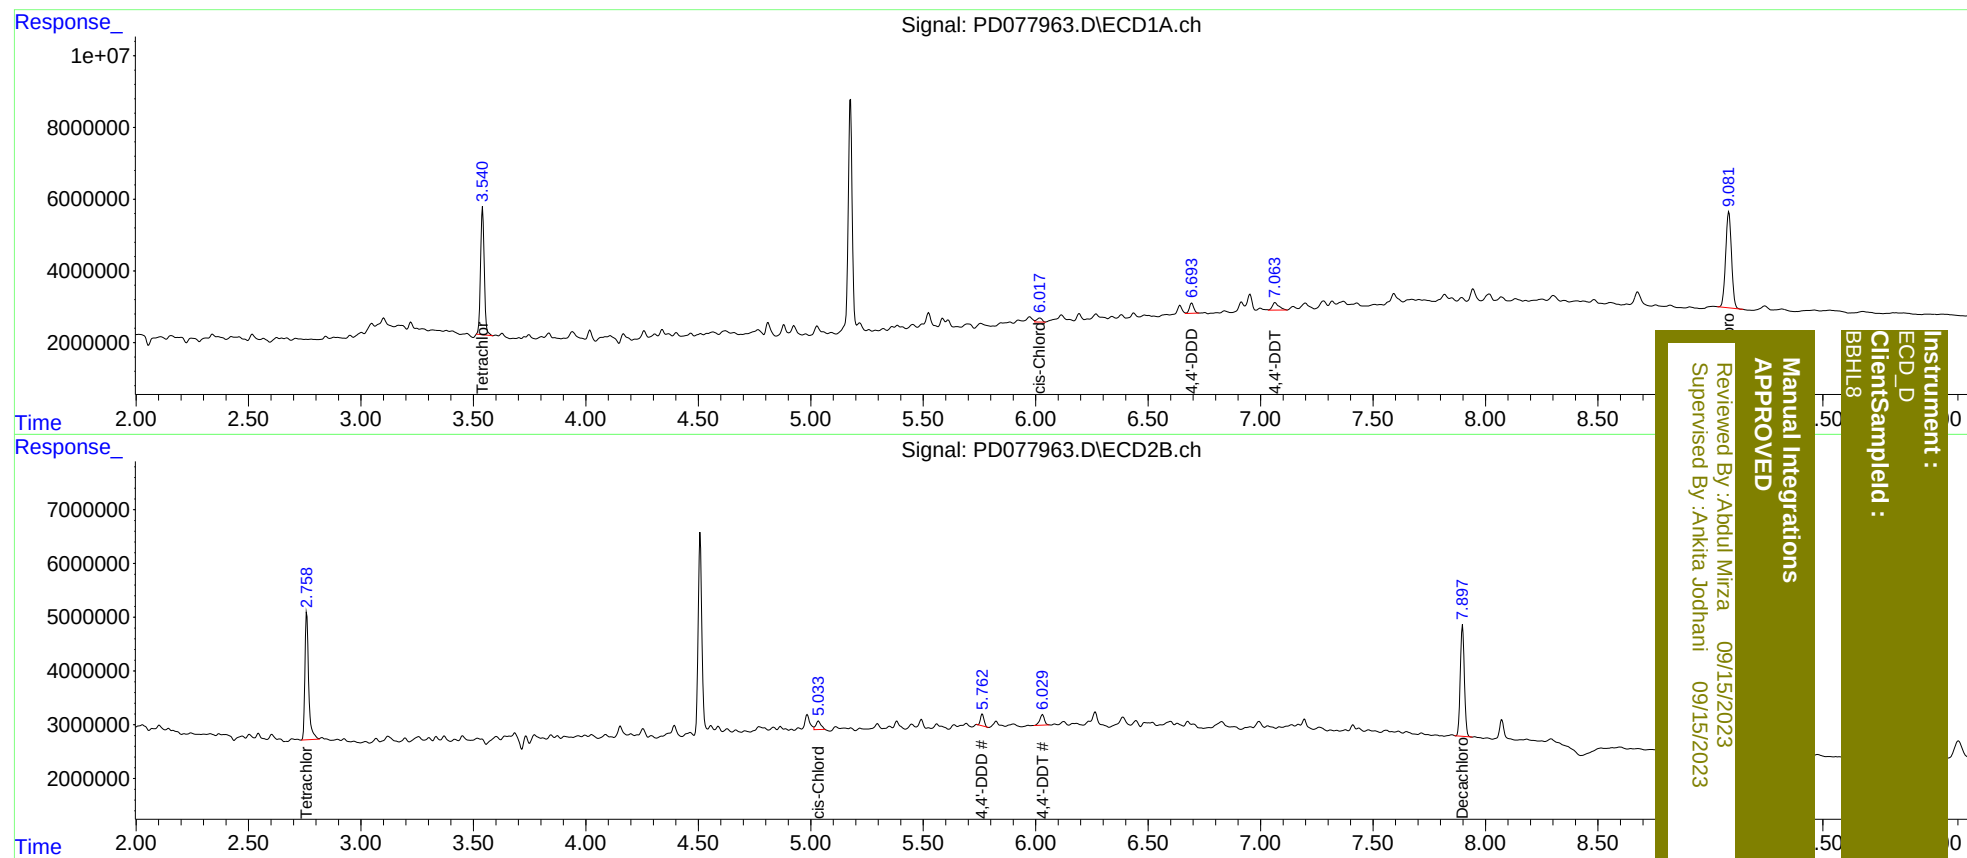

Instrument :
ECD_D
ClientSampled :
BBHL8

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023