

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091523\
 Data File : PD077994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 23:05
 Operator : AR\AJ
 Sample : 04380-22MS
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH4P4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/15/2023
 Supervised By : Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:35:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	56384346	34544164	22.219	23.374
27)	SA Decachlor...	9.081	7.897	65463707	34967679	20.956	21.591
Target Compounds							
2)	A alpha-BHC	3.998	3.261	115.7E6	67825035	27.028	29.922
3)	MA gamma-BHC...	4.331	3.591	107.6E6	71680268	26.613	33.199
4)	MA Heptachlor	4.921	3.929	106.7E6	62023377	25.535	27.897
5)	MB Aldrin	5.265	4.209	115.8E6	56848395	27.744	25.363
6)	B beta-BHC	4.528	3.886	43435438	23739404	23.643	24.026m
7)	B delta-BHC	4.777	4.117	108.7E6	60062227	27.070	26.946
8)	B Heptachlo...	5.692	4.711	100.8E6	56759909	26.085	27.023
9)	A Endosulfan I	6.078	5.081	95291585	54440981	28.388	30.330
10)	B trans-Chl...	5.948	4.961	95000801	54428488	25.515	27.256
11)	B cis-Chlor...	6.028	5.025	98428209	55980598	25.539	27.374
12)	B 4,4'-DDE	6.200	5.213	180.6E6	103.9E6	50.944	54.674
13)	MA Dieldrin	6.354	5.345	205.5E6	118.7E6	54.907	57.466
14)	MA Endrin	6.585	5.621	168.1E6	103.8E6	54.471	56.763
15)	B Endosulfa...	6.805	5.915	174.4E6	102.7E6	52.669	56.777
16)	A 4,4'-DDD	6.719	5.768	149.5E6	85261107	56.213	63.346
17)	MA 4,4'-DDT	7.034	6.019	151.6E6	84064358	55.335	59.479
18)	B Endrin al...	6.935	6.095	128.9E6	75040191	49.586	53.347
19)	B Endosulfa...	7.170	6.318	160.7E6	93876435	53.018	56.817
20)	A Methoxychlor	7.510	6.595	416.3E6	239.6E6	266.900	307.065
21)	B Endrin ke...	7.657	6.824	181.8E6	112.4E6	52.811	58.681

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091523\
Data File : PD077994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 23:05
Operator : AR\AJ
Sample : 04380-22MS
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:35:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

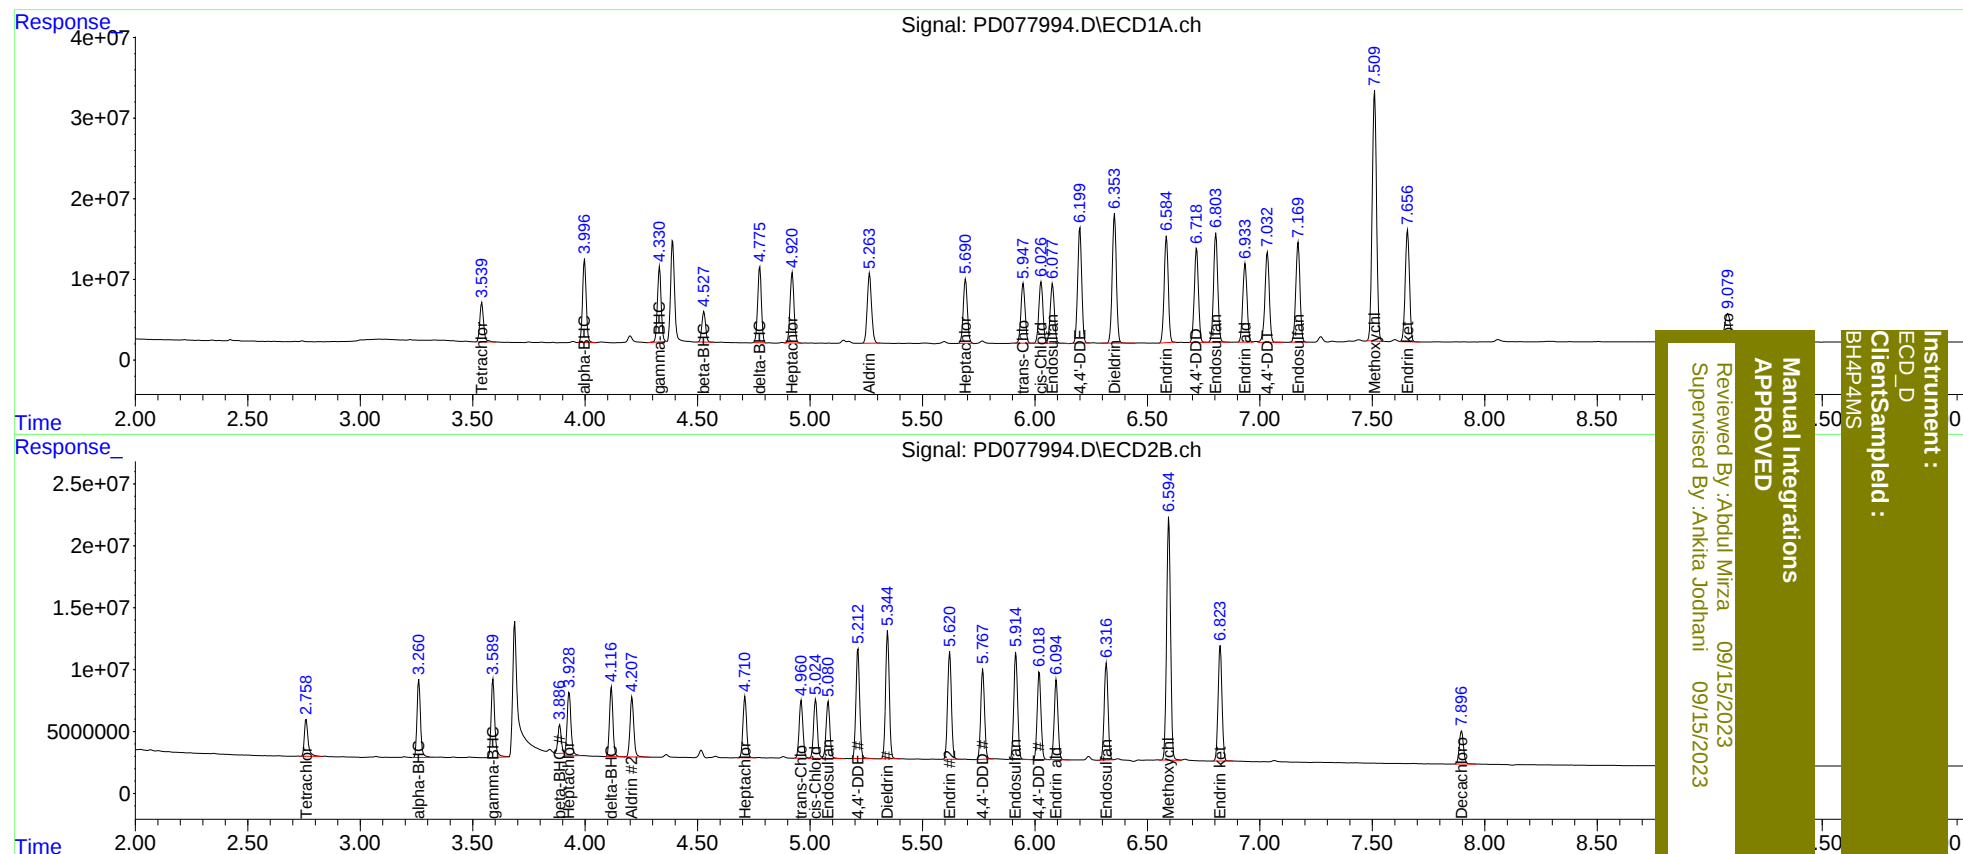

Instrument :
ECD_D
ClientSampled :
BH4P4MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023