

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091524\
 Data File : PD085191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2024 08:05
 Operator : AR\AJ
 Sample : P3934-03MSD 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHMK7MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/16/2024
 Supervised By :Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:43:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 03:41:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.902	18614459	73940981	19.501	21.905m
27) SA Decachlor...	9.030	8.101	26113589	69726596	21.675	21.024
Target Compounds						
2) A alpha-BHC	3.982	3.414	96482669	282.5E6	56.784	55.615
3) MA gamma-BHC...	4.309	3.748	110.4E6	271.2E6	68.649m	56.430
4) MA Heptachlor	4.908	4.101	85297408	238.7E6	56.398	56.901m
5) MB Aldrin	5.249	4.389	83571354	235.0E6	53.517	53.899
6) B beta-BHC	4.493	4.040	34860941	112.1E6	50.015	52.713m
7) B delta-BHC	4.741	4.280	89404545	270.4E6	54.502	55.260
8) B Heptachlo...	5.667	4.893	76265087	220.7E6	53.263	53.613
9) A Endosulfan I	6.050	5.267	72427700	206.7E6	54.740	54.199m
10) B trans-Chl...	5.922	5.145	74549865	228.9E6	54.798	57.067m
11) B cis-Chlor...	6.003	5.209	77087278	229.5E6	54.396	56.528m
12) B 4,4'-DDE	6.172	5.396	140.7E6	433.8E6	113.782	112.916
13) MA Dieldrin	6.322	5.535	159.5E6	466.8E6	110.865	110.654
14) MA Endrin	6.547	5.813	137.6E6	434.7E6	124.937m	119.315
15) B Endosulfa...	6.760	6.104	134.0E6	410.4E6	106.536	116.004m
16) A 4,4'-DDD	6.679	5.951	111.9E6	389.9E6	118.272	118.219m
17) MA 4,4'-DDT	6.994	6.207	107.7E6	367.8E6	121.146m	116.032m
18) B Endrin al...	6.888	6.282	96856808	304.6E6	116.200	114.240m
19) B Endosulfa...	7.122	6.507	125.4E6	390.9E6	114.332	113.867m
20) A Methoxychlor	7.466	6.778	291.5E6	869.4E6	570.377	545.272m
21) B Endrin ke...	7.602	7.018	137.2E6	461.9E6	117.765	109.360

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091524\
Data File : PD085191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2024 08:05
Operator : AR\AJ
Sample : P3934-03MSD 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:43:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 03:41:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

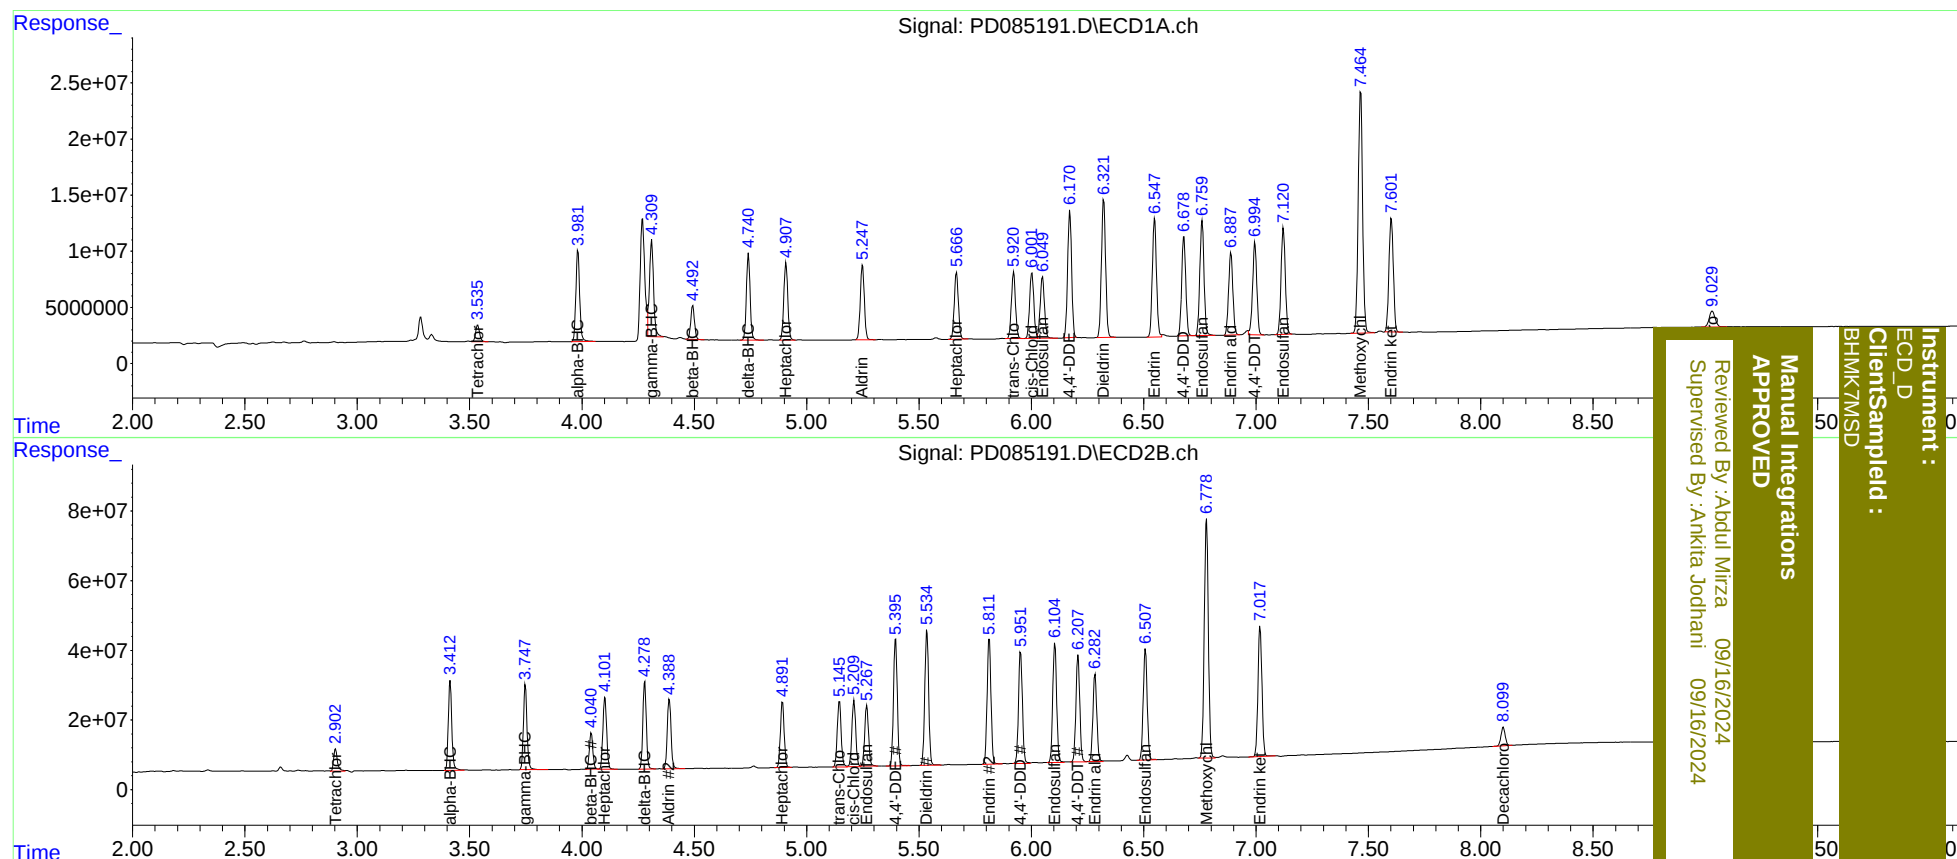

Instrument :
ECD_D
Client Sampled :
BHMK7MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/16/2024
Supervised By: Ankita Jodhani 09/16/2024