

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091619\
 Data File : PD054611.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 00:53
 Operator : SG\AJ
 Sample : K4810-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AL8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 05:59:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 05:19:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.967	0	3457280	N.D.	3.568
27)	SA Decachlor...	7.977	9.004	6346749	4923343	5.817	4.396
Target Compounds							
10)	B trans-Chl...	0.000	6.047	0	4939808	N.D.	3.596


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091619\
Data File : PD054611.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 00:53
Operator : SG\AJ
Sample : K4810-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AL8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 05:59:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 05:19:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

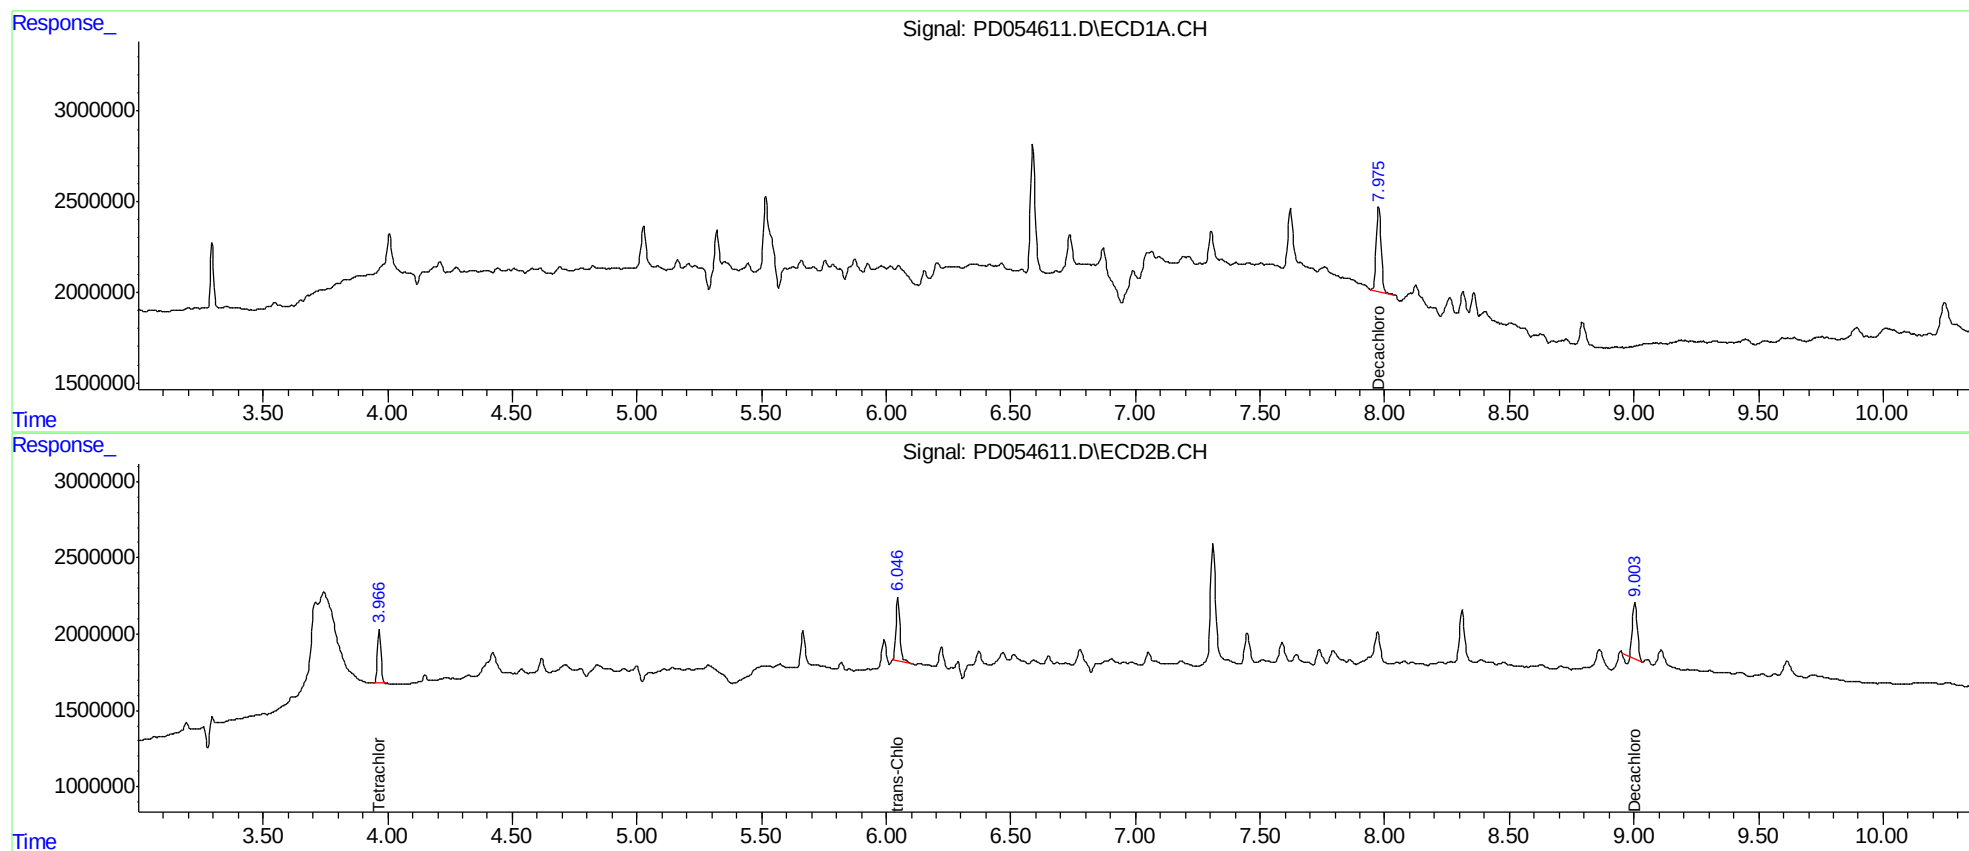


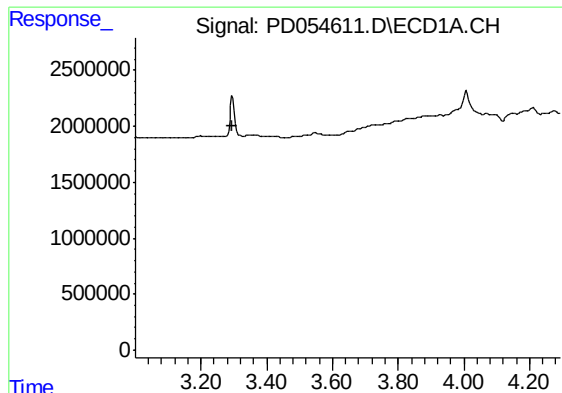

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AL8

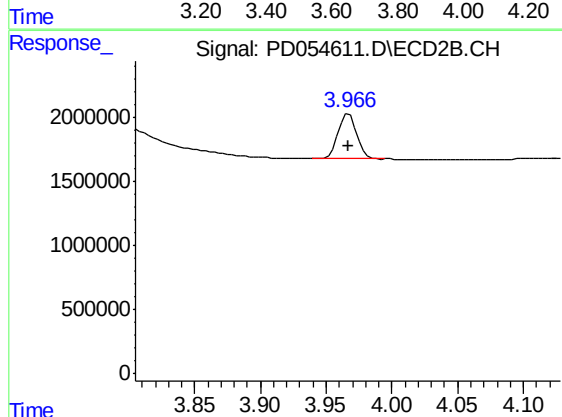


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 3457280
Conc: 3.57 ng/ml

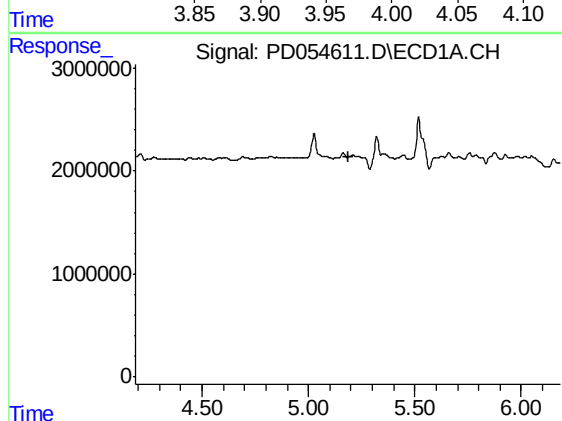


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

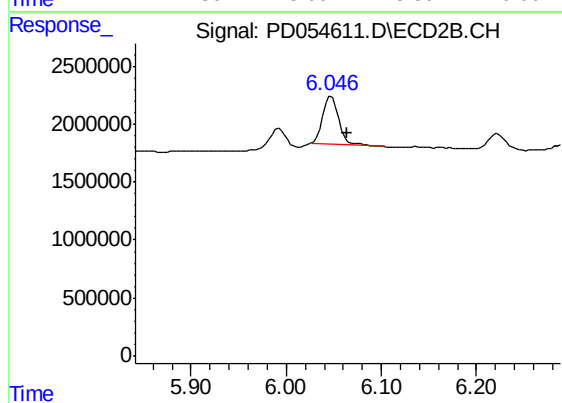

#10 trans-Chlordane


R.T.: 6.047 min
Delta R.T.: -0.016 min
Response: 4939808
Conc: 3.60 ng/ml

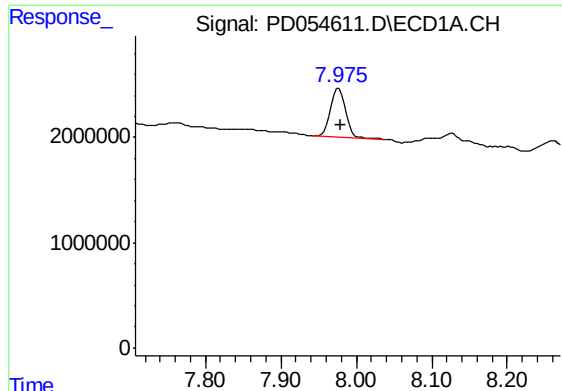

#27 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 6346749
Conc: 5.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AL8

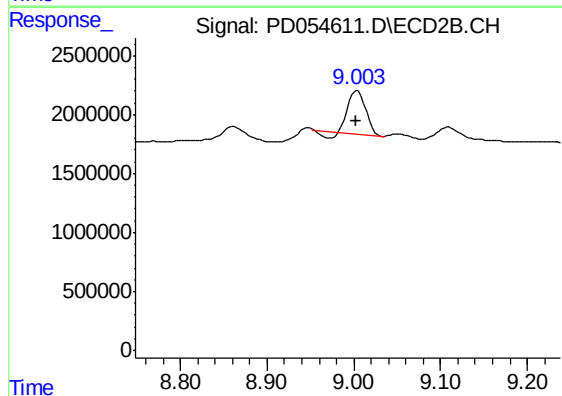

#27 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.000 min
Response: 4923343
Conc: 4.40 ng/ml