

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091619\
 Data File : PD054614.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 1:35
 Operator : SG\AJ
 Sample : K4810-22
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AM2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 06:00:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 05:19:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.296	3.967	7582816	8362350	8.344	8.631
27)	SA Decachlor...	7.977	9.002	12859530	13130229	11.785	11.723
Target Compounds							
10)	B trans-Chl...	0.000	6.047	0	2986099	N.D.	2.174


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091619\
Data File : PD054614.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 1:35
Operator : SG\AJ
Sample : K4810-22
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AM2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 06:00:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 05:19:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

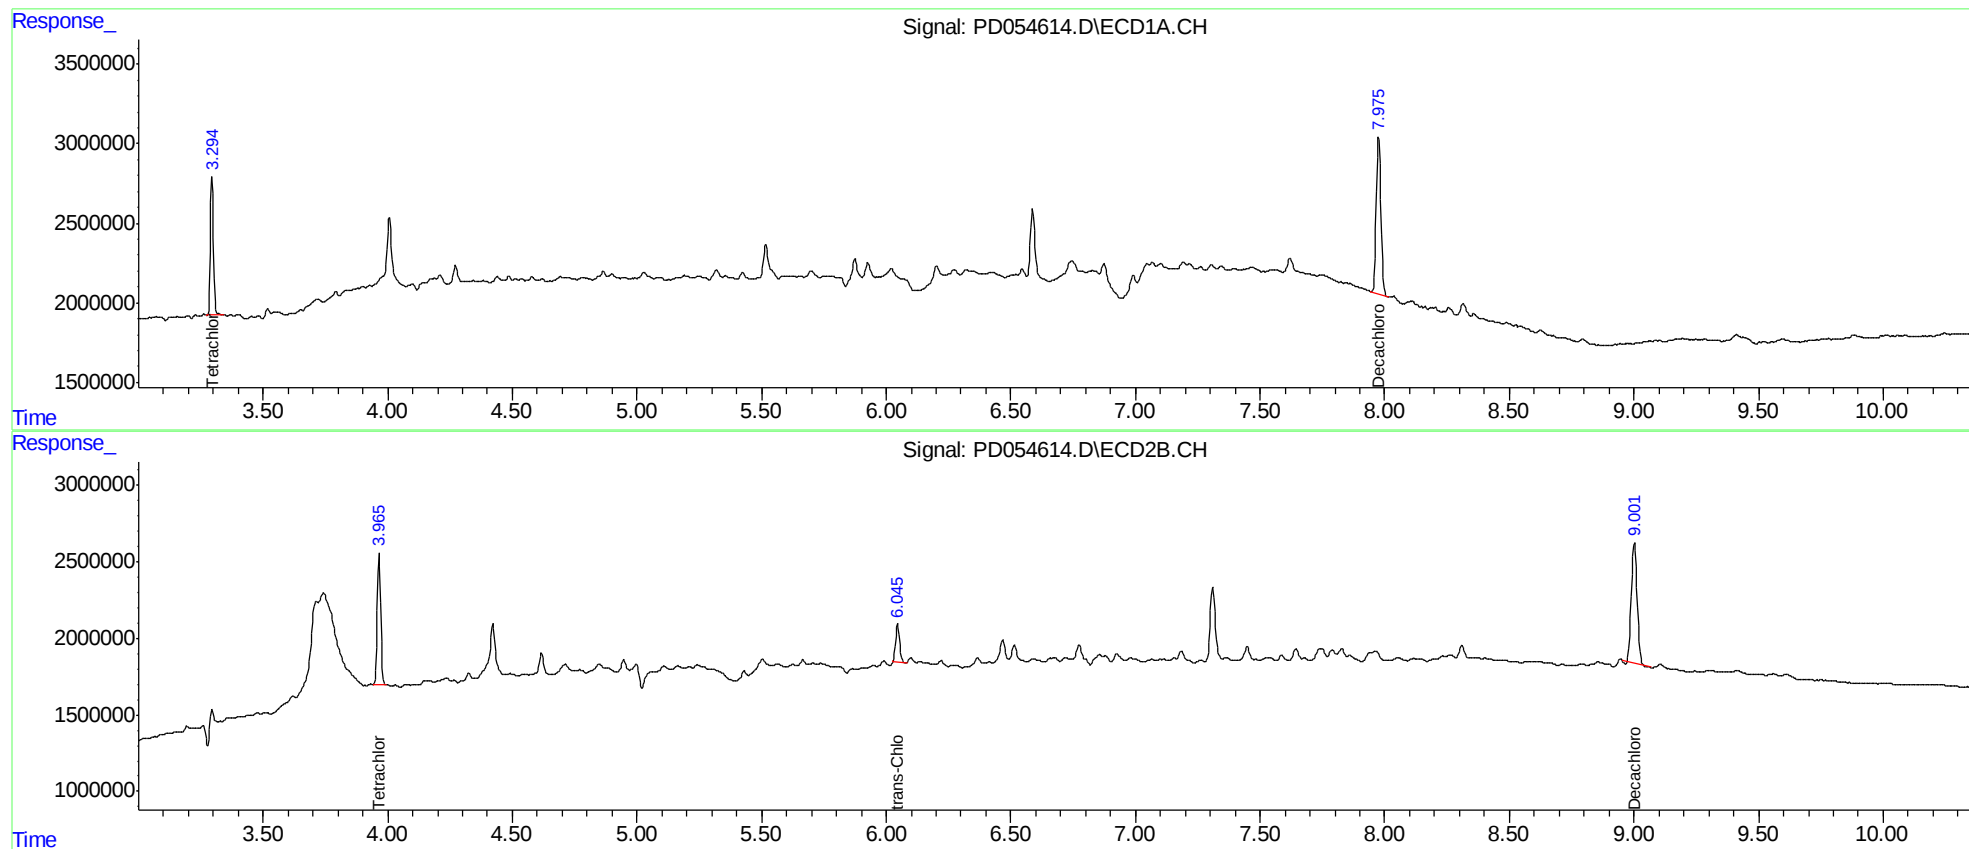


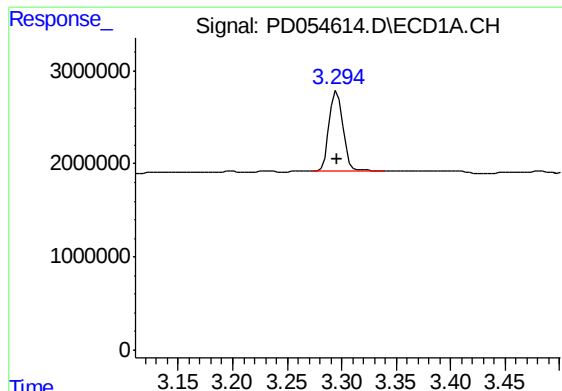

#1 Tetrachloro-m-xylene


R.T.: 3.296 min
Delta R.T.: 0.000 min
Response: 7582816
Conc: 8.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AM2

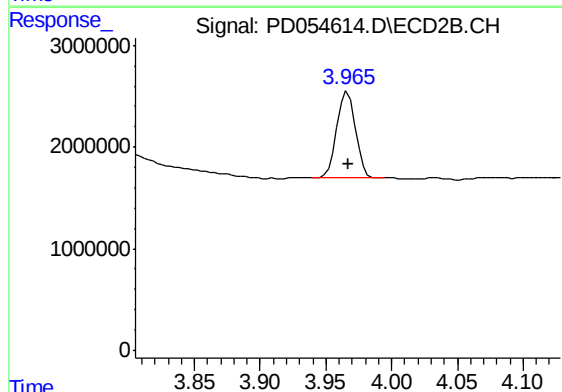


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 8362350
Conc: 8.63 ng/ml

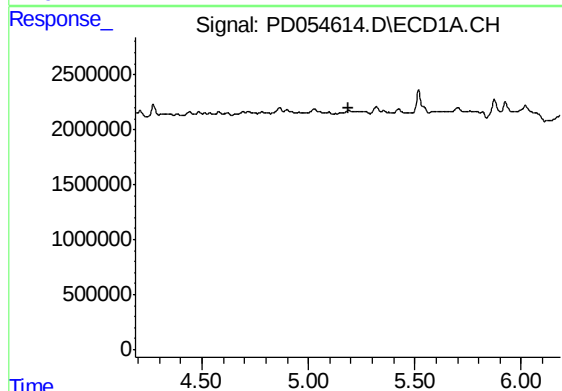


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

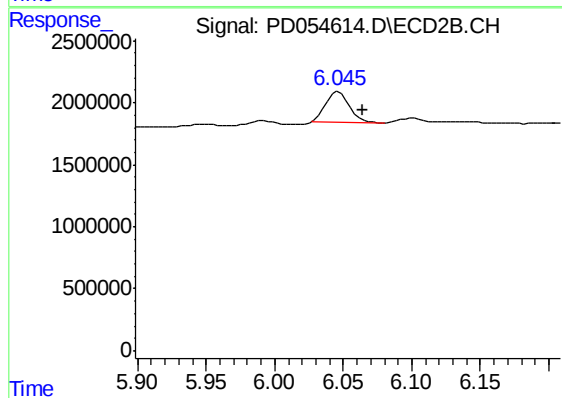

#10 trans-Chlordane


R.T.: 6.047 min
Delta R.T.: -0.017 min
Response: 2986099
Conc: 2.17 ng/ml

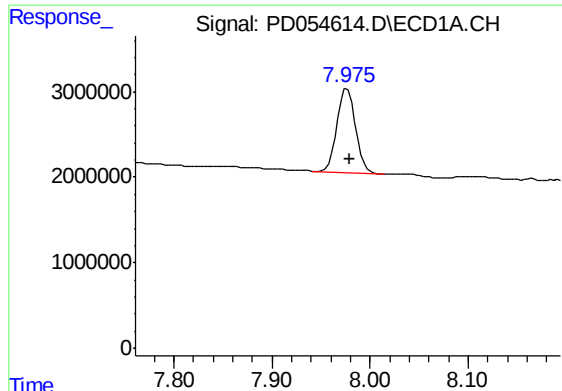

#27 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 12859530
Conc: 11.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AM2

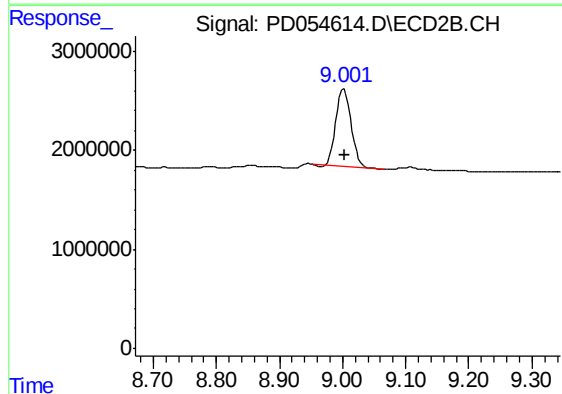

#27 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: -0.001 min
Response: 13130229
Conc: 11.72 ng/ml