

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091619\
 Data File : PD054629.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 5:05
 Operator : SG\AJ
 Sample : K4779-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AJ5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 06:03:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 05:19:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.296	3.967	10857132	11946820	11.947	12.331
27) SA Decachlor...	7.977	9.004	20390115	20809715	18.687	18.580
Target Compounds						
10) B trans-Chl...	0.000	6.047	0	3815714	N.D.	2.778


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091619\
Data File : PD054629.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 5:05
Operator : SG\AJ
Sample : K4779-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AJ5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 06:03:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 05:19:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

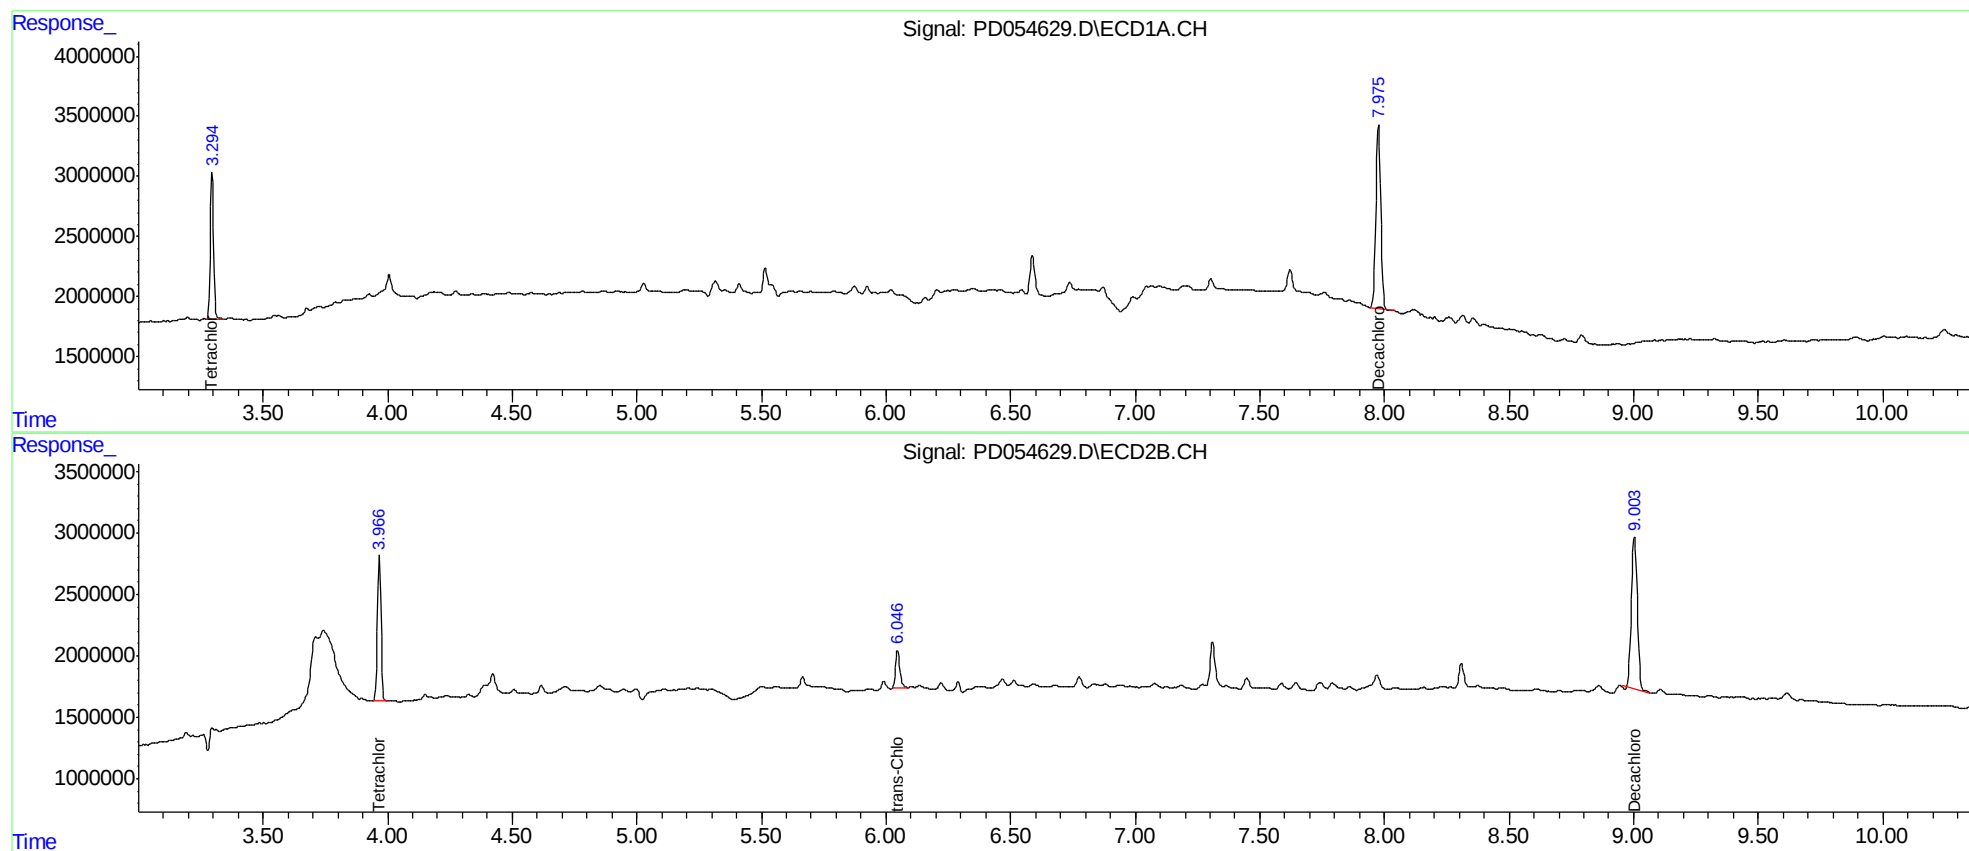


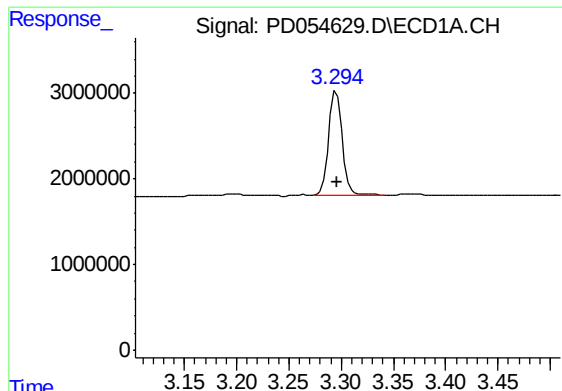

#1 Tetrachloro-m-xylene


R.T.: 3.296 min
Delta R.T.: 0.000 min
Response: 10857132
Conc: 11.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AJ5

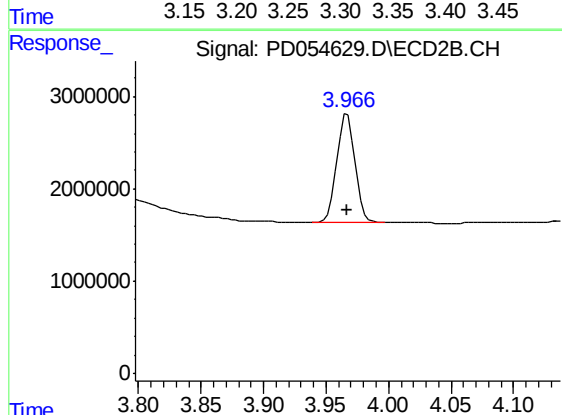


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 11946820
Conc: 12.33 ng/ml

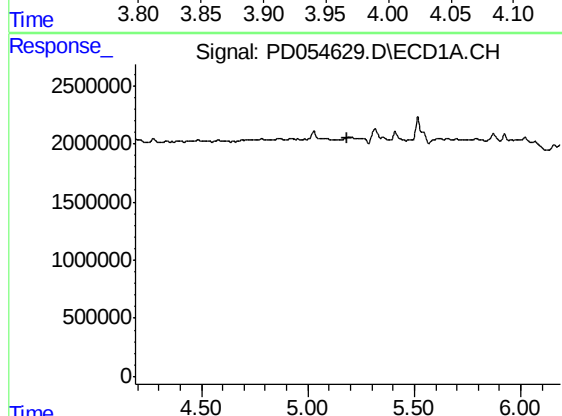


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

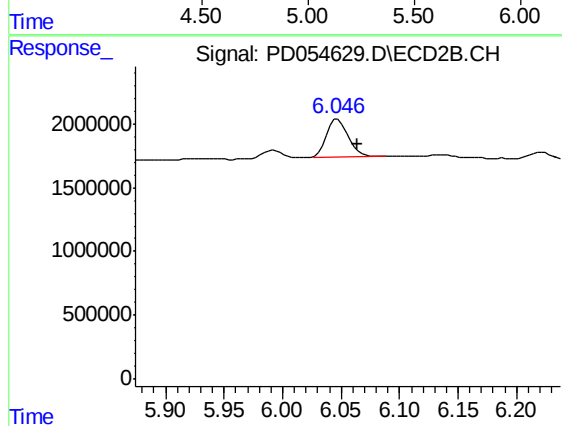

#10 trans-Chlordane


R.T.: 6.047 min
Delta R.T.: -0.017 min
Response: 3815714
Conc: 2.78 ng/ml

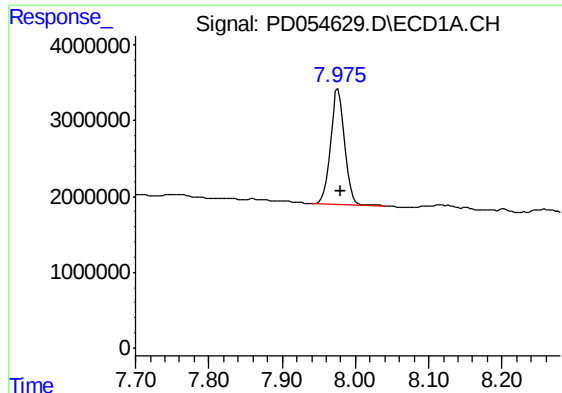

#27 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 20390115
Conc: 18.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AJ5

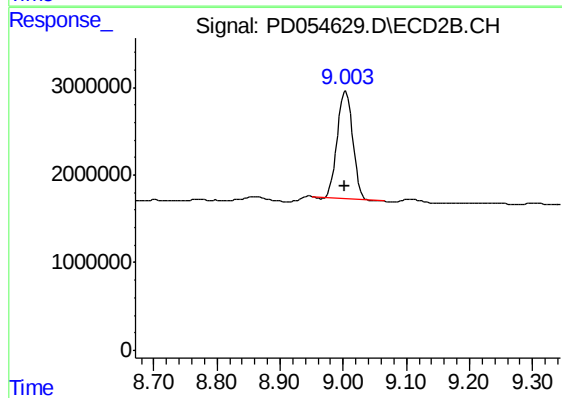

#27 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.001 min
Response: 20809715
Conc: 18.58 ng/ml