

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 19:08
 Operator : DD\AJ
 Sample : PCHLORIC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:30:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:28:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	4876166	8586700	4.723	4.914
28)	SA Decachlor...	7.837	8.858	5032766	8755874	5.253	5.653
Target Compounds							
23)	Chlordane-1	0.000	4.840	0	6702239	N.D.	95.594 #
24)	Chlordane-2	0.000	5.303	0	4584781	N.D.	67.651 #
25)	Chlordane-3	5.064	5.944	4867019	15170691	46.664	55.666
26)	Chlordane-4	5.119	6.017	4673498	16759774	46.622	51.369
27)	Chlordane-5	0.000	6.814	0	2653554	N.D.	45.021 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 19:08
Operator : DD\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:30:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:28:07 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

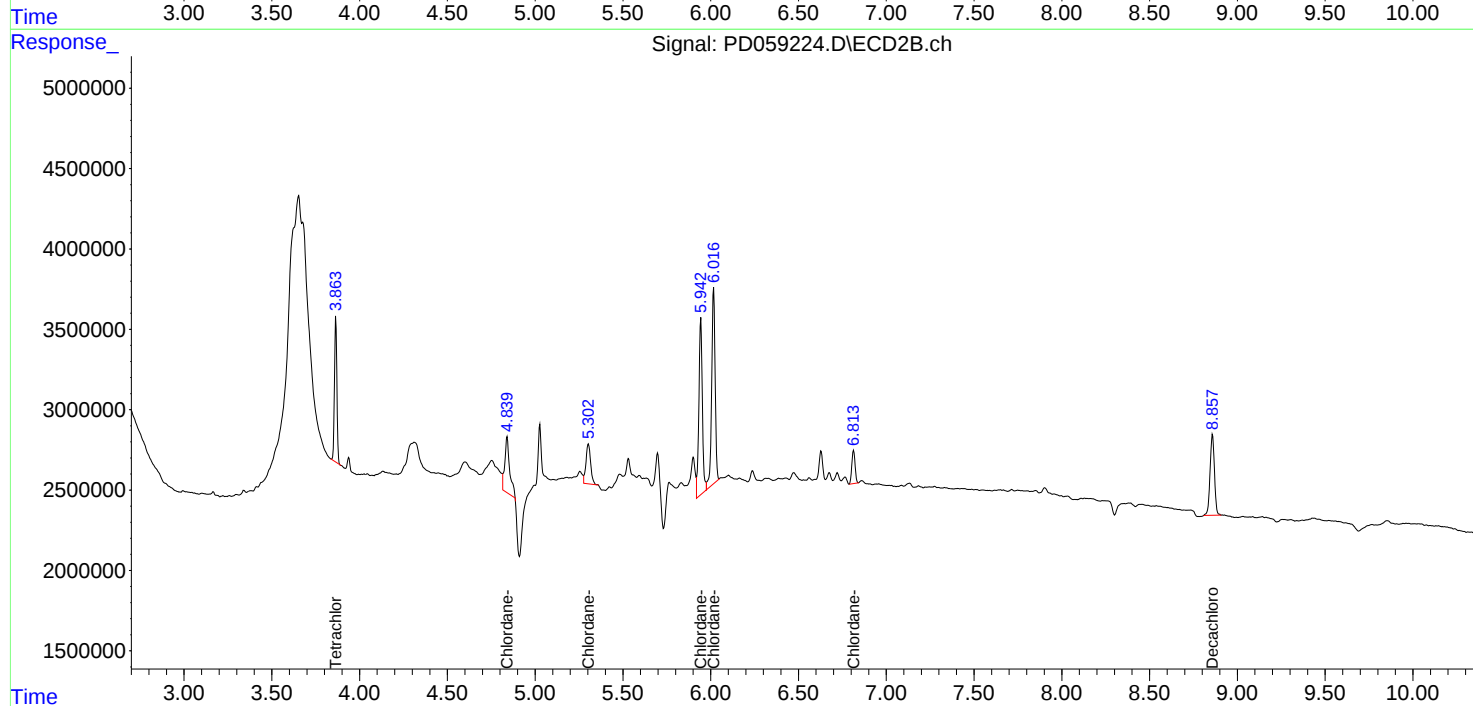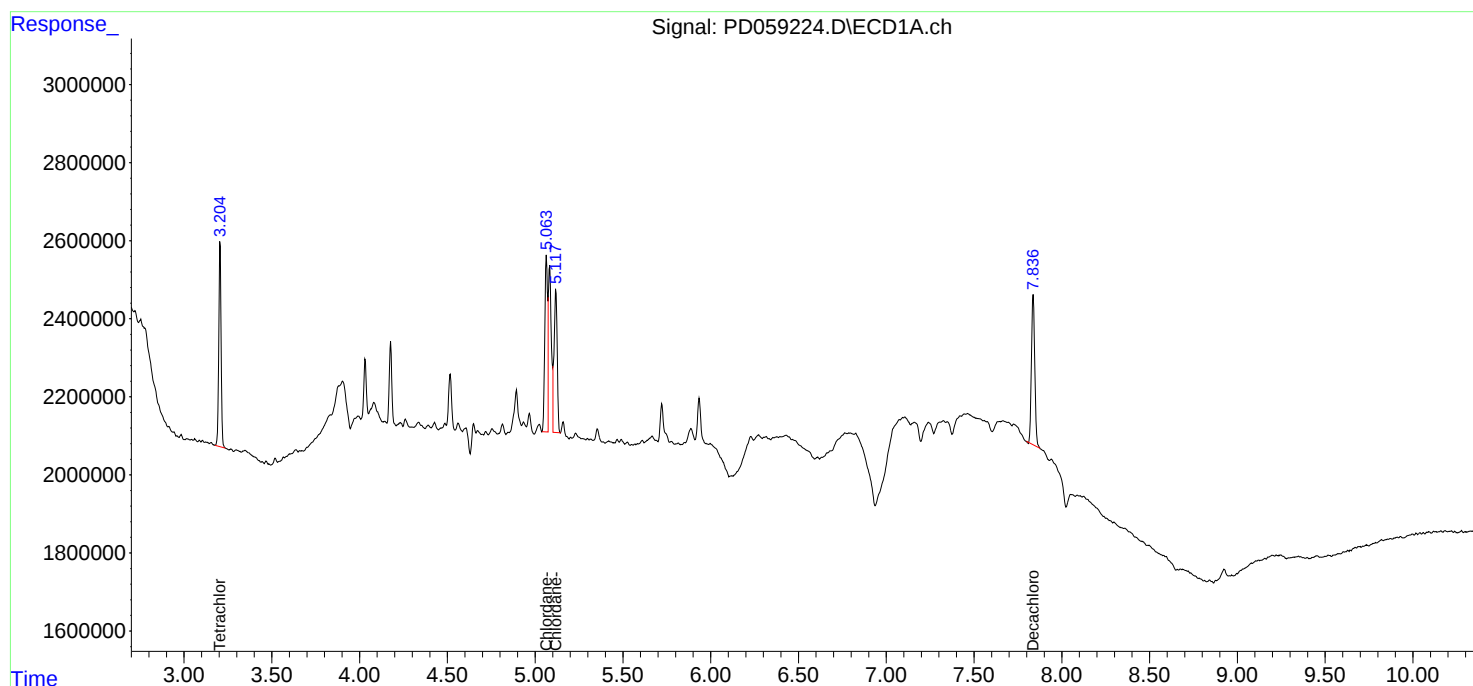

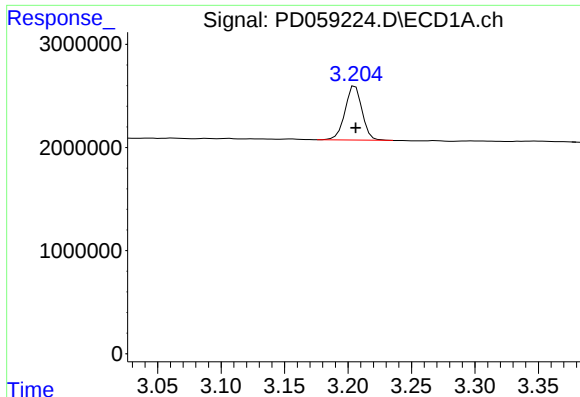


#1 Tetrachloro-m-xylene

R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 4876166
Conc: 4.72 ng/ml

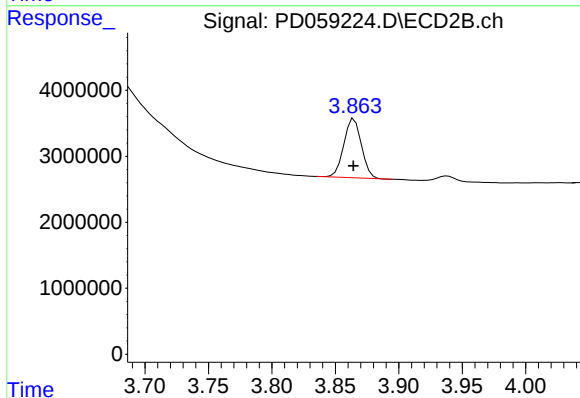


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 8586700
Conc: 4.91 ng/ml

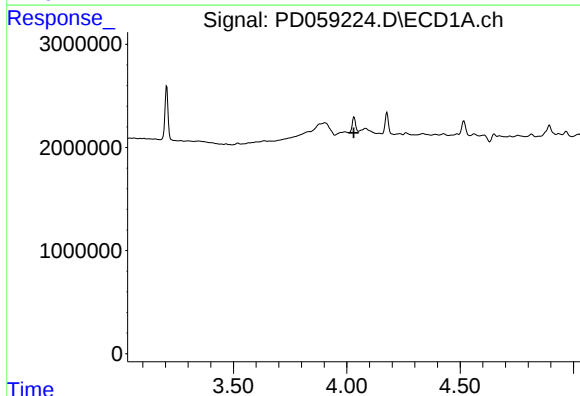


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.032 min
Response: 0
Conc: N.D.

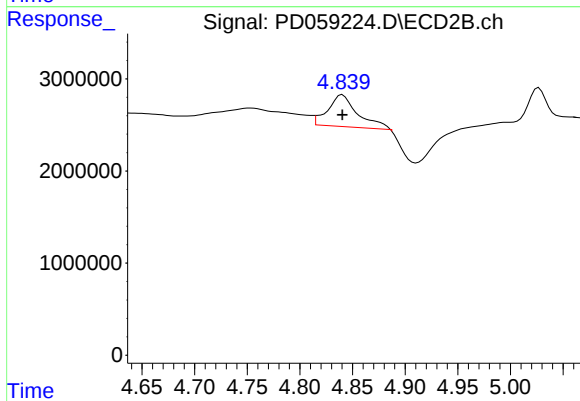


#23 Chlordane-1

R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 6702239
Conc: 95.59 ng/ml

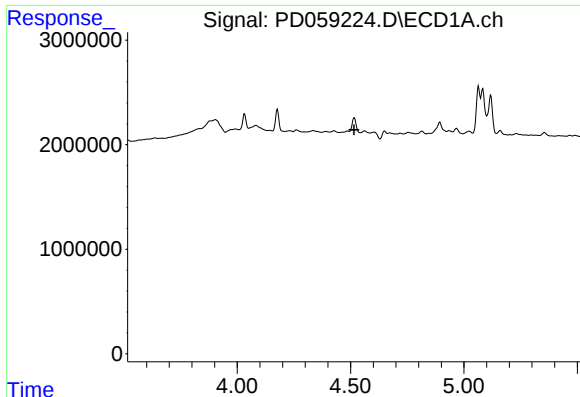


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.516 min
Response: 0
Conc: N.D.

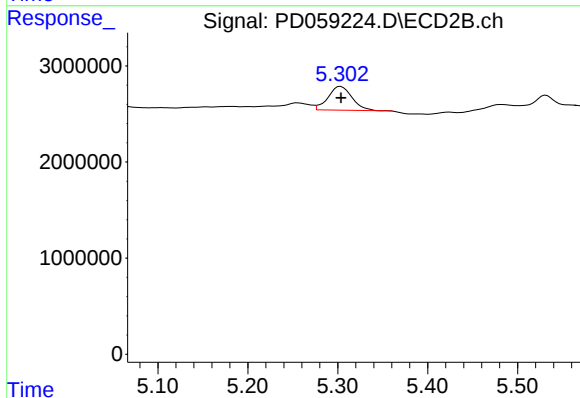


#24 Chlordane-2

R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 4584781
Conc: 67.65 ng/ml

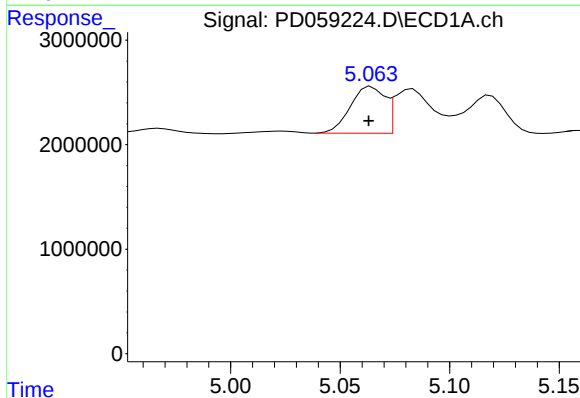


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.001 min
Response: 4867019
Conc: 46.66 ng/ml

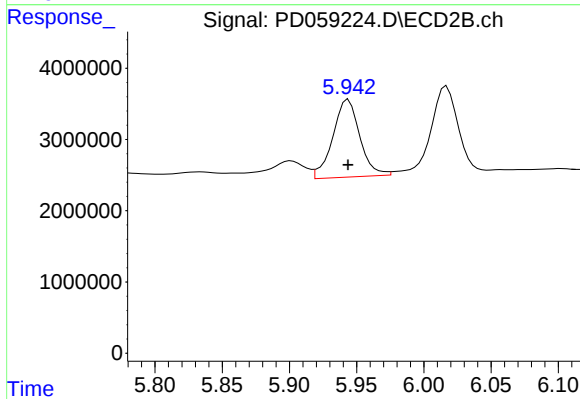


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 15170691
Conc: 55.67 ng/ml

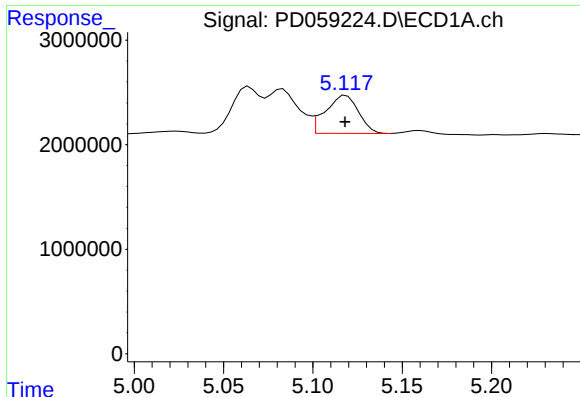


#26 Chlordane-4

R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 4673498
Conc: 46.62 ng/ml

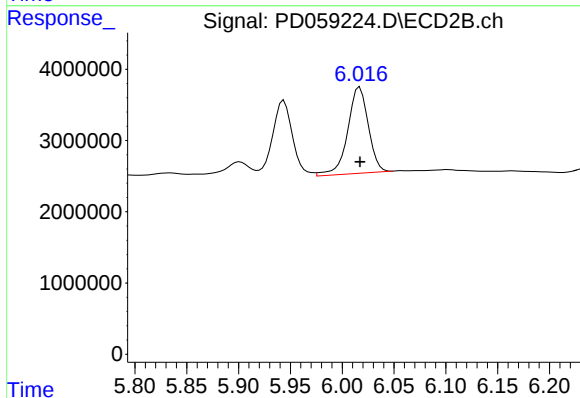


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 16759774
Conc: 51.37 ng/ml

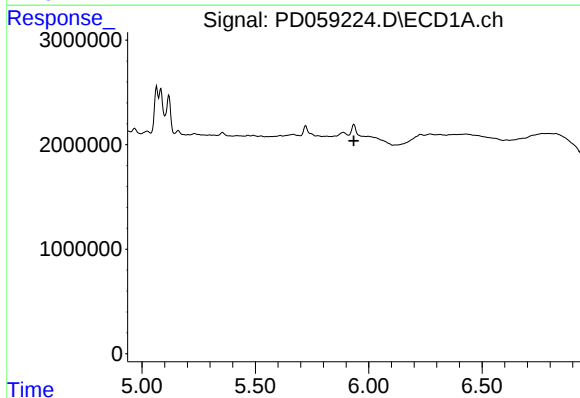


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.934 min
Response: 0
Conc: N.D.

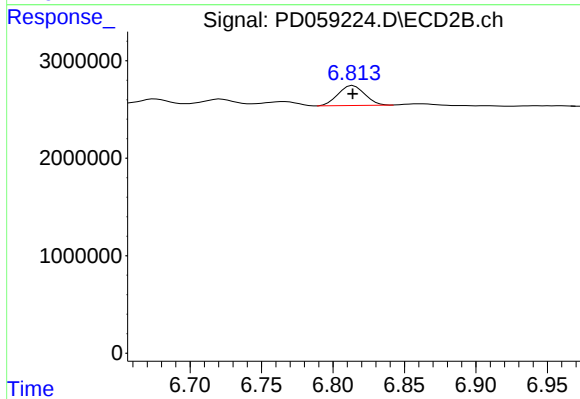

#27 Chlordane-5

R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 2653554
Conc: 45.02 ng/ml

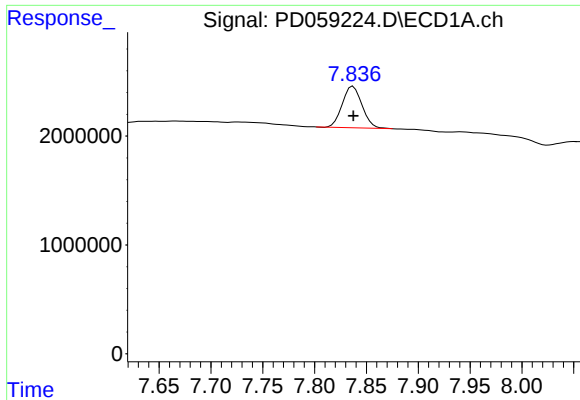


#28 Decachlorobiphenyl

R.T.: 7.837 min

Delta R.T.: 0.000 min

Response: 5032766

Conc: 5.25 ng/ml

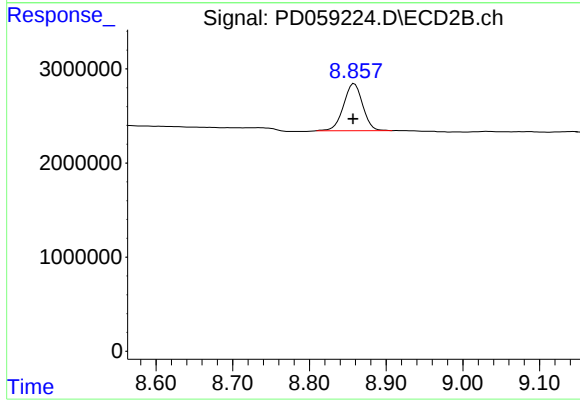

#28 Decachlorobiphenyl

R.T.: 8.858 min

Delta R.T.: 0.001 min

Response: 8755874

Conc: 5.65 ng/ml