

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 21:01
 Operator : DD\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD091620TOX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 04:06:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 04:05:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.206	3.865	44923548	84216313	50.162	49.572
7) SA Decachlor...	7.838	8.857	47469119	78910980	50.878	49.625
Target Compounds						
2) Toxaphene-1	5.588	6.410	5132054	8929416	513.147	482.917
3) Toxaphene-2	5.964	6.704	7821629	10637535	495.544	503.414
4) Toxaphene-3	6.206	6.990	7998430	22868795	508.090	520.539
5) Toxaphene-4	6.340	7.073	3609349	14267686	539.473	514.780
6) Toxaphene-5	6.622	7.485	2768008	10976523	474.950	511.678

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 21:01
Operator : DD\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 04:06:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 04:05:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

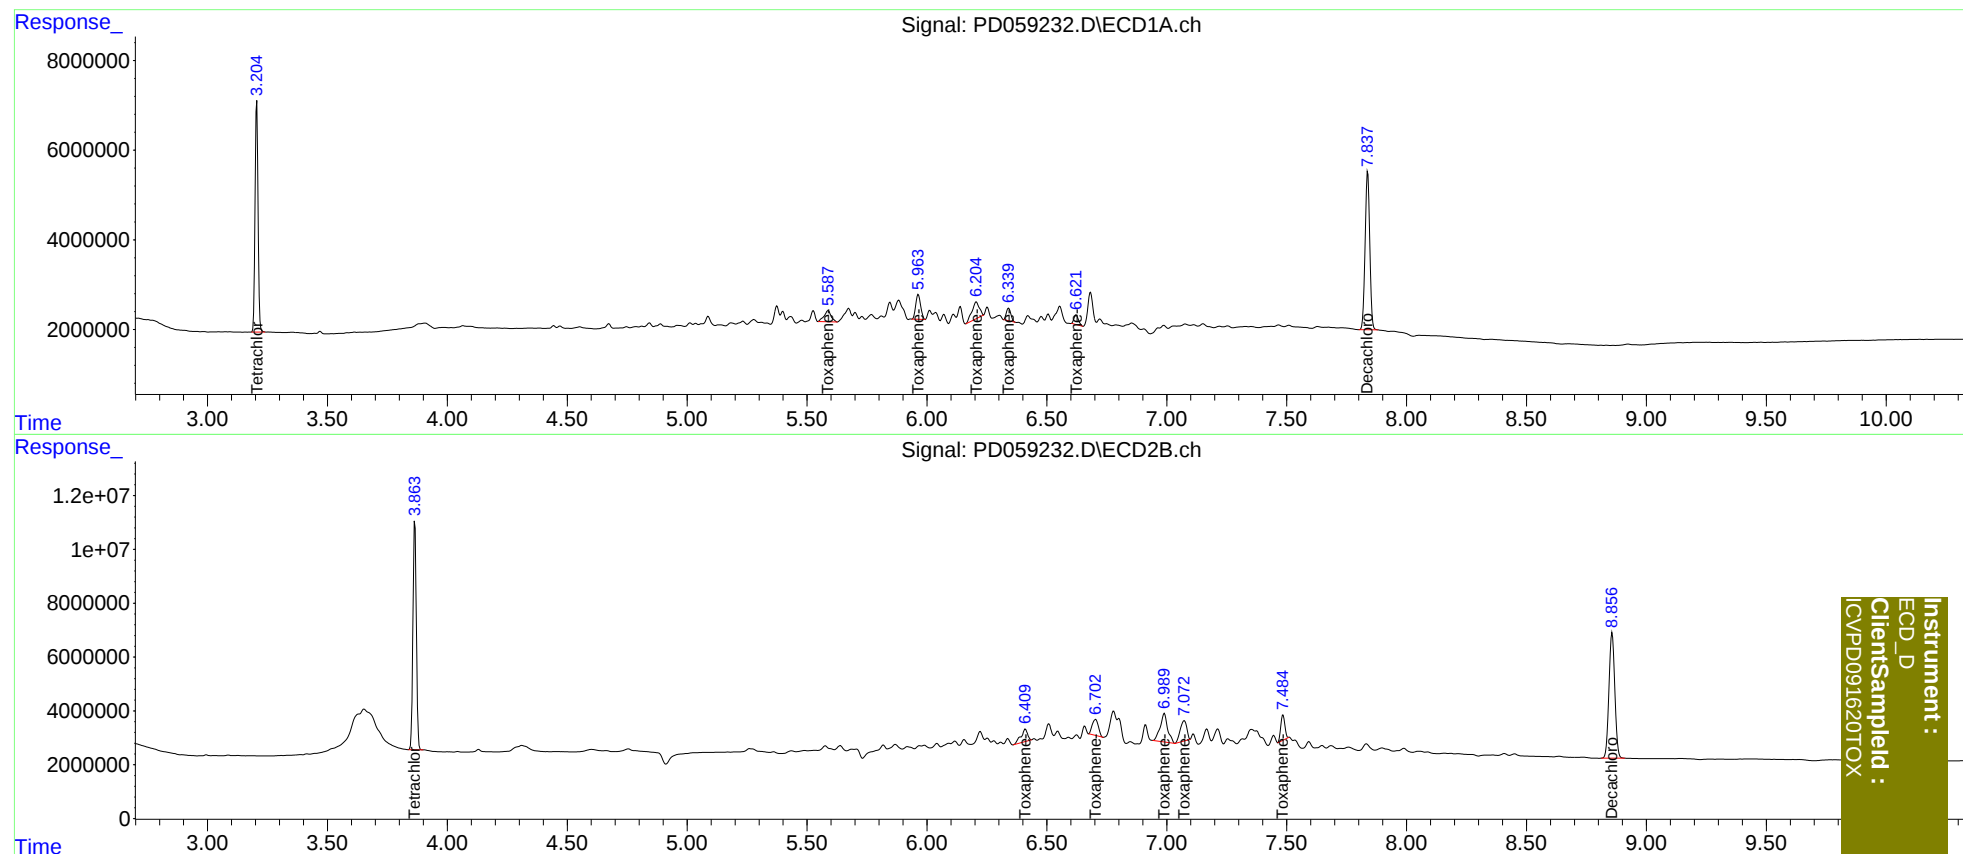

Instrument :
ECD_D
ClientSample :
ICV\PD091620\TOX