

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 16:47
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 04:10:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:41:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	20638701	38931991	22.899	23.044
28)	SA Decachlor...	7.837	8.858	20908561	36473040	22.444	23.315
Target Compounds							
9)	A Endosulfan I	5.170	6.063	10494987	19762398	10.009	10.272
10)	B gamma-Chl...	5.063	5.943	11274461	20792819	9.866	9.973
12)	B 4,4'-DDE	5.289	6.176	22838704	41086529	20.521	20.401
13)	MA Dieldrin	5.408	6.319	23187325	43359342	20.810	20.909
19)	B Endosulfa...	6.310	7.091	18428247	35396387	19.717	19.980
20)	A Methoxychlor	6.576	7.419	41463300	100.5E6	106.838	103.525
21)	B Endrin ke...	6.789	7.556	22745333	40490364	20.434	20.728



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 16:47
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 04:10:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:41:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

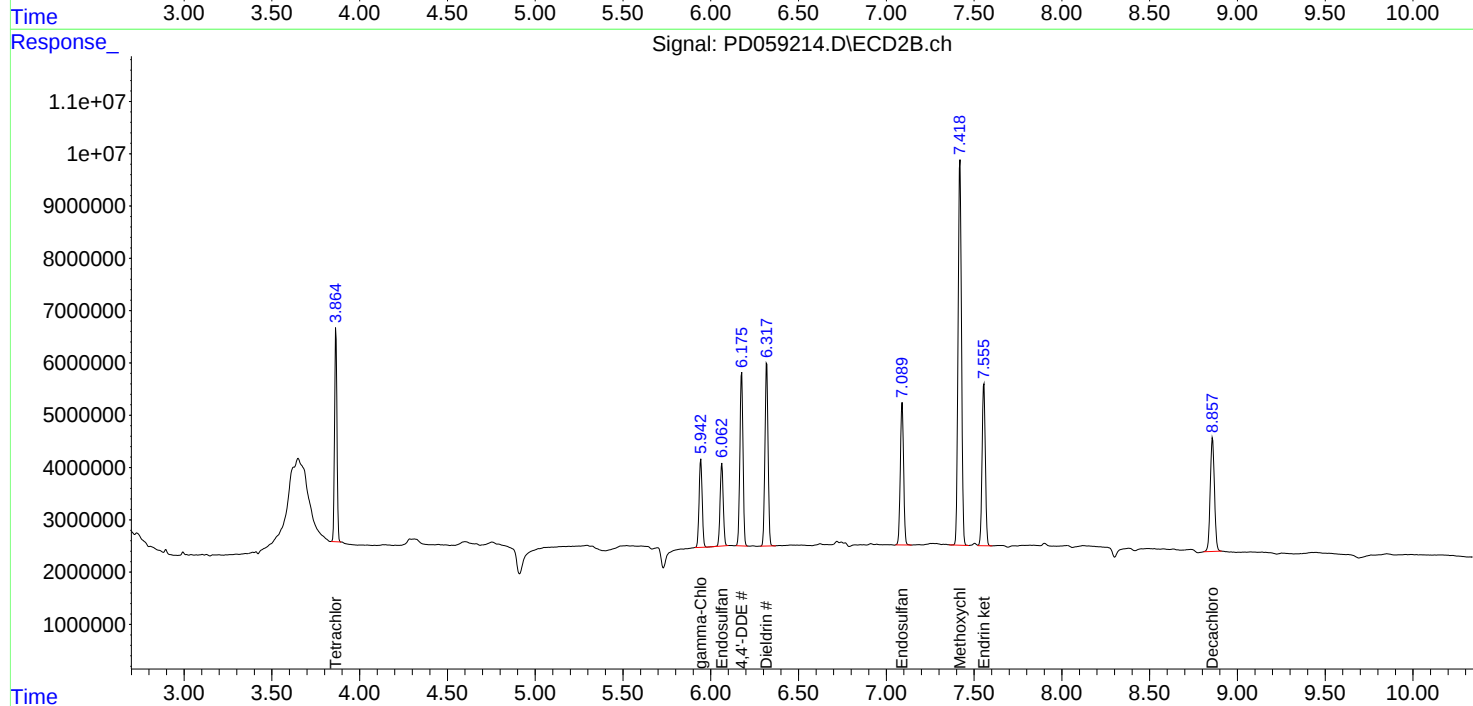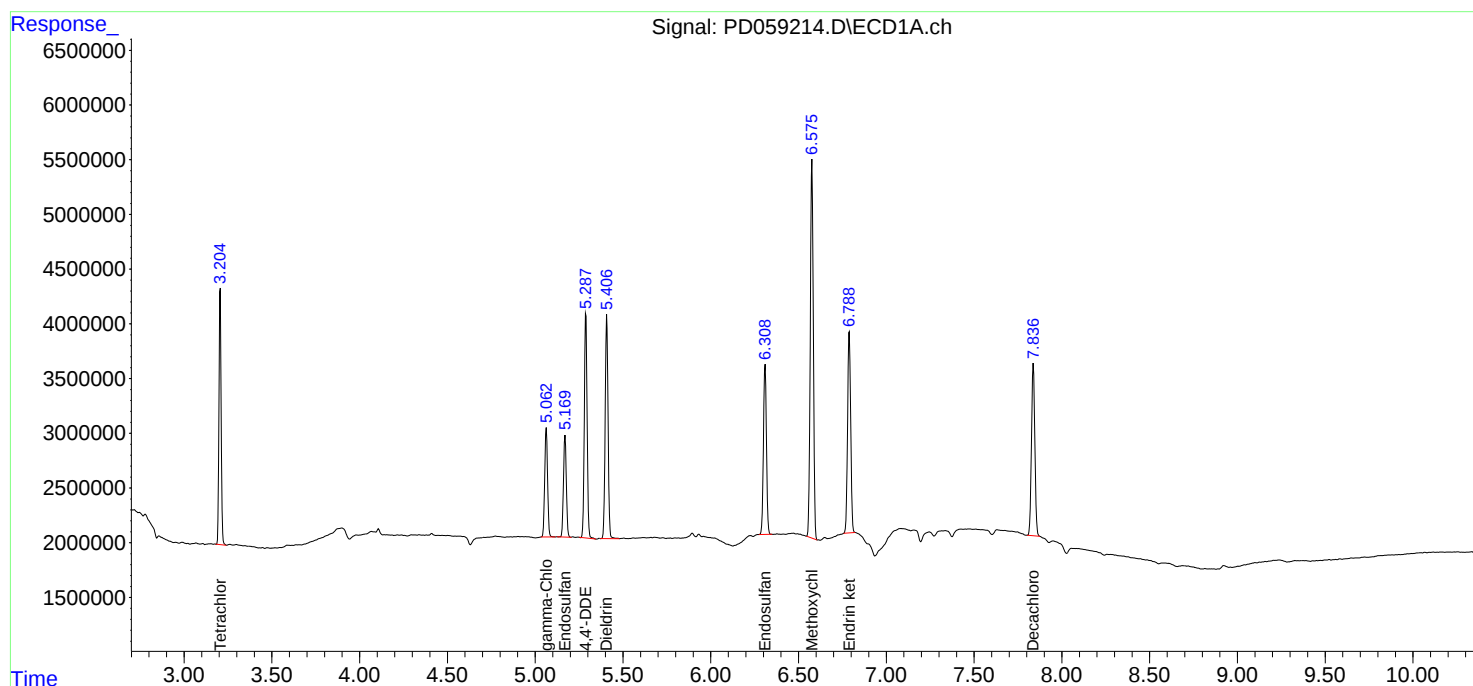


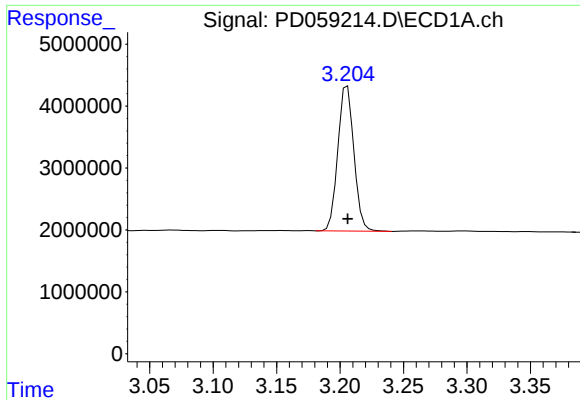

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 20638701
Conc: 22.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

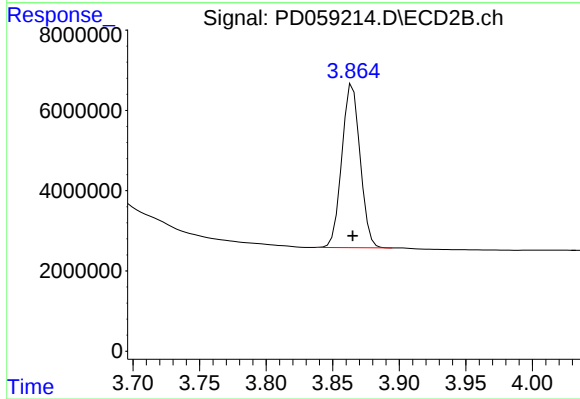


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 38931991
Conc: 23.04 ng/ml

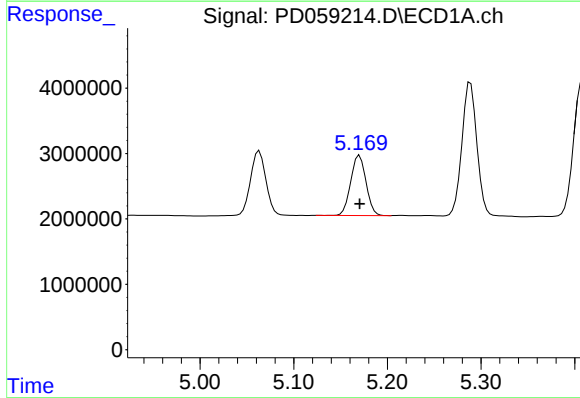


#9 Endosulfan I

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 10494987
Conc: 10.01 ng/ml

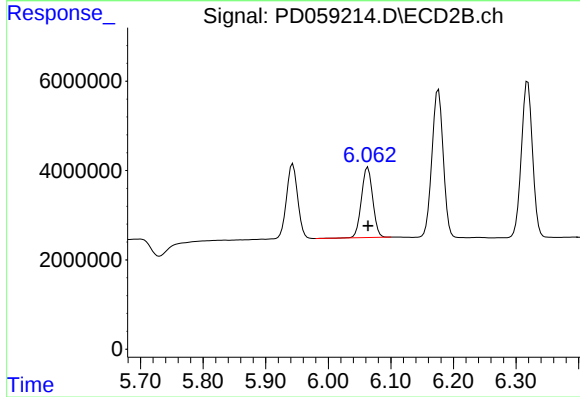

#9 Endosulfan I


R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 19762398
Conc: 10.27 ng/ml

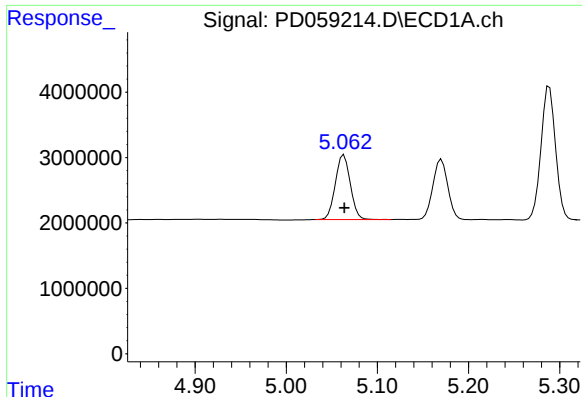

#10 gamma-Chlordane


R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 11274461
Conc: 9.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

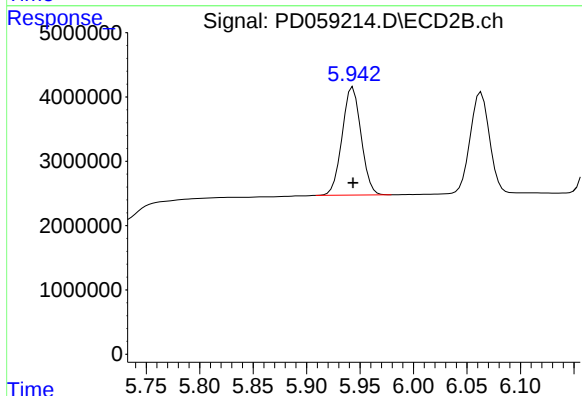


#10 gamma-Chlordane

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 20792819
Conc: 9.97 ng/ml

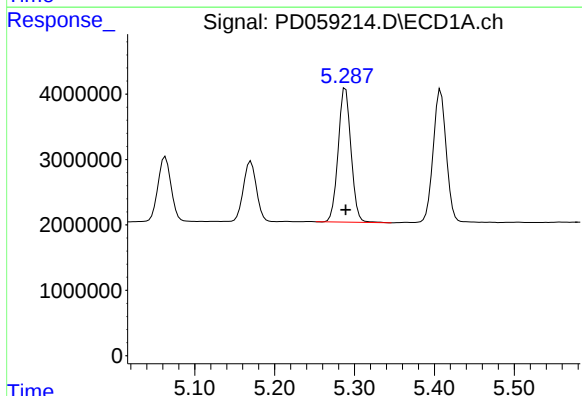


#12 4,4'-DDE

R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 22838704
Conc: 20.52 ng/ml

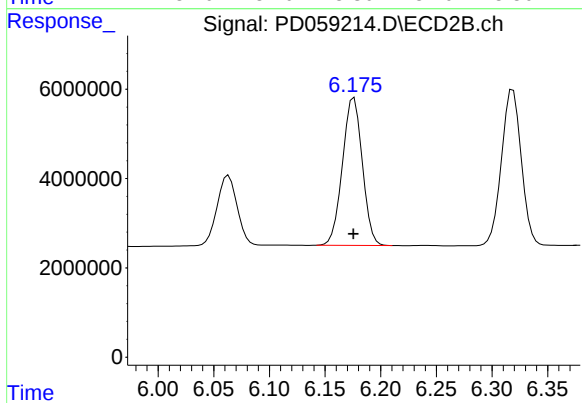

#12 4,4'-DDE


R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 41086529
Conc: 20.40 ng/ml

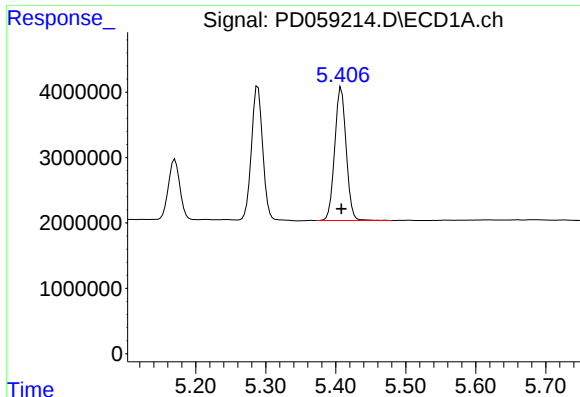

#13 Dieldrin


R.T.: 5.408 min
Delta R.T.: 0.000 min
Response: 23187325
Conc: 20.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

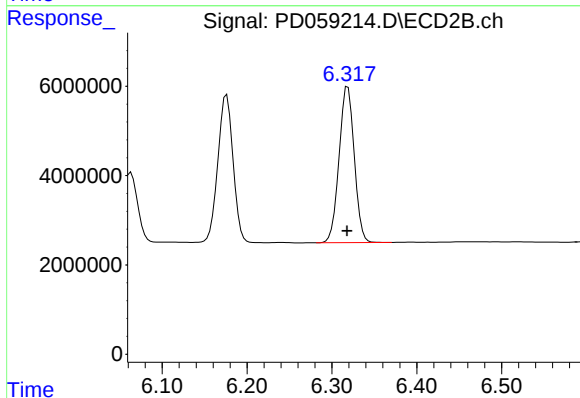


#13 Dieldrin

R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 43359342
Conc: 20.91 ng/ml

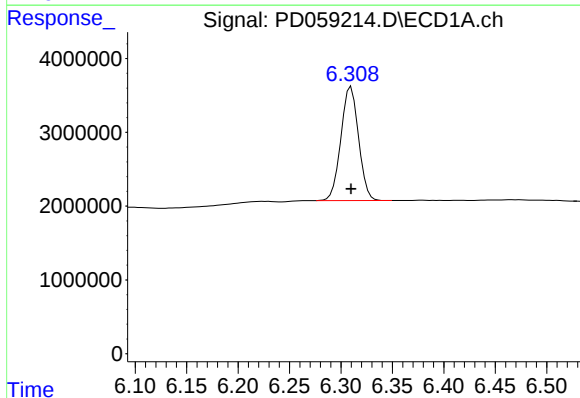


#19 Endosulfan Sulfate

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 18428247
Conc: 19.72 ng/ml

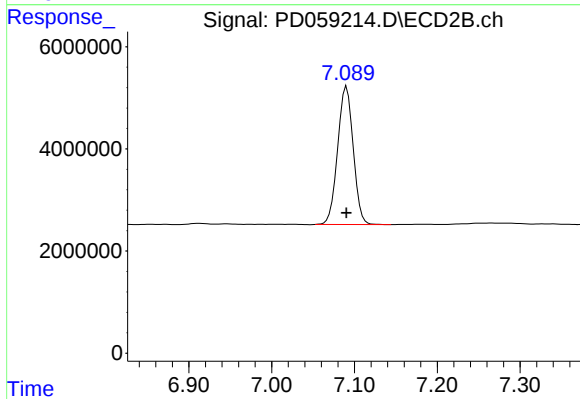

#19 Endosulfan Sulfate


R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 35396387
Conc: 19.98 ng/ml

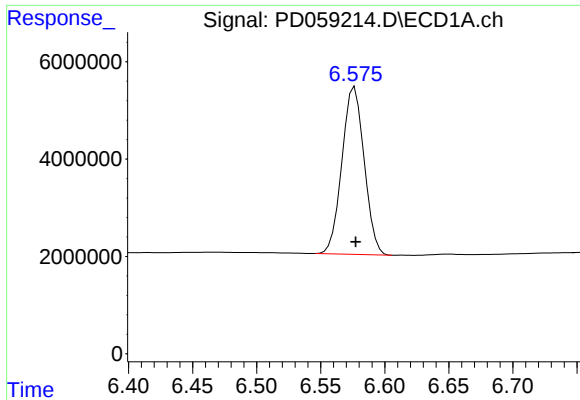

#20 Methoxychlor


R.T.: 6.576 min
Delta R.T.: 0.000 min
Response: 41463300
Conc: 106.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

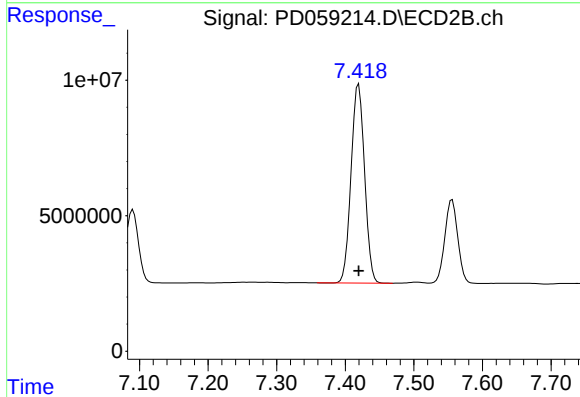


#20 Methoxychlor

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 100523425
Conc: 103.52 ng/ml

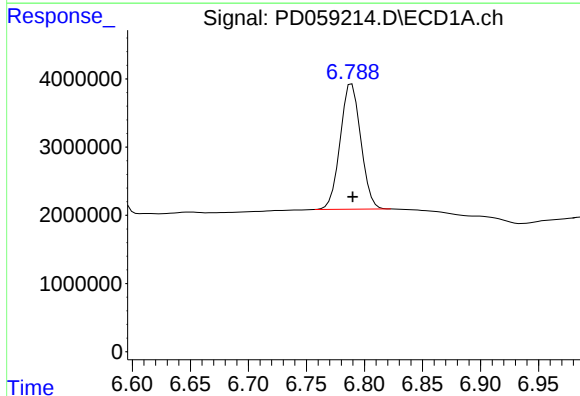


#21 Endrin ketone

R.T.: 6.789 min
Delta R.T.: 0.000 min
Response: 22745333
Conc: 20.43 ng/ml

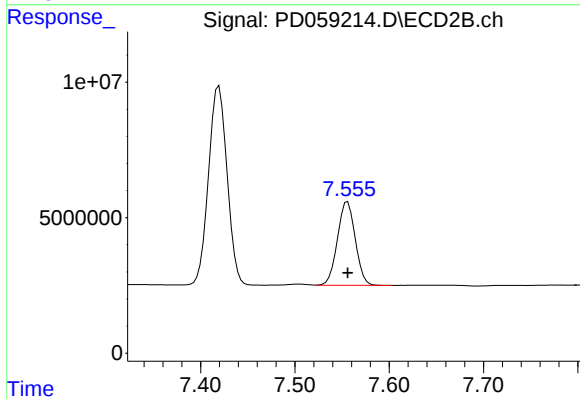

#21 Endrin ketone


R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 40490364
Conc: 20.73 ng/ml

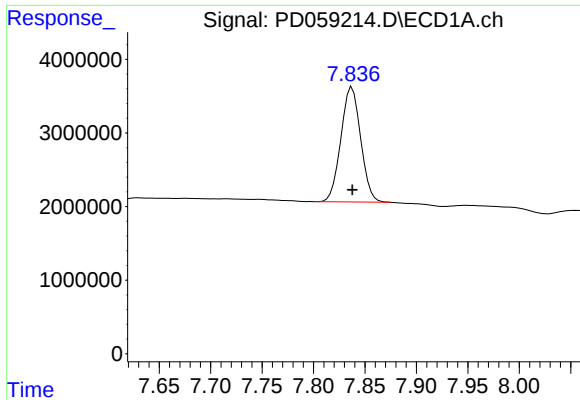

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: 0.000 min
Response: 20908561
Conc: 22.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

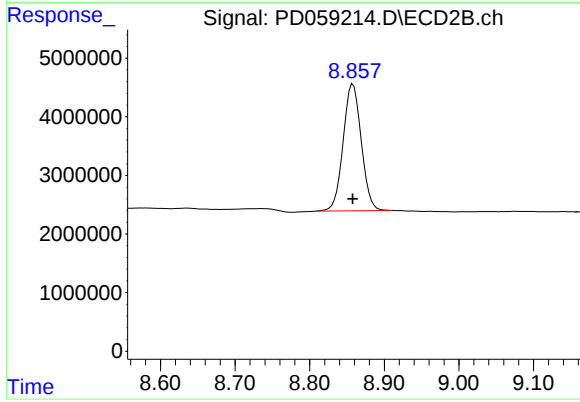

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 36473040
Conc: 23.32 ng/ml