

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 18:11
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:29:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:28:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	101.4E6	164.5E6	98.244	94.124
28)	SA Decachlor...	7.837	8.858	91294903	146.3E6	95.294	94.437
Target Compounds							
23)	Chlordane-1	4.033	4.841	28842891	63106519	993.304	900.085
24)	Chlordane-2	4.517	5.304	32699383	62692204	944.982	925.062
25)	Chlordane-3	5.064	5.944	103.0E6	264.4E6	987.851	970.284
26)	Chlordane-4	5.120	6.017	97027154	314.4E6	967.932	963.684
27)	Chlordane-5	5.935	6.813	34348019	58443628	990.430	991.566



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 18:11
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:29:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:28:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

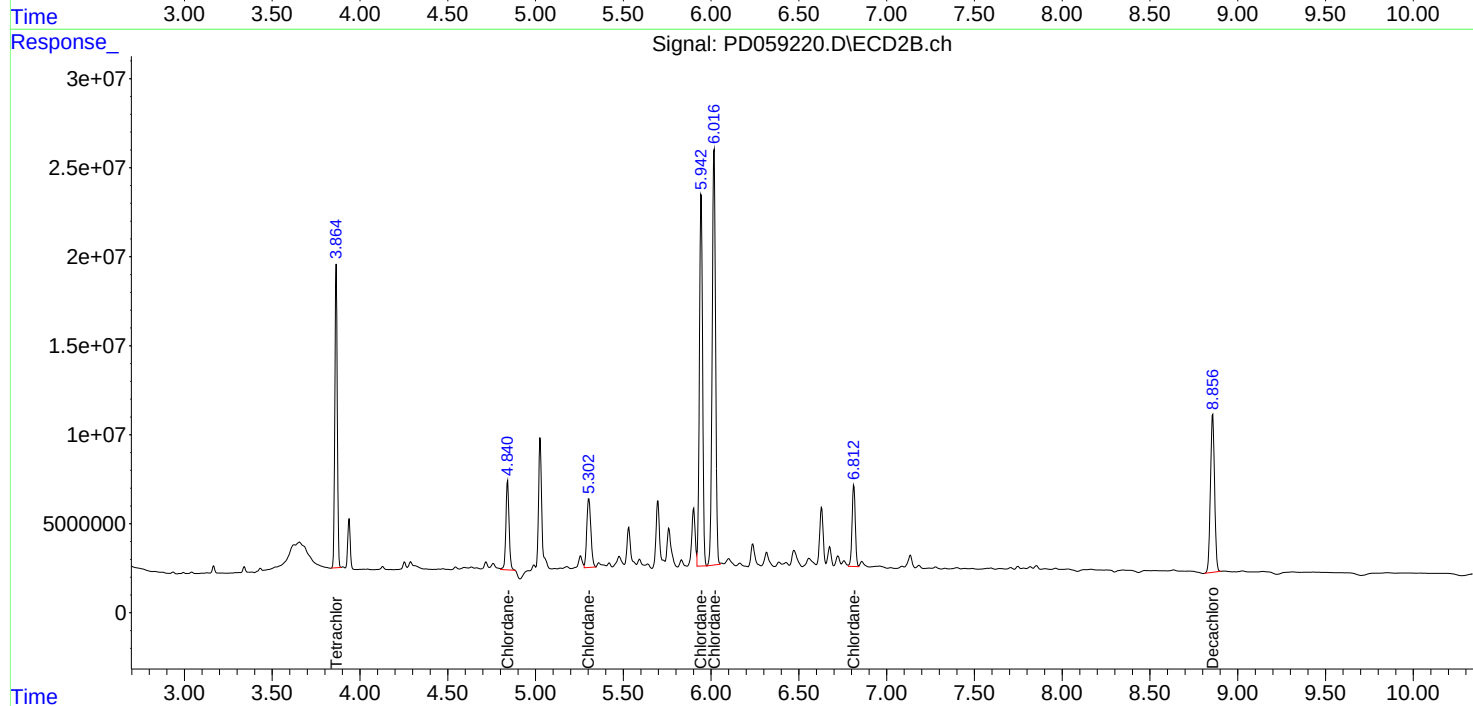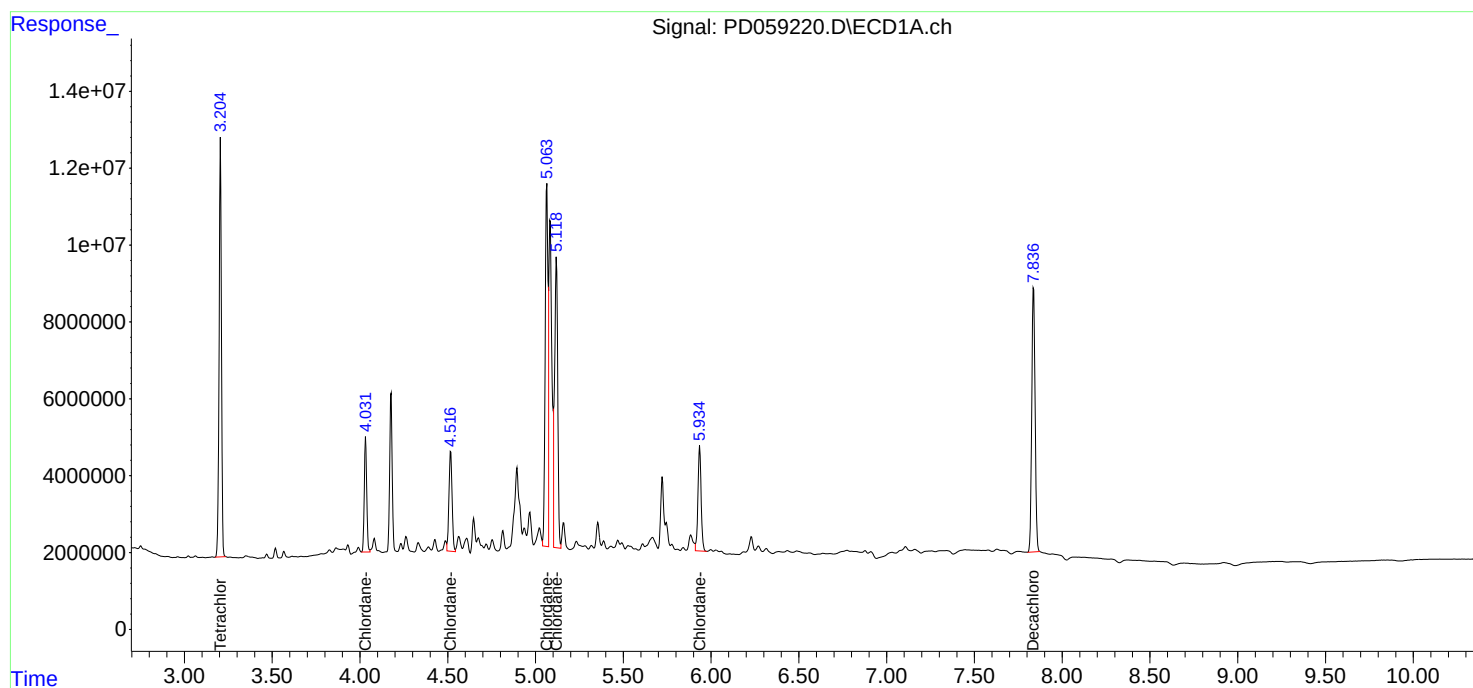


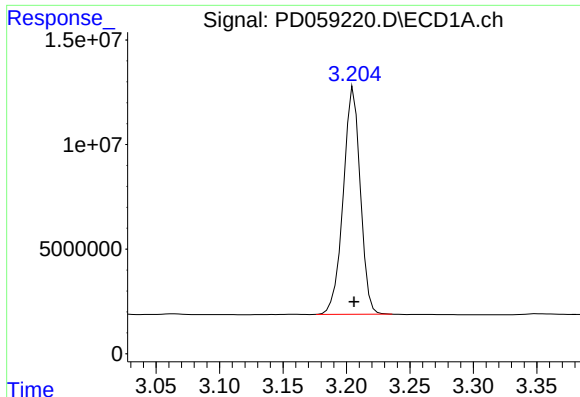

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 101428116
Conc: 98.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

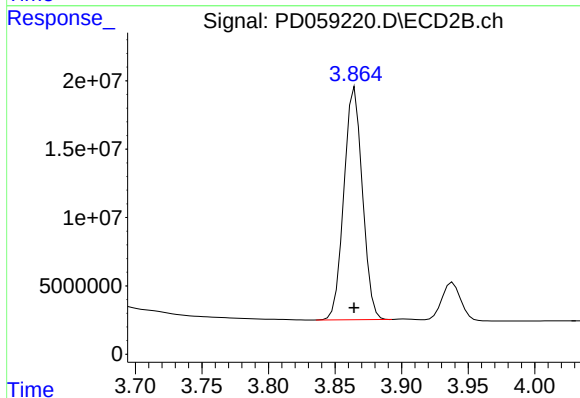


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 164487910
Conc: 94.12 ng/ml

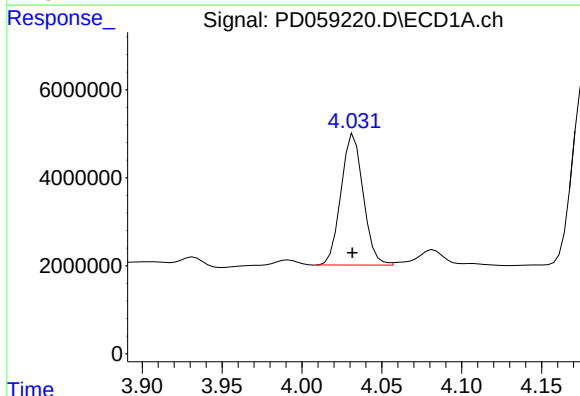


#23 Chlordane-1

R.T.: 4.033 min
Delta R.T.: 0.001 min
Response: 28842891
Conc: 993.30 ng/ml

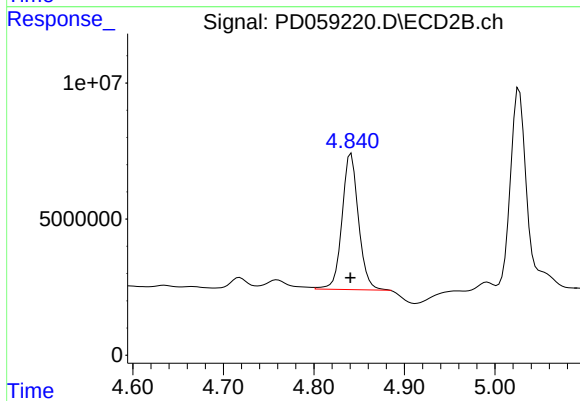

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 63106519
Conc: 900.09 ng/ml

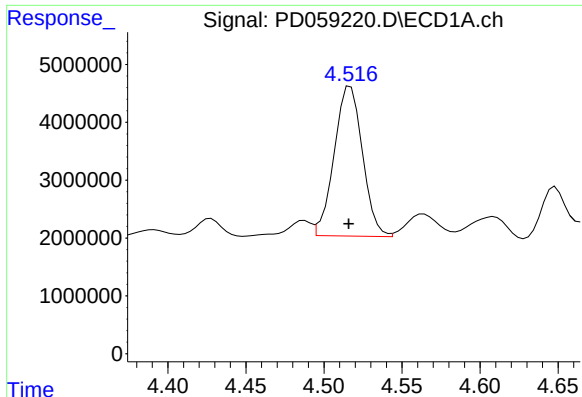

#24 Chlordane-2


R.T.: 4.517 min
Delta R.T.: 0.001 min
Response: 32699383
Conc: 944.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

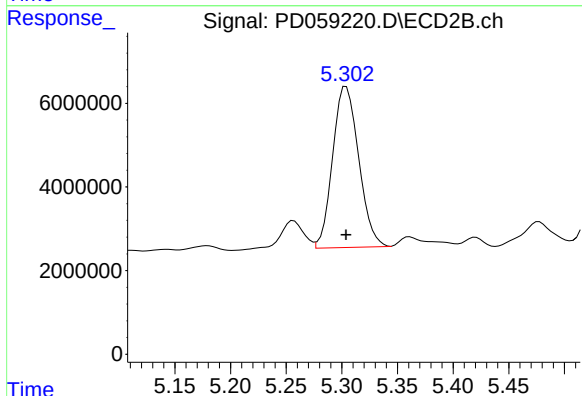


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 62692204
Conc: 925.06 ng/ml

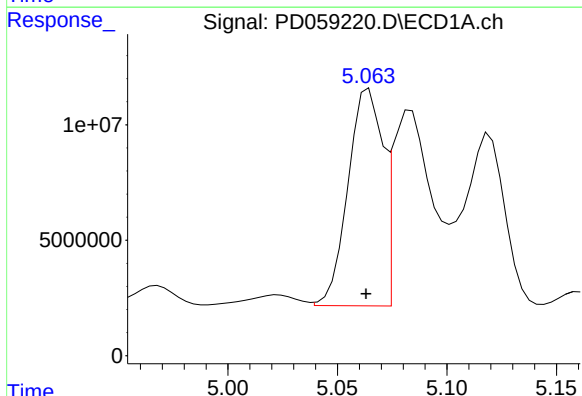


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.001 min
Response: 103032347
Conc: 987.85 ng/ml

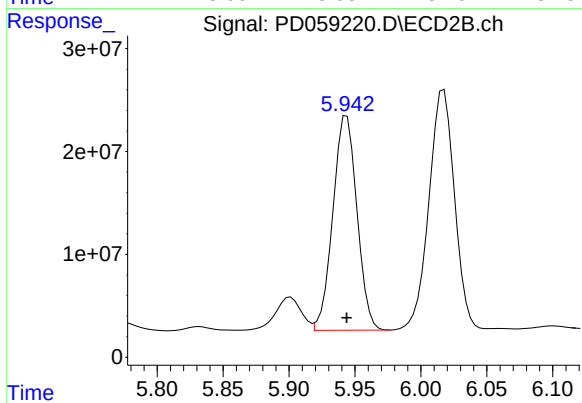

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 264430790
Conc: 970.28 ng/ml

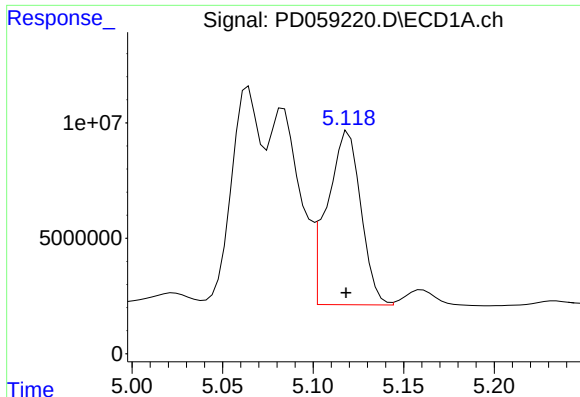

#26 Chlordane-4


R.T.: 5.120 min
Delta R.T.: 0.001 min
Response: 97027154
Conc: 967.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

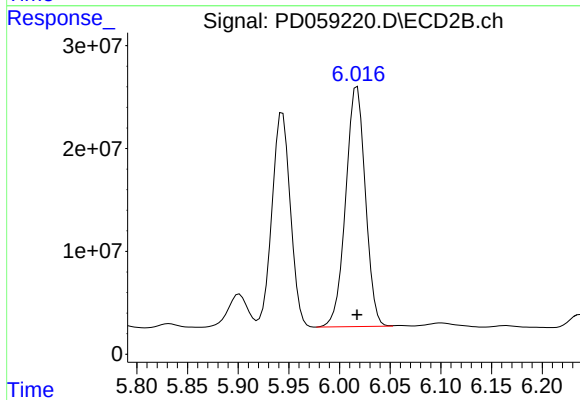


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 314417003
Conc: 963.68 ng/ml

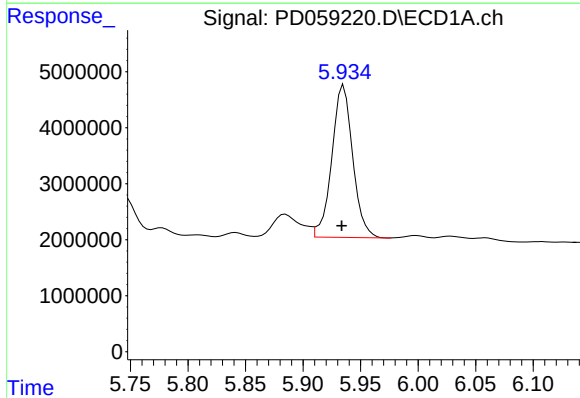


#27 Chlordane-5

R.T.: 5.935 min
Delta R.T.: 0.001 min
Response: 34348019
Conc: 990.43 ng/ml

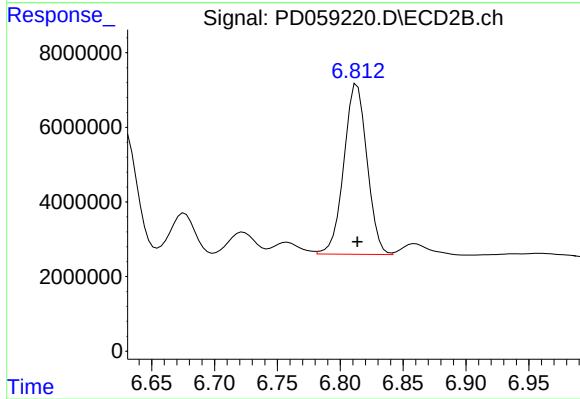

#27 Chlordane-5


R.T.: 6.813 min
Delta R.T.: 0.000 min
Response: 58443628
Conc: 991.57 ng/ml

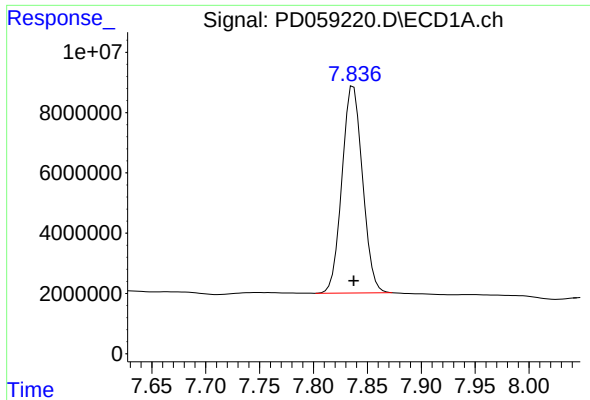

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: 0.000 min
Response: 91294903
Conc: 95.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

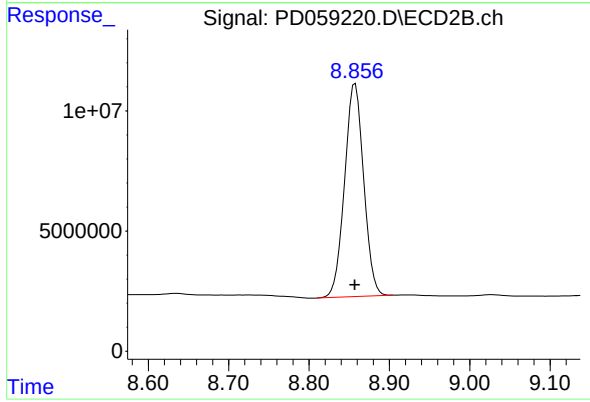

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 146278408
Conc: 94.44 ng/ml