

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 18:26
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:29:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:28:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.205	3.865	78617091	130.0E6	76.149	74.408
28)	SA Decachlor...	7.837	8.857	70912386	113.1E6	74.019	73.028
Target Compounds							
23)	Chlordane-1	4.032	4.841	22653458	50967480	780.150	726.947
24)	Chlordane-2	4.516	5.304	25696196	49693756	742.597	733.262
25)	Chlordane-3	5.064	5.944	79404897	206.6E6	761.316	758.027
26)	Chlordane-4	5.119	6.017	76445327	245.3E6	762.610	751.844
27)	Chlordane-5	5.935	6.814	26671602	44913240	769.080	762.007


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 18:26
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:29:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:28:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

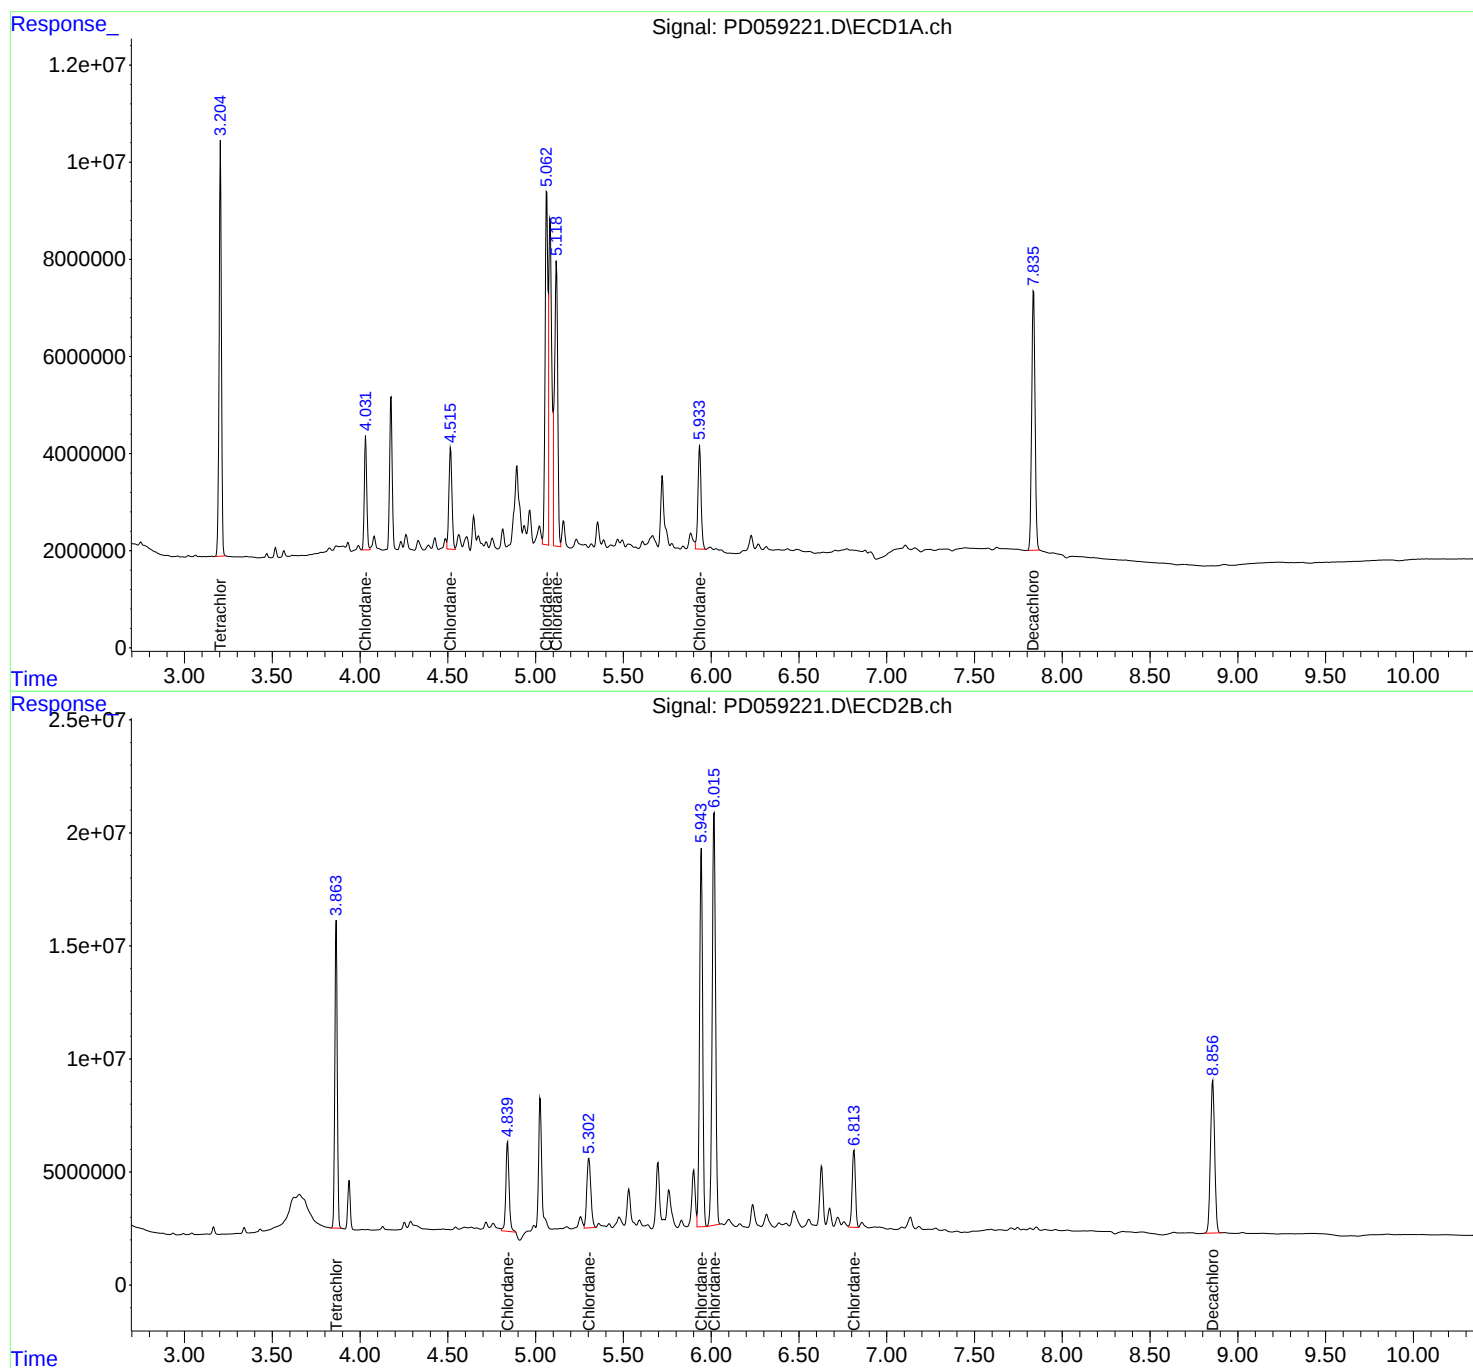


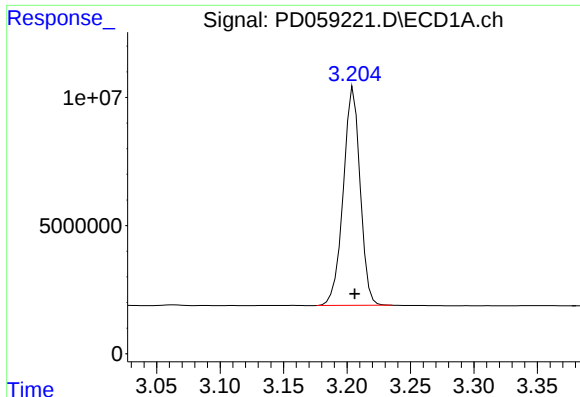

#1 Tetrachloro-m-xylene


R.T.: 3.205 min
Delta R.T.: 0.000 min
Response: 78617091
Conc: 76.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

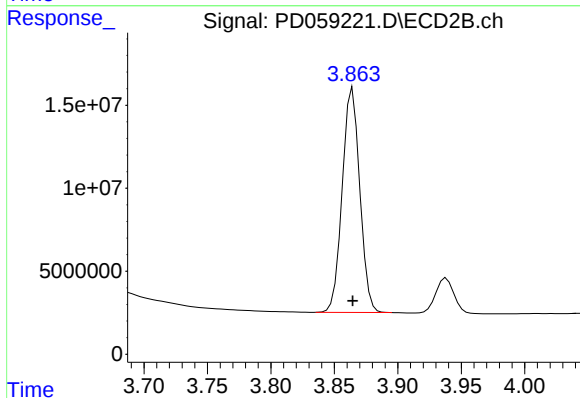


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 130032994
Conc: 74.41 ng/ml

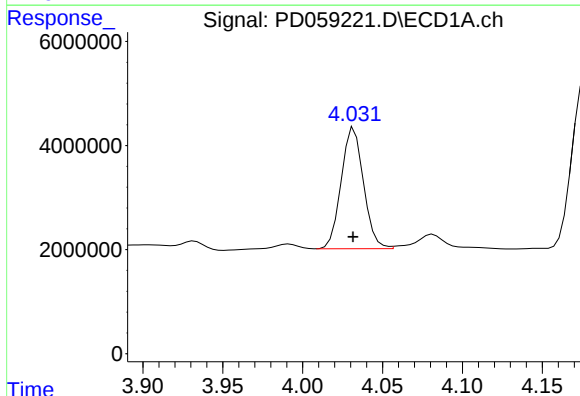


#23 Chlordane-1

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 22653458
Conc: 780.15 ng/ml

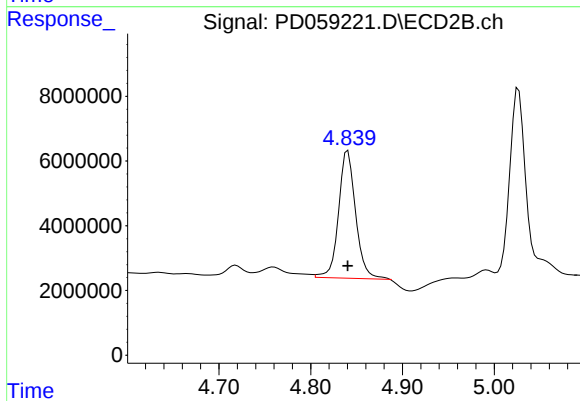

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 50967480
Conc: 726.95 ng/ml

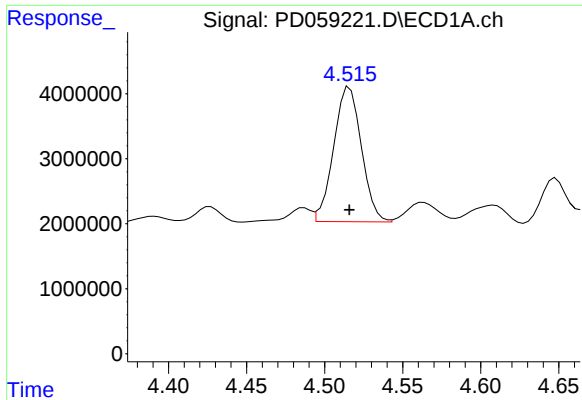

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 25696196
Conc: 742.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

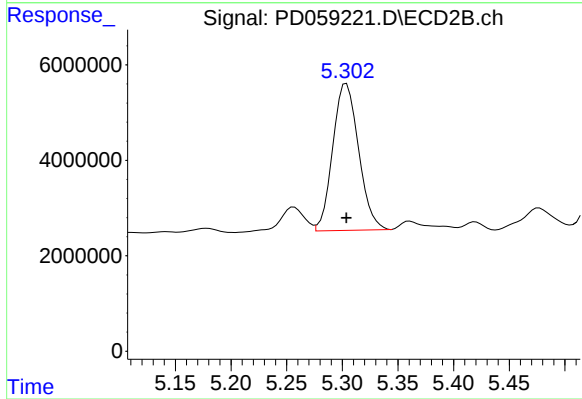


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 49693756
Conc: 733.26 ng/ml

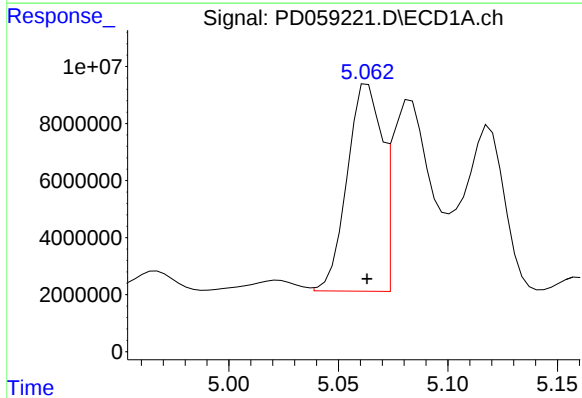


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 79404897
Conc: 761.32 ng/ml

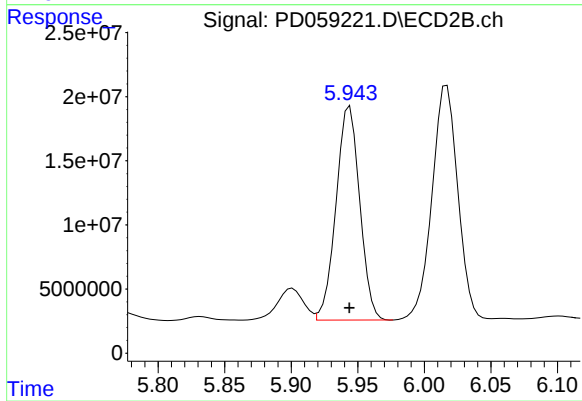

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 206584372
Conc: 758.03 ng/ml

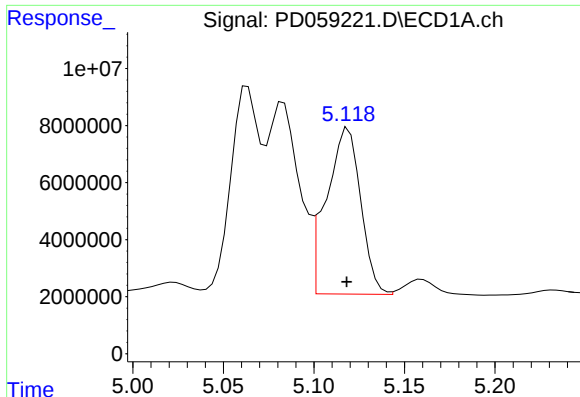

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 76445327
Conc: 762.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

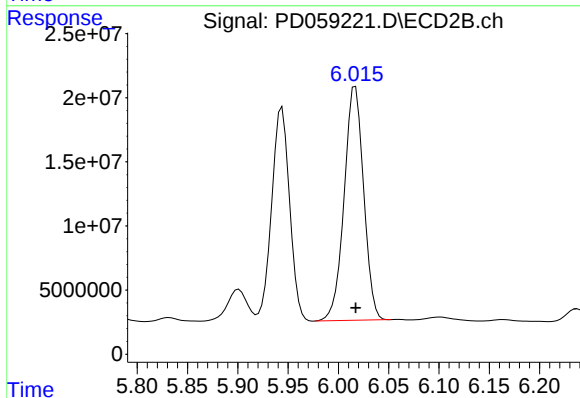


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 245300898
Conc: 751.84 ng/ml

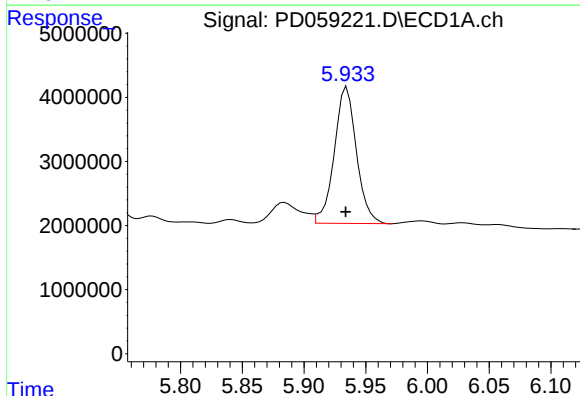


#27 Chlordane-5

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 26671602
Conc: 769.08 ng/ml

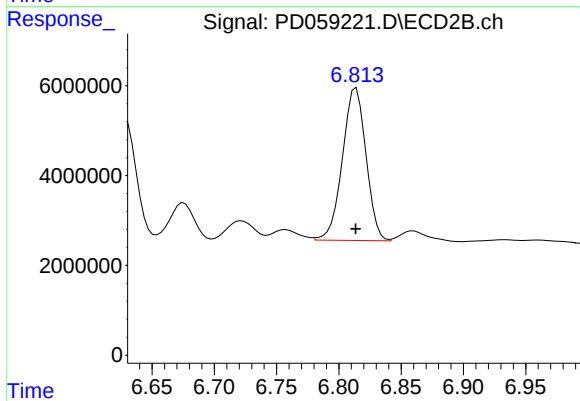

#27 Chlordane-5


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 44913240
Conc: 762.01 ng/ml

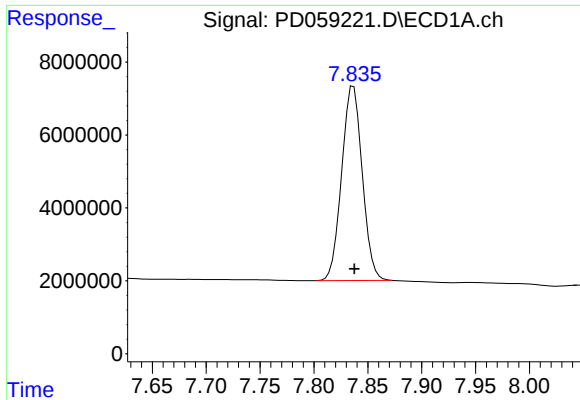

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: 0.000 min
Response: 70912386
Conc: 74.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

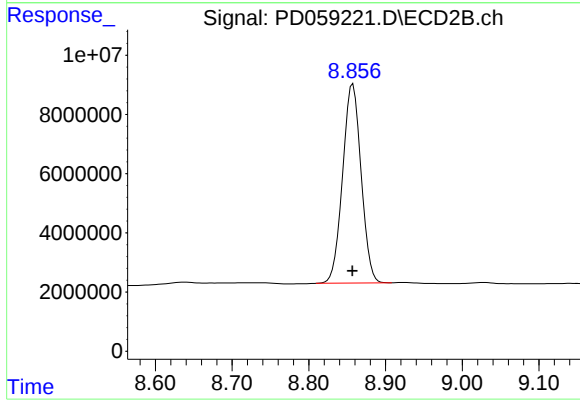

#28 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: 0.000 min
Response: 113117893
Conc: 73.03 ng/ml