

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 18:40
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:30:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:28:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.864	51620670	87378528	50.000	50.000
28)	SA Decachlor...	7.838	8.857	47901735	77447816	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.032	4.840	14518659	35055848	500.000	500.000
24)	Chlordane-2	4.516	5.304	17301587	33885399	500.000	500.000
25)	Chlordane-3	5.063	5.944	52149767	136.3E6	500.000	500.000
26)	Chlordane-4	5.118	6.017	50120868	163.1E6	500.000	500.000
27)	Chlordane-5	5.934	6.814	17339949	29470377	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 18:40
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:30:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:28:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

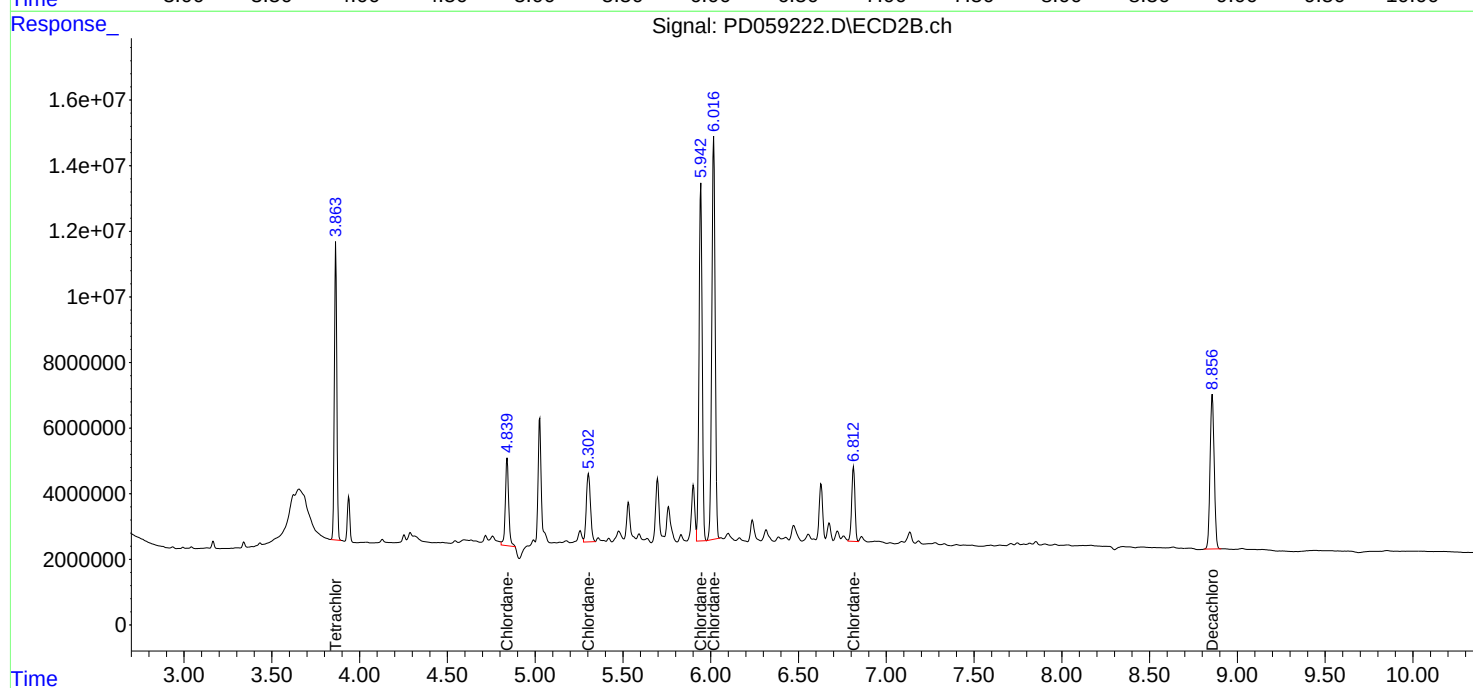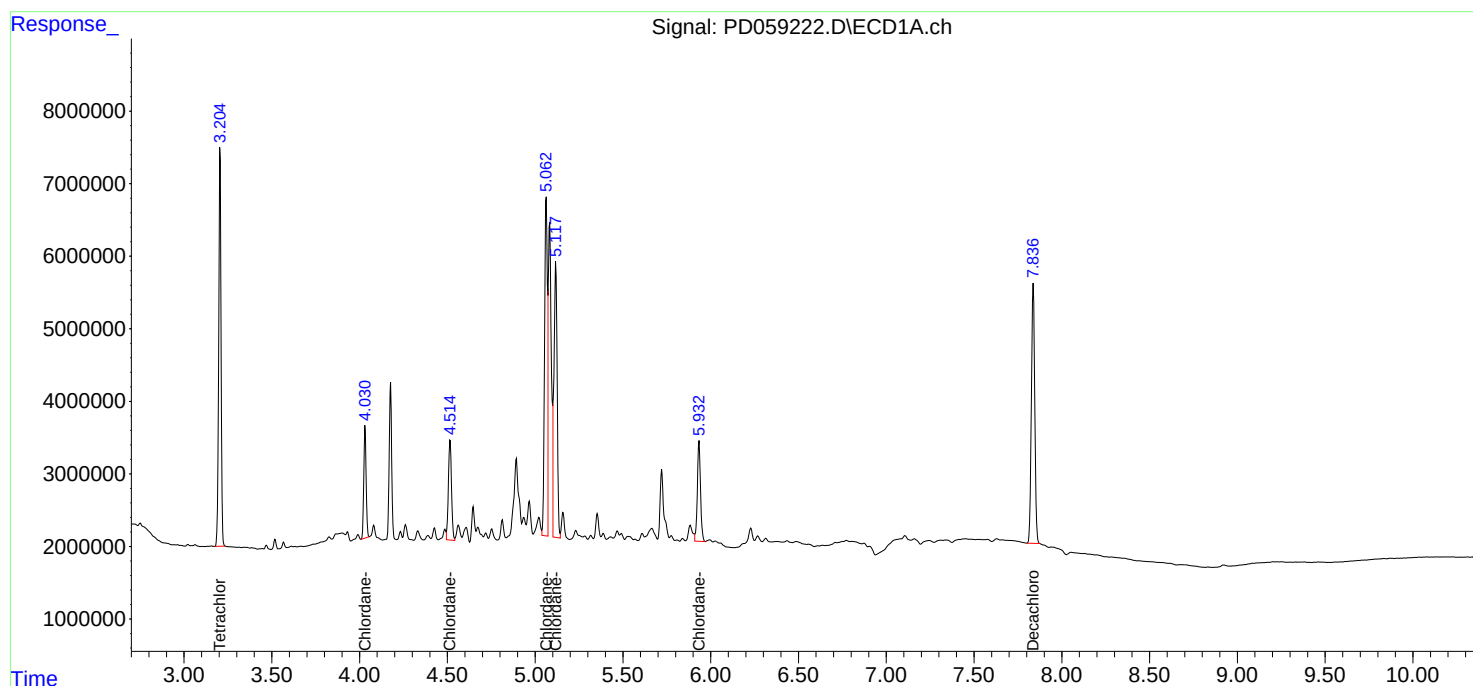


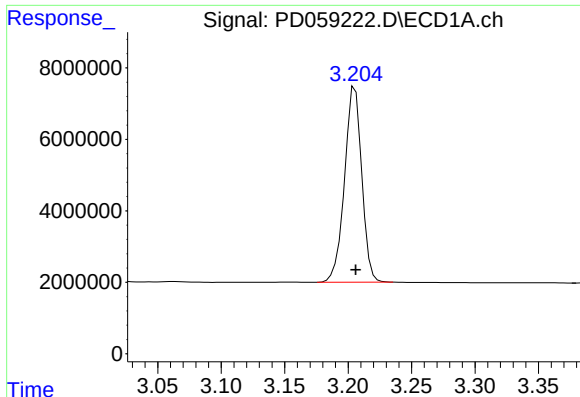

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 51620670
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

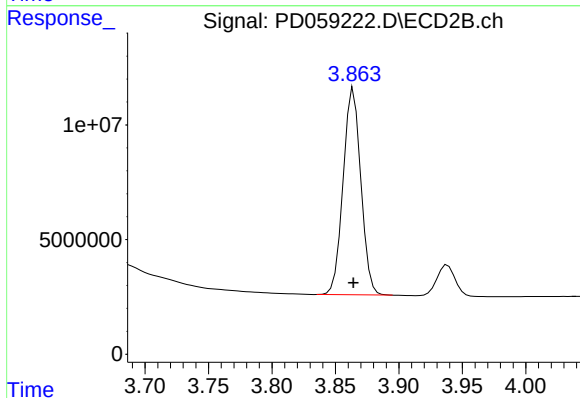


#1 Tetrachloro-m-xylene

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 87378528
Conc: 50.00 ng/ml

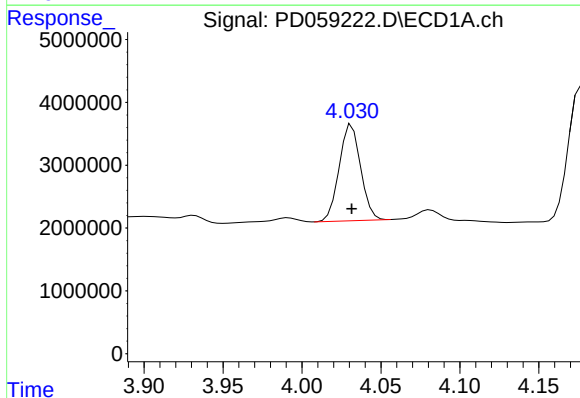


#23 Chlordane-1

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 14518659
Conc: 500.00 ng/ml

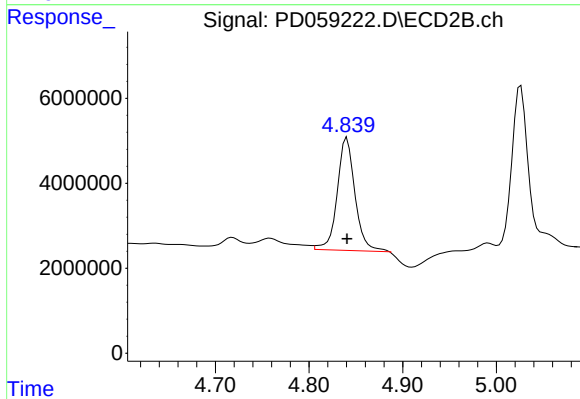

#23 Chlordane-1


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 35055848
Conc: 500.00 ng/ml

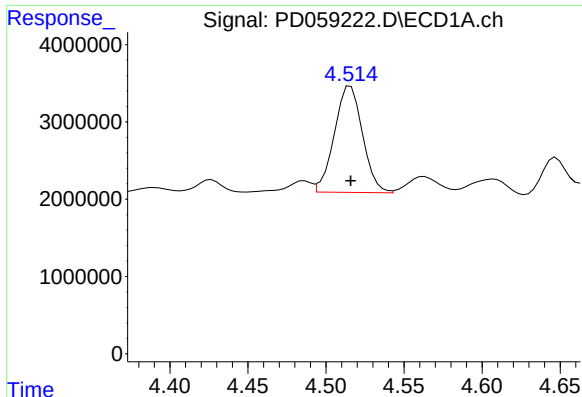

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 17301587
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

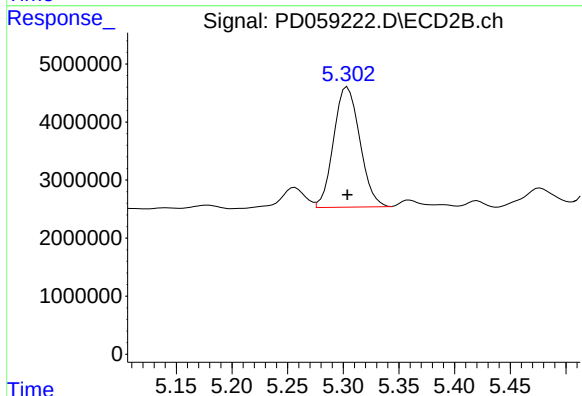


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 33885399
Conc: 500.00 ng/ml

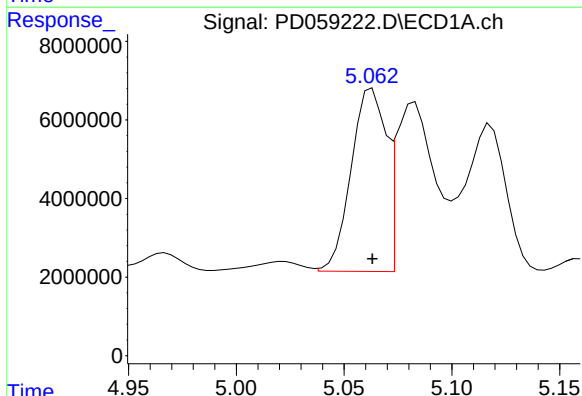


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 52149767
Conc: 500.00 ng/ml

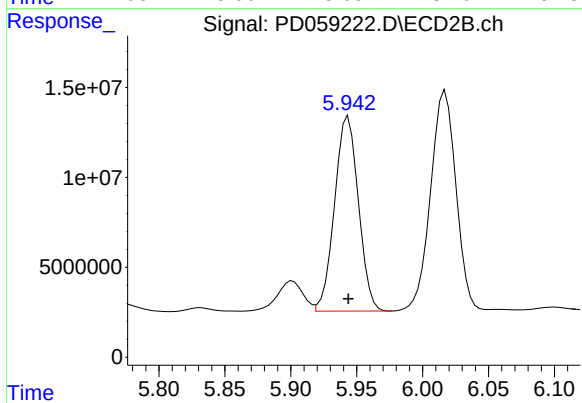

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 136264598
Conc: 500.00 ng/ml

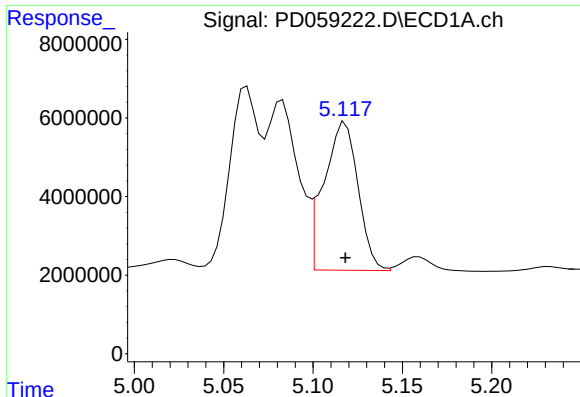

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 50120868
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

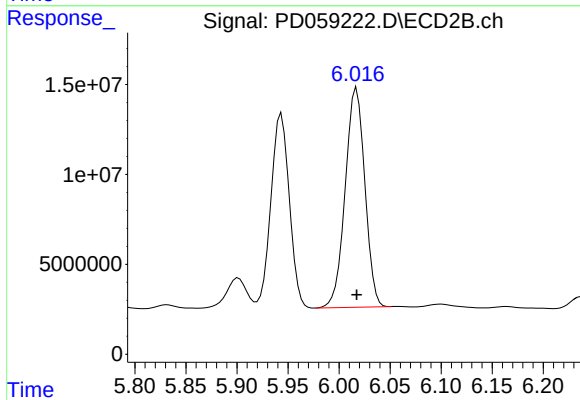


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 163132750
Conc: 500.00 ng/ml

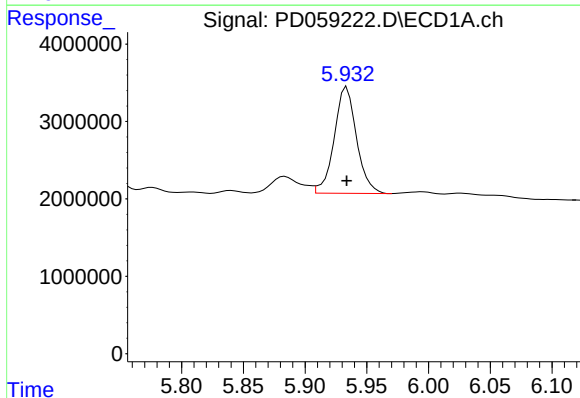


#27 Chlordane-5

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 17339949
Conc: 500.00 ng/ml

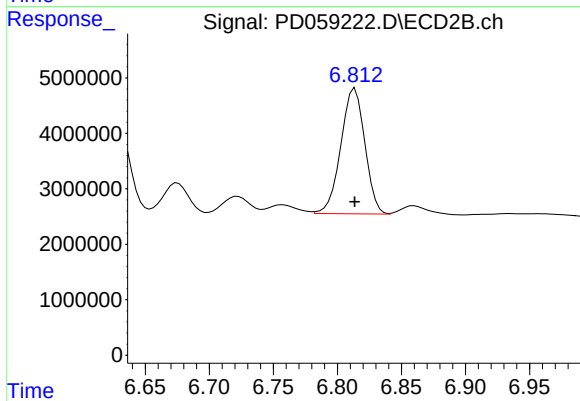

#27 Chlordane-5


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 29470377
Conc: 500.00 ng/ml

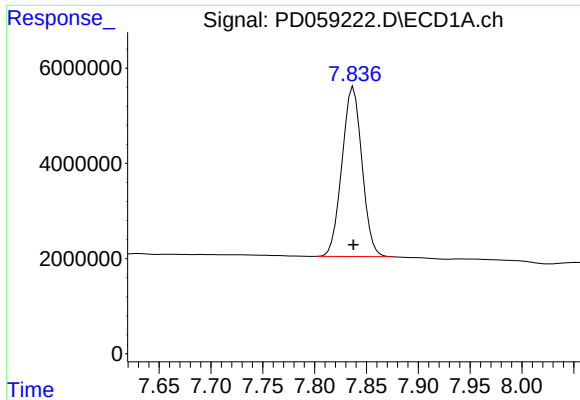

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 47901735
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

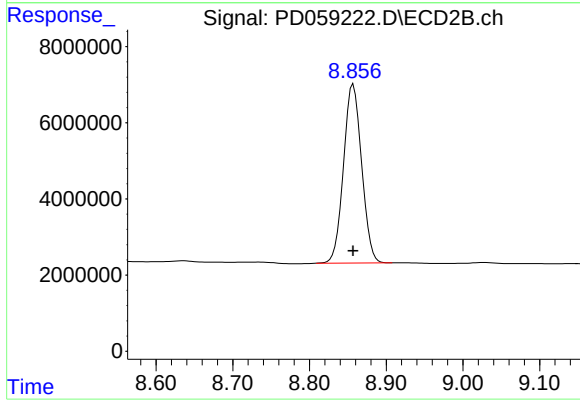

#28 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: 0.000 min
Response: 77447816
Conc: 50.00 ng/ml