

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 18:54
 Operator : DD\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:30:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:28:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.205	3.865	24935953	43395474	24.153	24.832
28)	SA Decachlor...	7.838	8.857	24057145	39977735	25.111	25.809
Target Compounds							
23)	Chlordane-1	4.032	4.841	7034650	18514834	242.262	264.076
24)	Chlordane-2	4.516	5.304	8978285	17734395	259.464	261.682
25)	Chlordane-3	5.064	5.944	24959032	66413614	239.301	243.694
26)	Chlordane-4	5.119	6.018	23355580	80206189	232.993	245.831
27)	Chlordane-5	5.935	6.814	8302968	14020621	239.417	237.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 18:54
Operator : DD\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:30:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:28:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

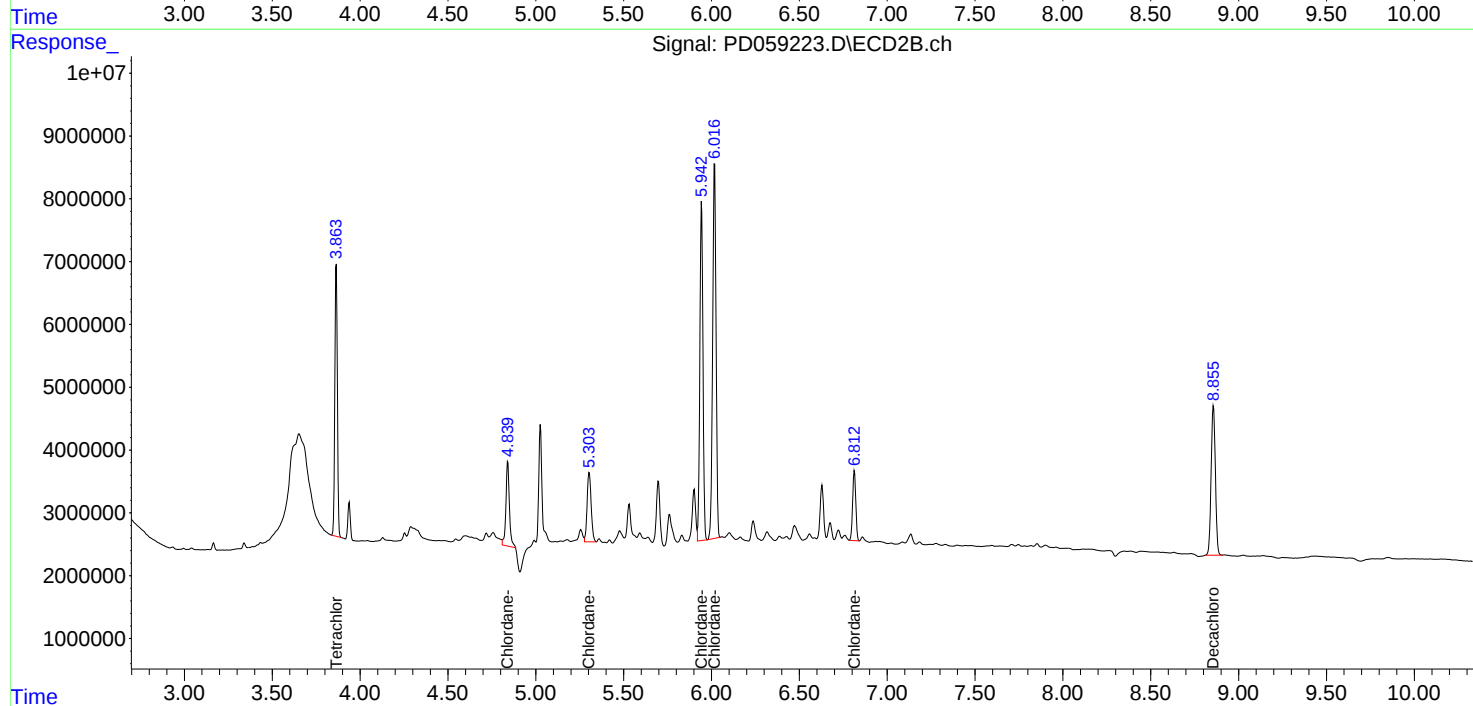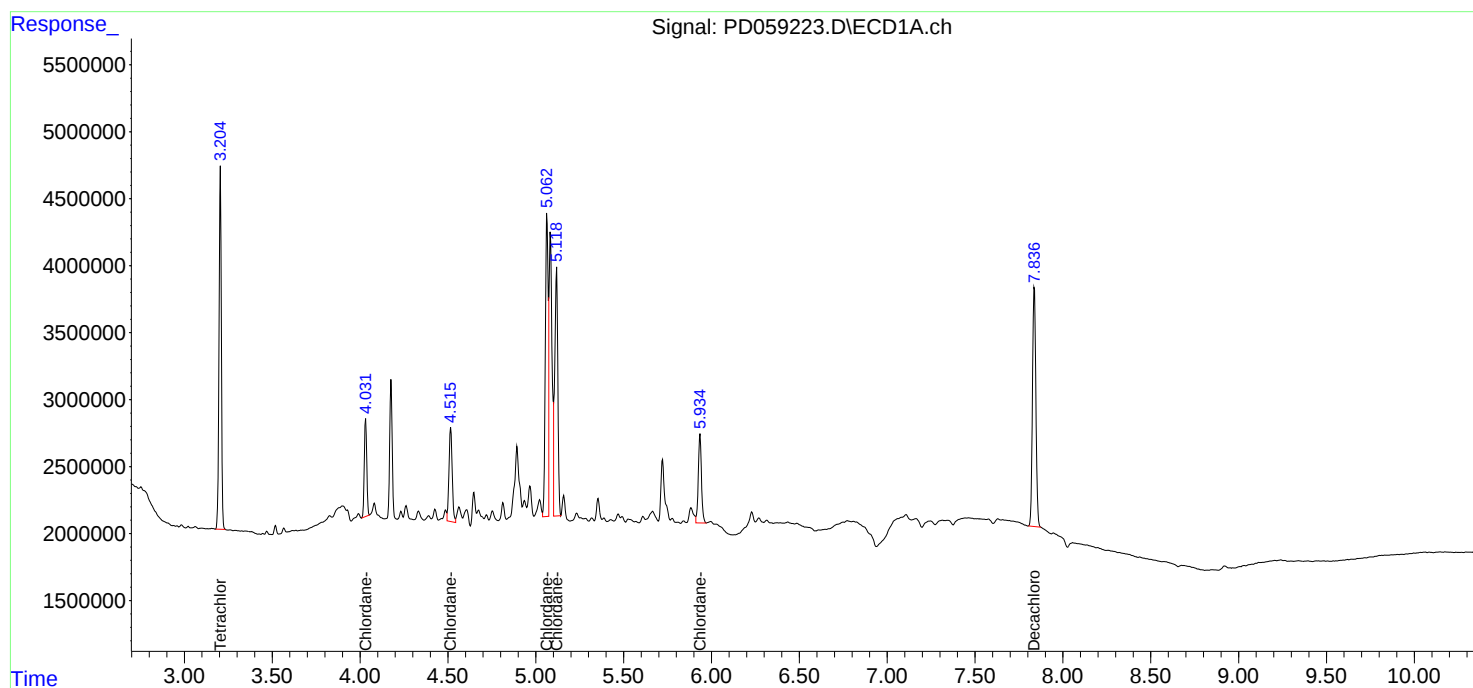


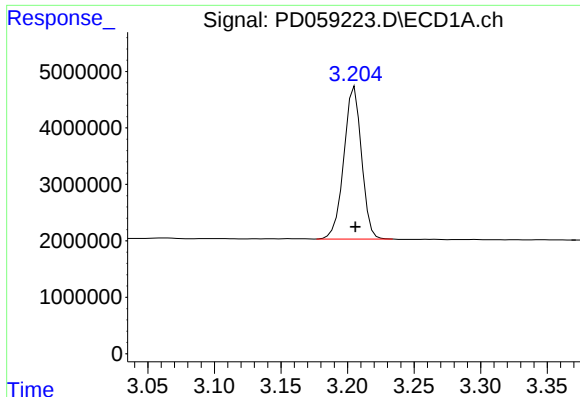

#1 Tetrachloro-m-xylene


R.T.: 3.205 min
Delta R.T.: 0.000 min
Response: 24935953
Conc: 24.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

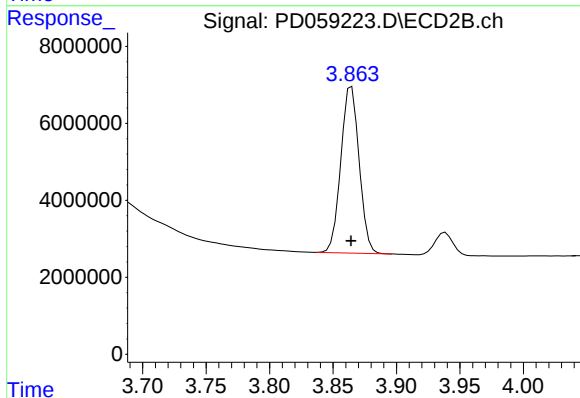


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 43395474
Conc: 24.83 ng/ml

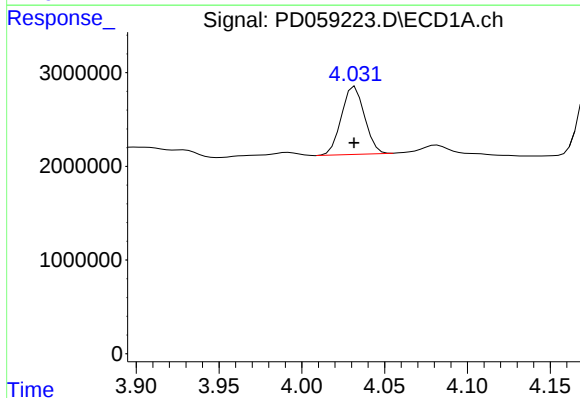


#23 Chlordane-1

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 7034650
Conc: 242.26 ng/ml

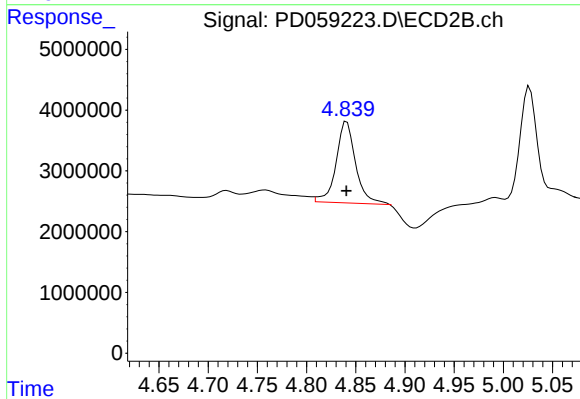

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 18514834
Conc: 264.08 ng/ml

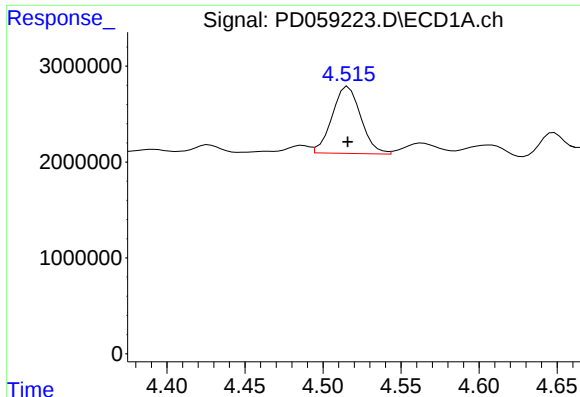

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 8978285
Conc: 259.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

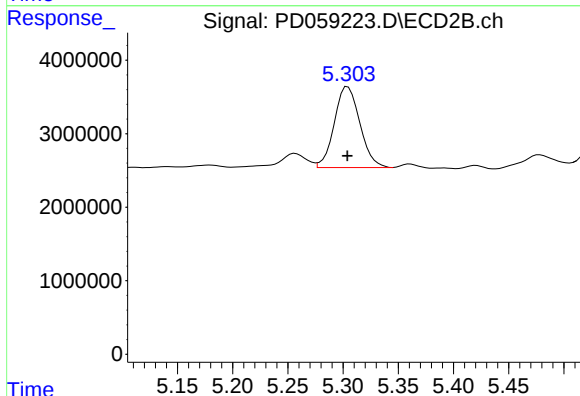


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 17734395
Conc: 261.68 ng/ml

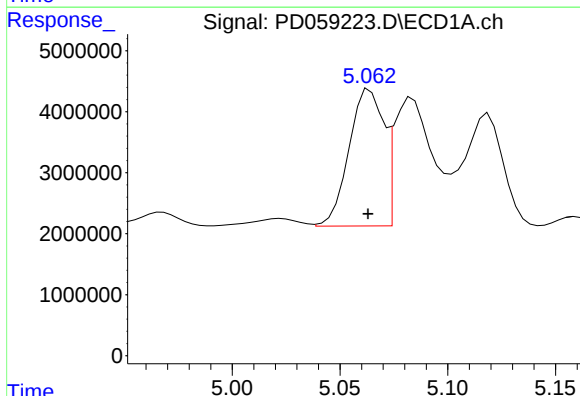


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 24959032
Conc: 239.30 ng/ml

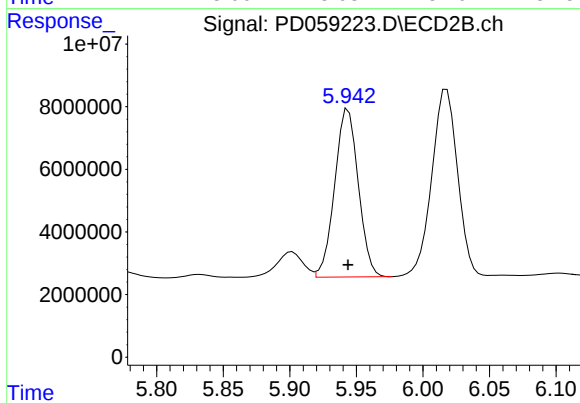

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 66413614
Conc: 243.69 ng/ml

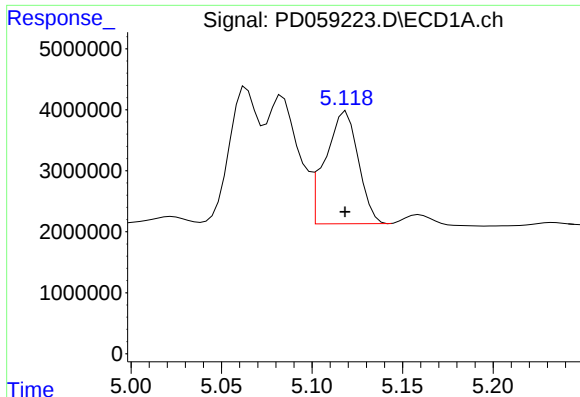

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 23355580
Conc: 232.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

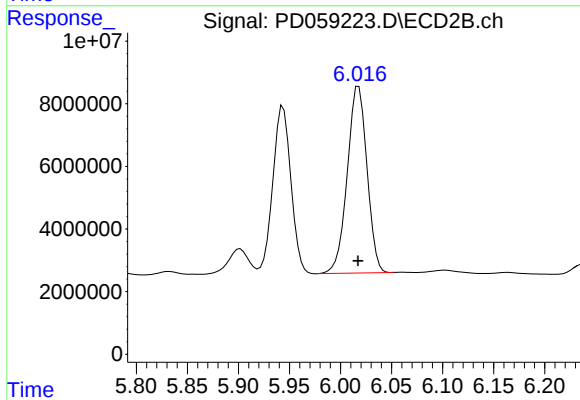


#26 Chlordane-4

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 80206189
Conc: 245.83 ng/ml

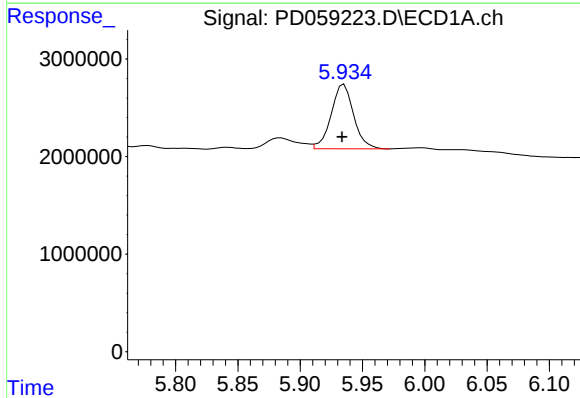


#27 Chlordane-5

R.T.: 5.935 min
Delta R.T.: 0.001 min
Response: 8302968
Conc: 239.42 ng/ml

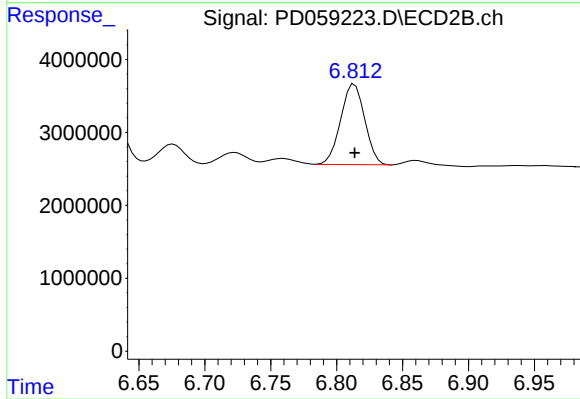

#27 Chlordane-5


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 14020621
Conc: 237.88 ng/ml

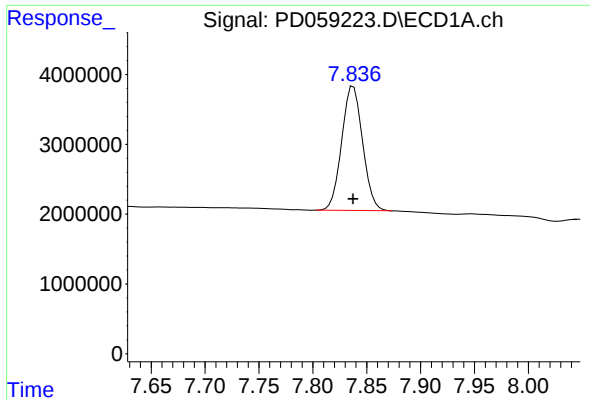

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 24057145
Conc: 25.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

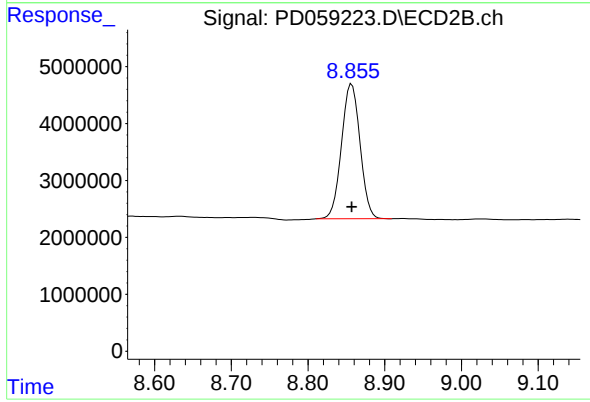

#28 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: 0.000 min
Response: 39977735
Conc: 25.81 ng/ml