

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
 Data File : PD059231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 20:47
 Operator : DD\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD091620CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 04:32:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:41:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	50310348	86372955	55.820	51.124
28)	SA Decachlor...	7.838	8.857	46846028	77702624	50.286	49.671
Target Compounds							
23)	Chlordane-1	4.032	4.841	14433823	30592542	500.337	436.100
24)	Chlordane-2	4.517	5.304	16161078	32873015	468.913	457.223
25)	Chlordane-3	5.064	5.944	49789370	131.8E6	487.766	493.871
26)	Chlordane-4	5.119	6.017	47222224	158.1E6	485.737	493.230
27)	Chlordane-5	5.935	6.814	16490007	28694837	484.974	500.918



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091620\
Data File : PD059231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 20:47
Operator : DD\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD091620CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 04:32:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:41:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

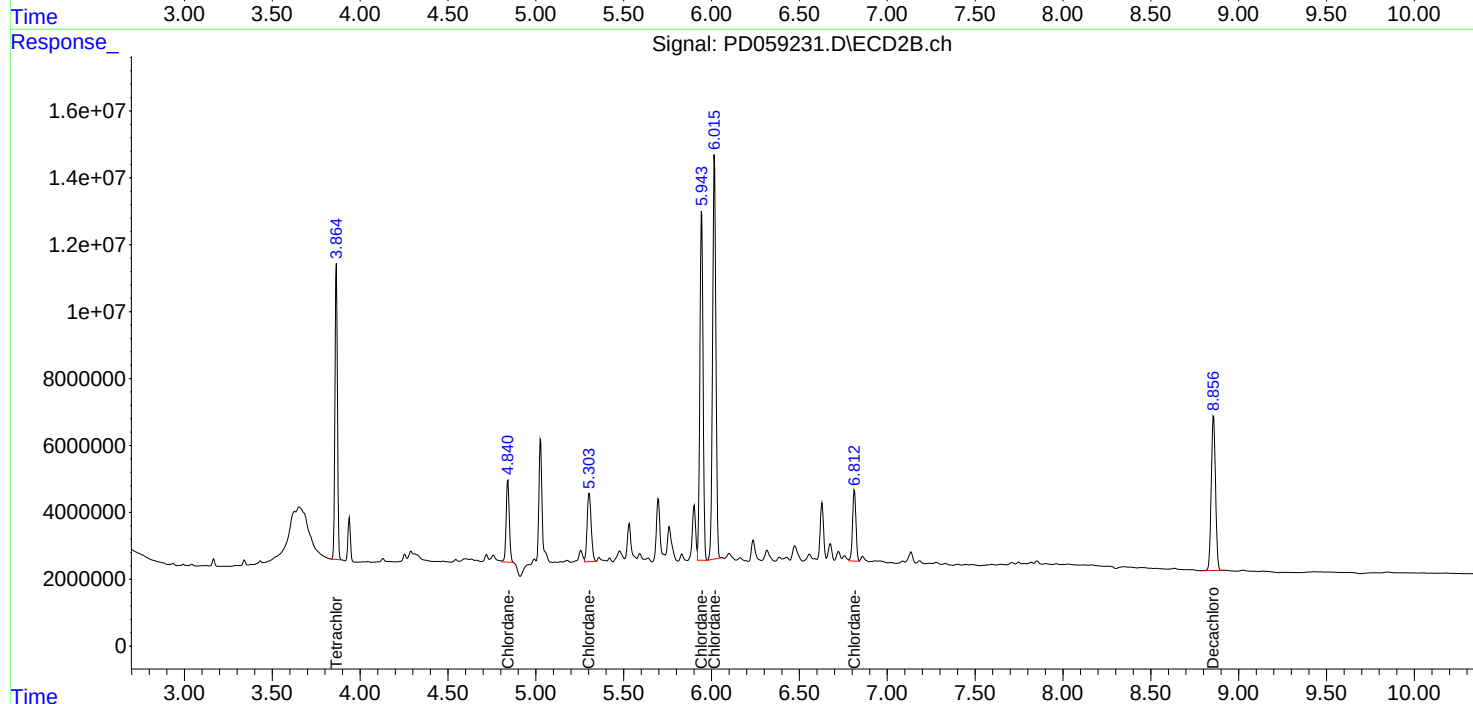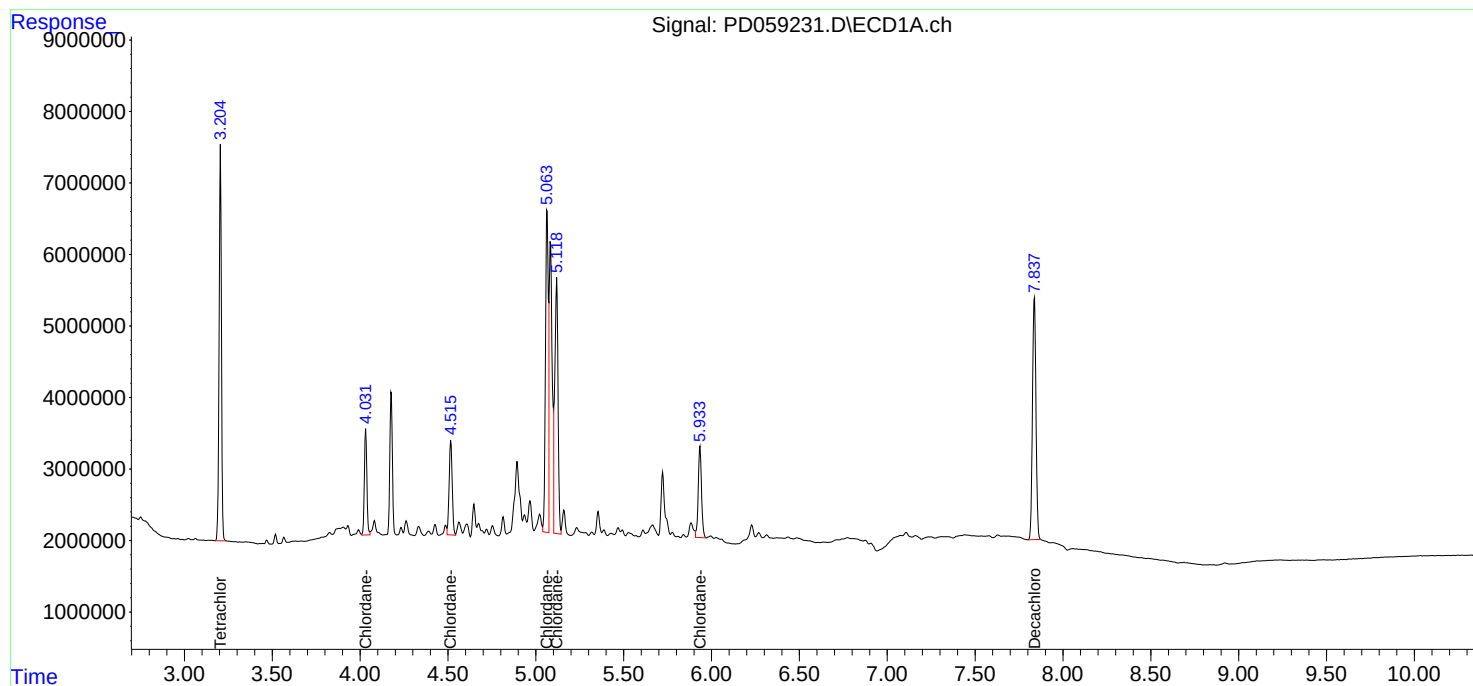


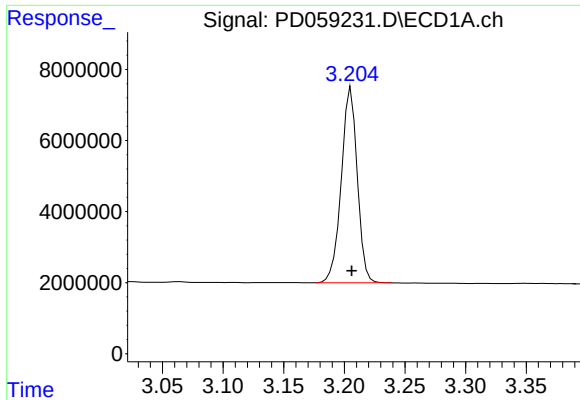

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 50310348
Conc: 55.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091620CHLOR

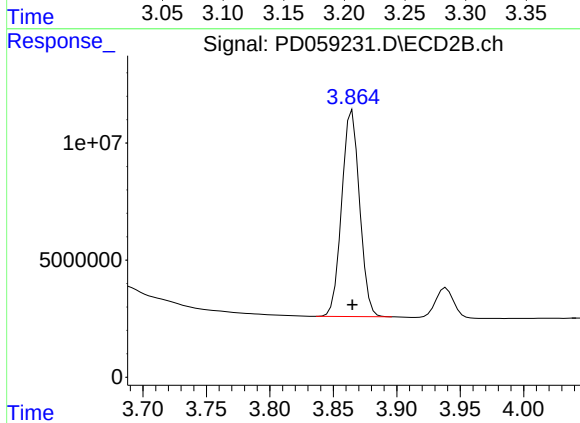


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 86372955
Conc: 51.12 ng/ml

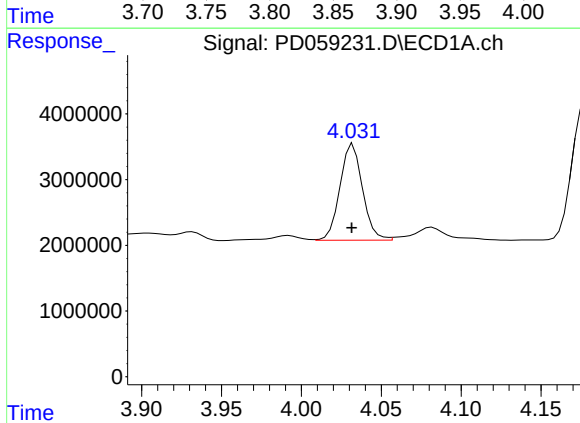


#23 Chlordane-1

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 14433823
Conc: 500.34 ng/ml

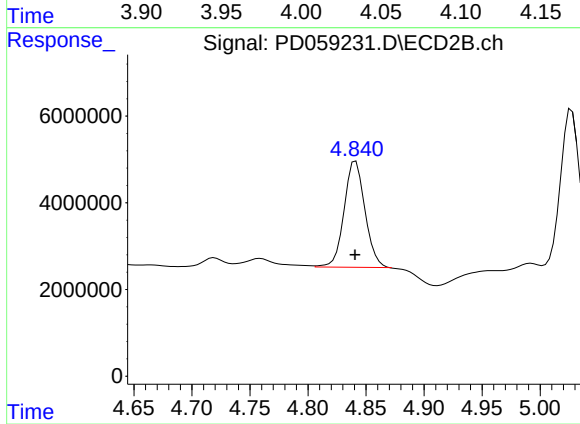

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 30592542
Conc: 436.10 ng/ml

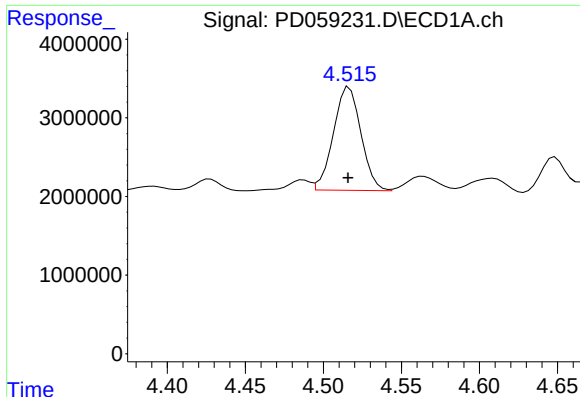

#24 Chlordane-2


R.T.: 4.517 min
Delta R.T.: 0.000 min
Response: 16161078
Conc: 468.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091620CHLOR

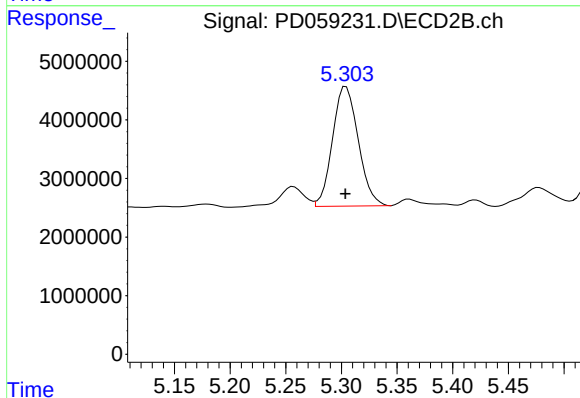


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 32873015
Conc: 457.22 ng/ml

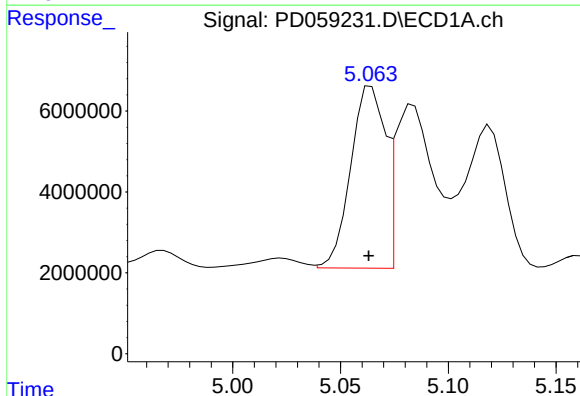


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.001 min
Response: 49789370
Conc: 487.77 ng/ml

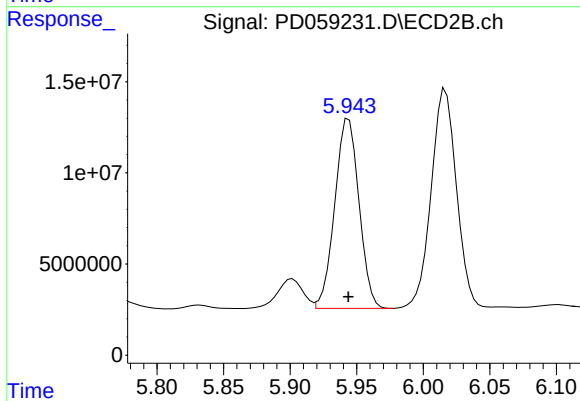

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 131841548
Conc: 493.87 ng/ml

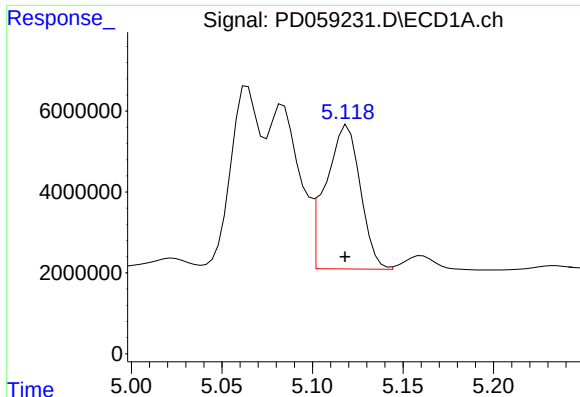

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.001 min
Response: 47222224
Conc: 485.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091620CHLOR

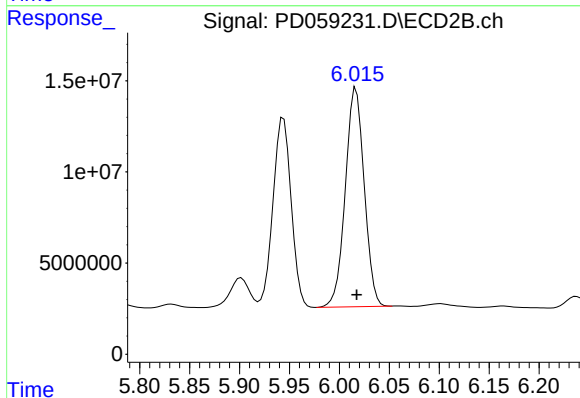


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 158121135
Conc: 493.23 ng/ml

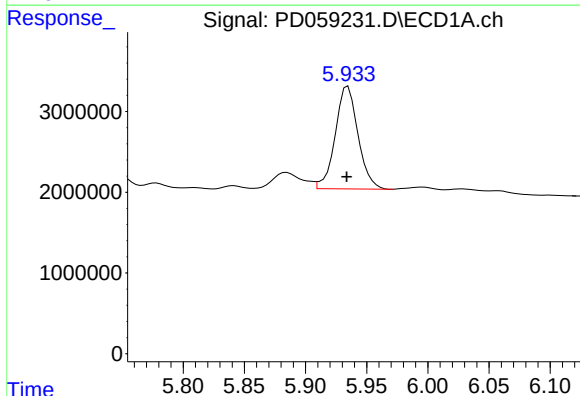


#27 Chlordane-5

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 16490007
Conc: 484.97 ng/ml

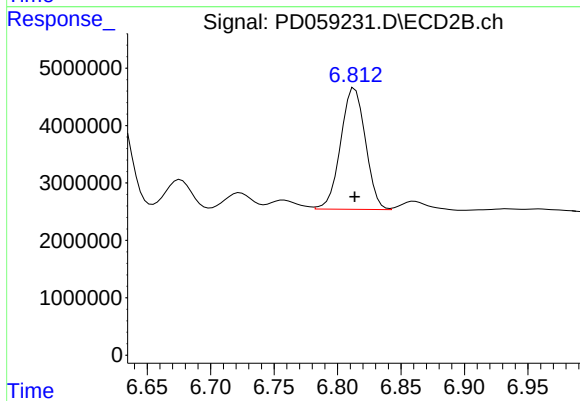

#27 Chlordane-5


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 28694837
Conc: 500.92 ng/ml

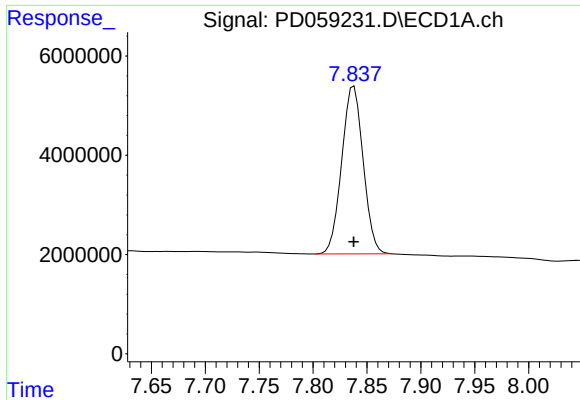

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 46846028
Conc: 50.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD091620CHLOR

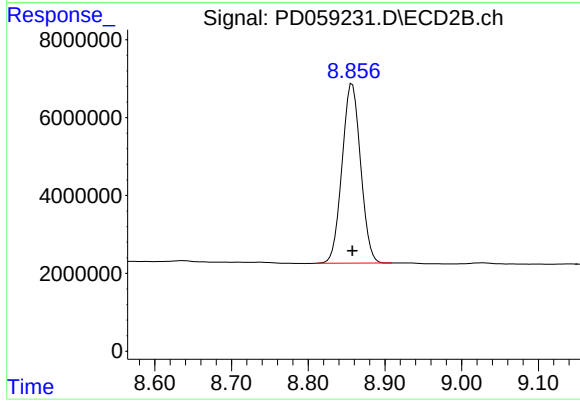

#28 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: 0.000 min
Response: 77702624
Conc: 49.67 ng/ml