


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

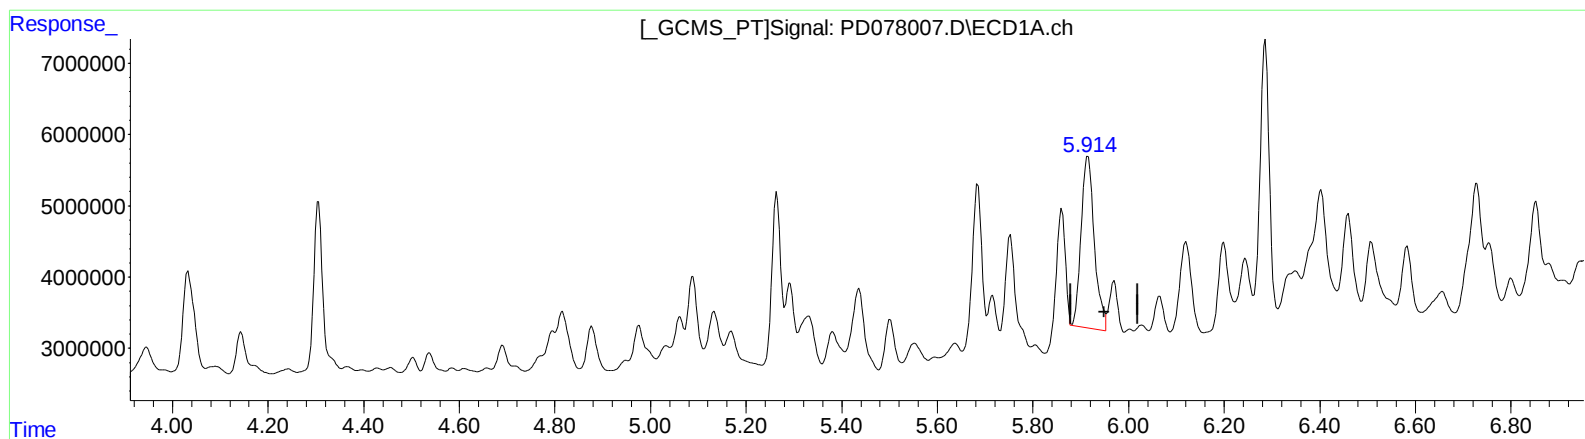


(10) trans-Chlordane (B)
5.914min 12.555 ng/ml m
response 46745524

(10) trans-Chlordane #2 (B)
4.939min 7.241 ng/ml m
response 14460158

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

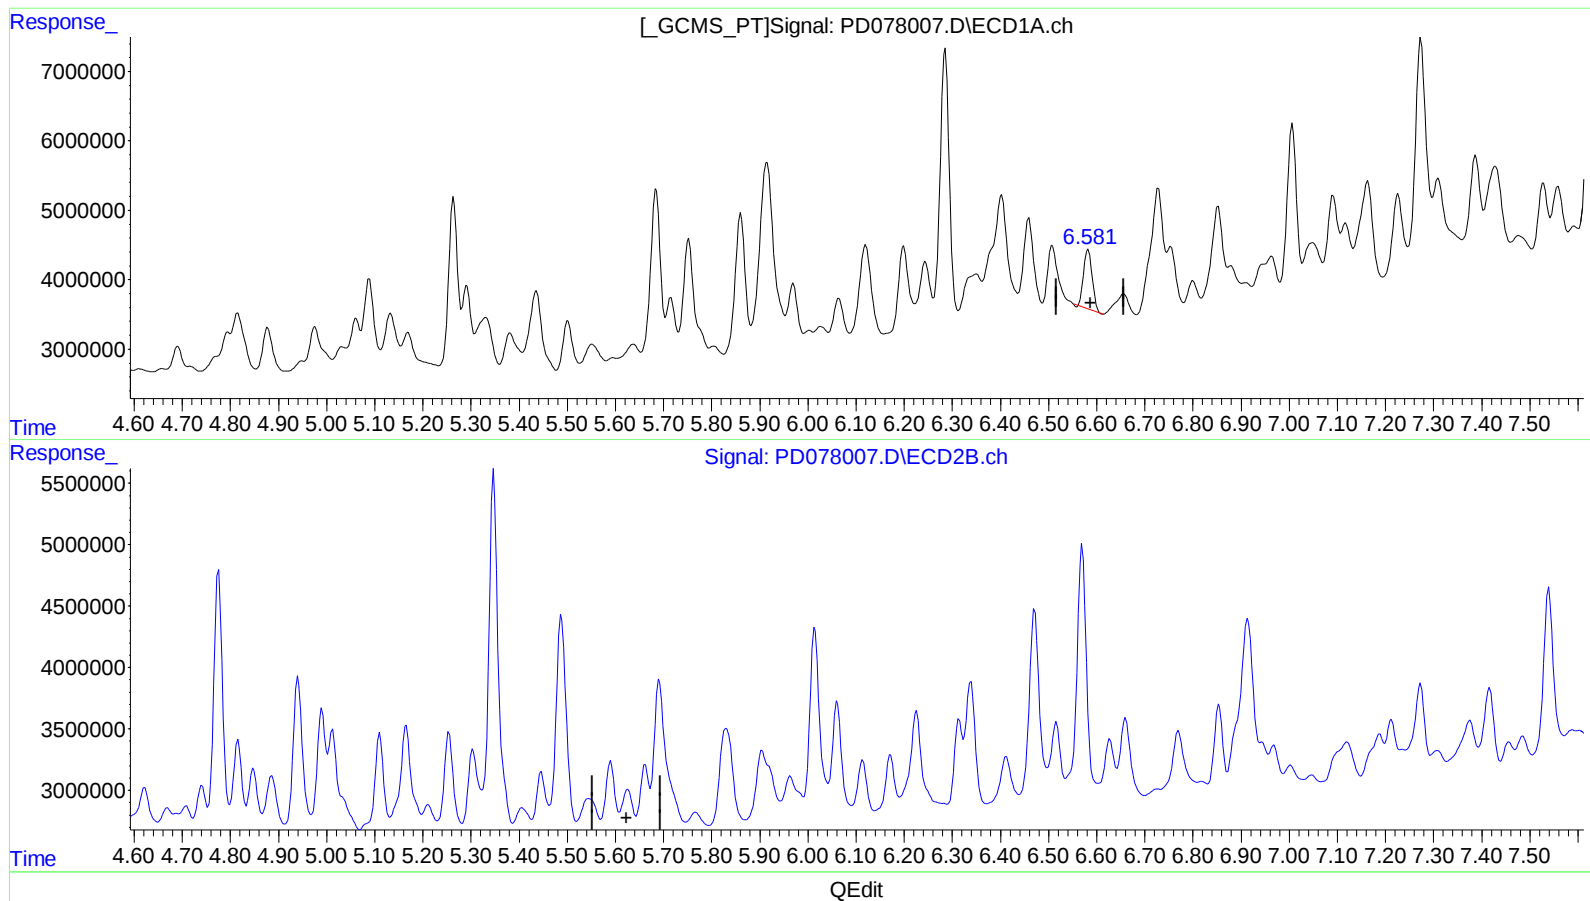

(14) Endrin (MA)

6.583min 3.401 ng/ml

response 10491520

(14) Endrin #2 (MA)


5.626min -0.786 ng/ml

response -1437057

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

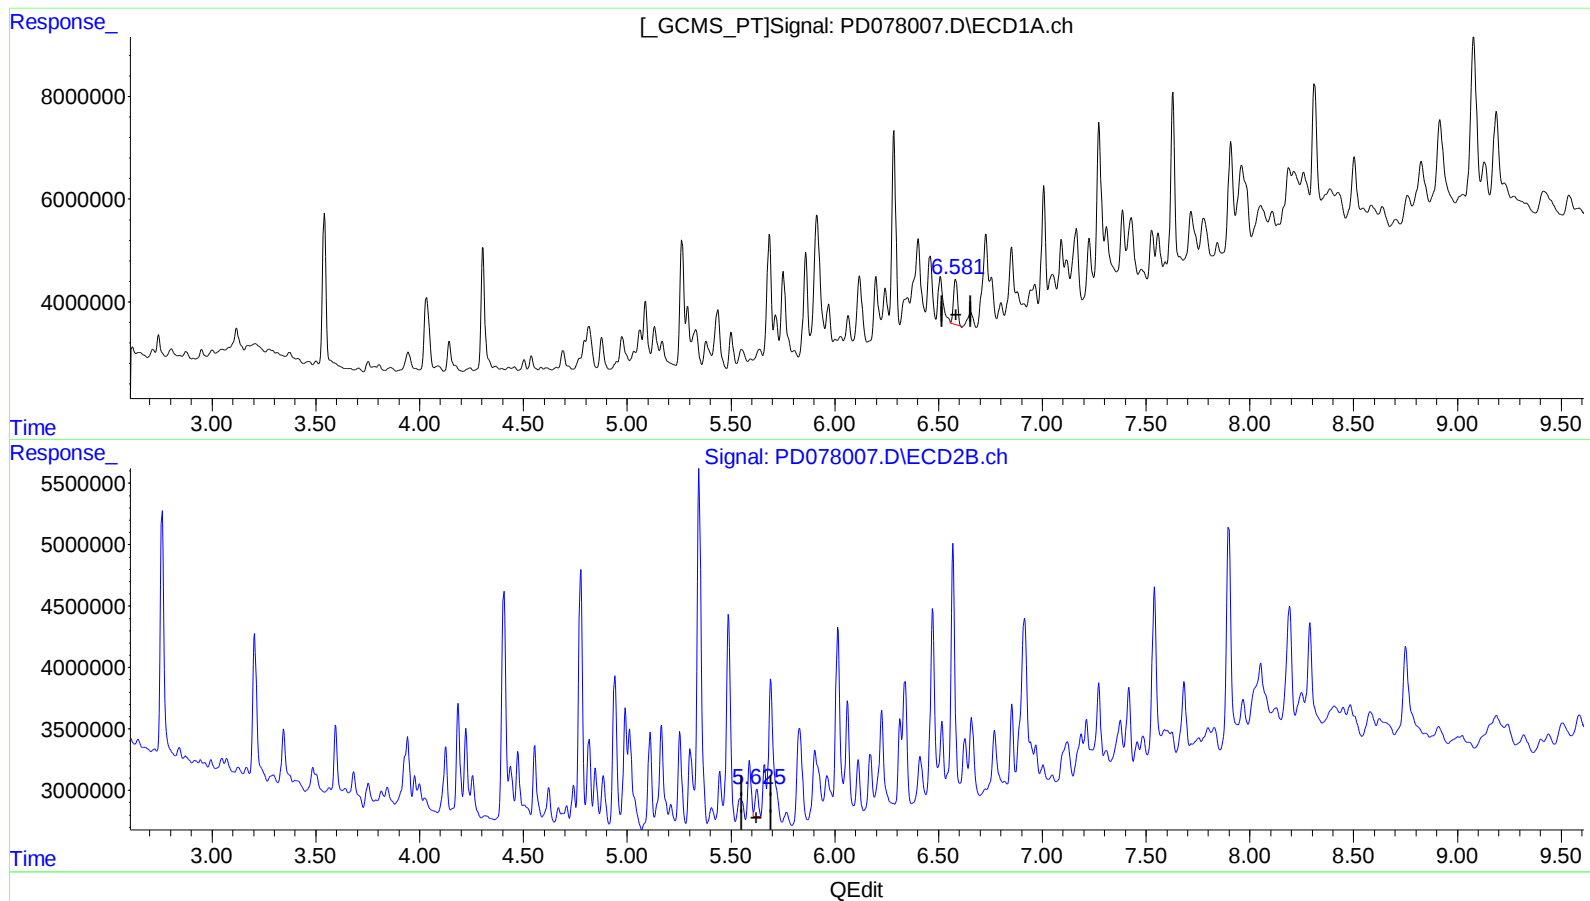

(14) Endrin (MA)

6.581min 3.618 ng/ml m

response 11163745

(14) Endrin #2 (MA)



5.625min 1.452 ng/ml m

response 2655115

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

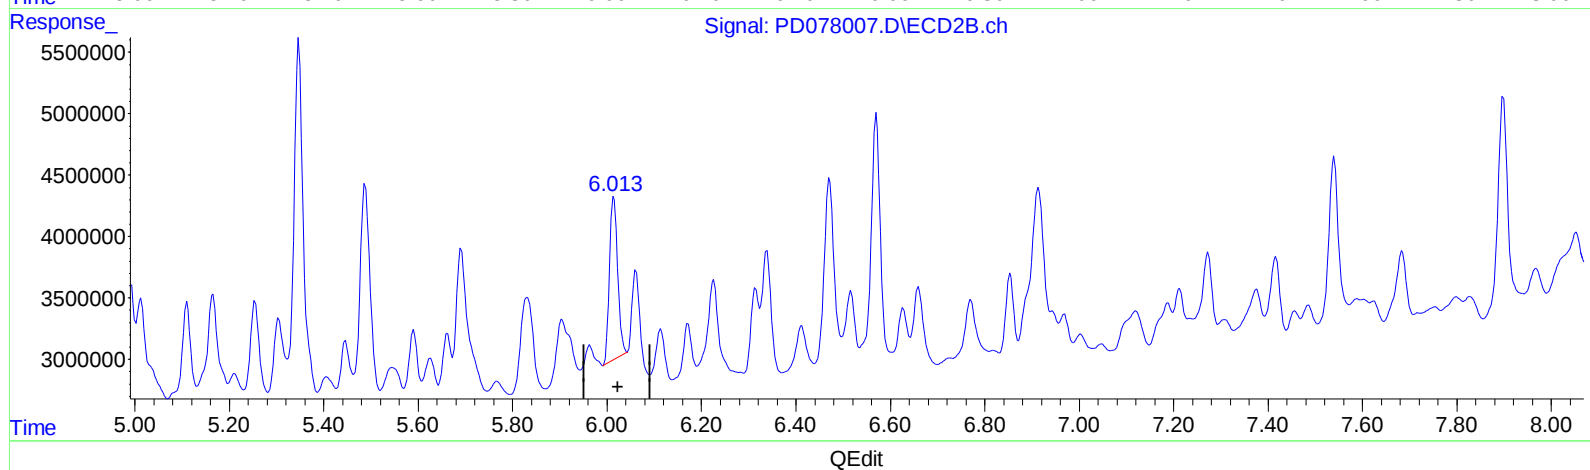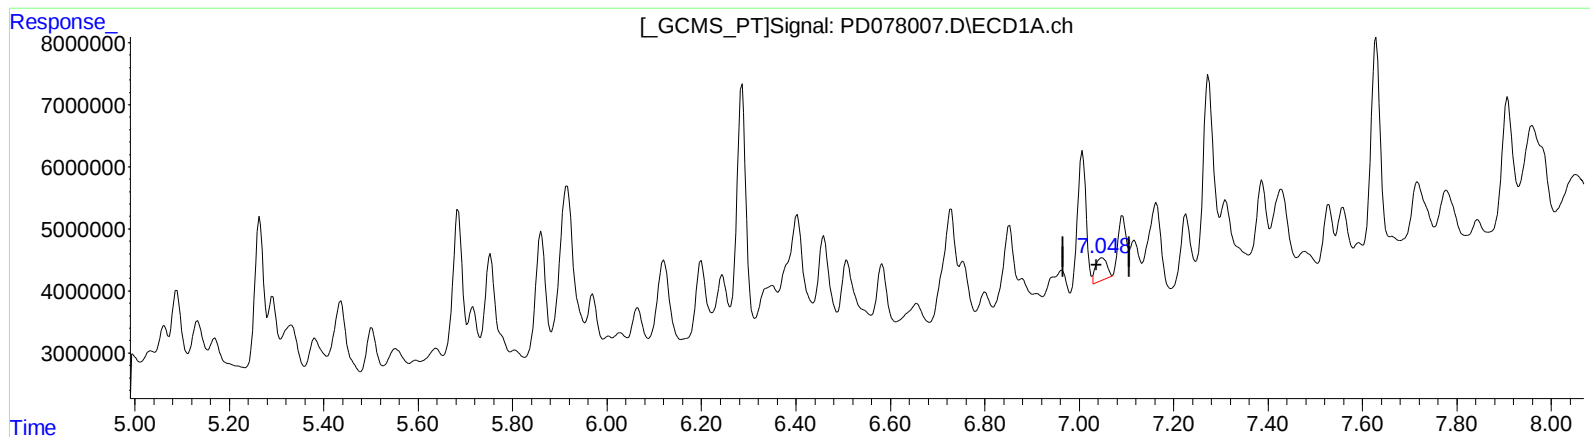

(17) 4,4'-DDT (MA)

7.049min 2.202 ng/ml

response 6032121

(17) 4,4'-DDT #2 (MA)


6.015min 11.334 ng/ml

response 16019252

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

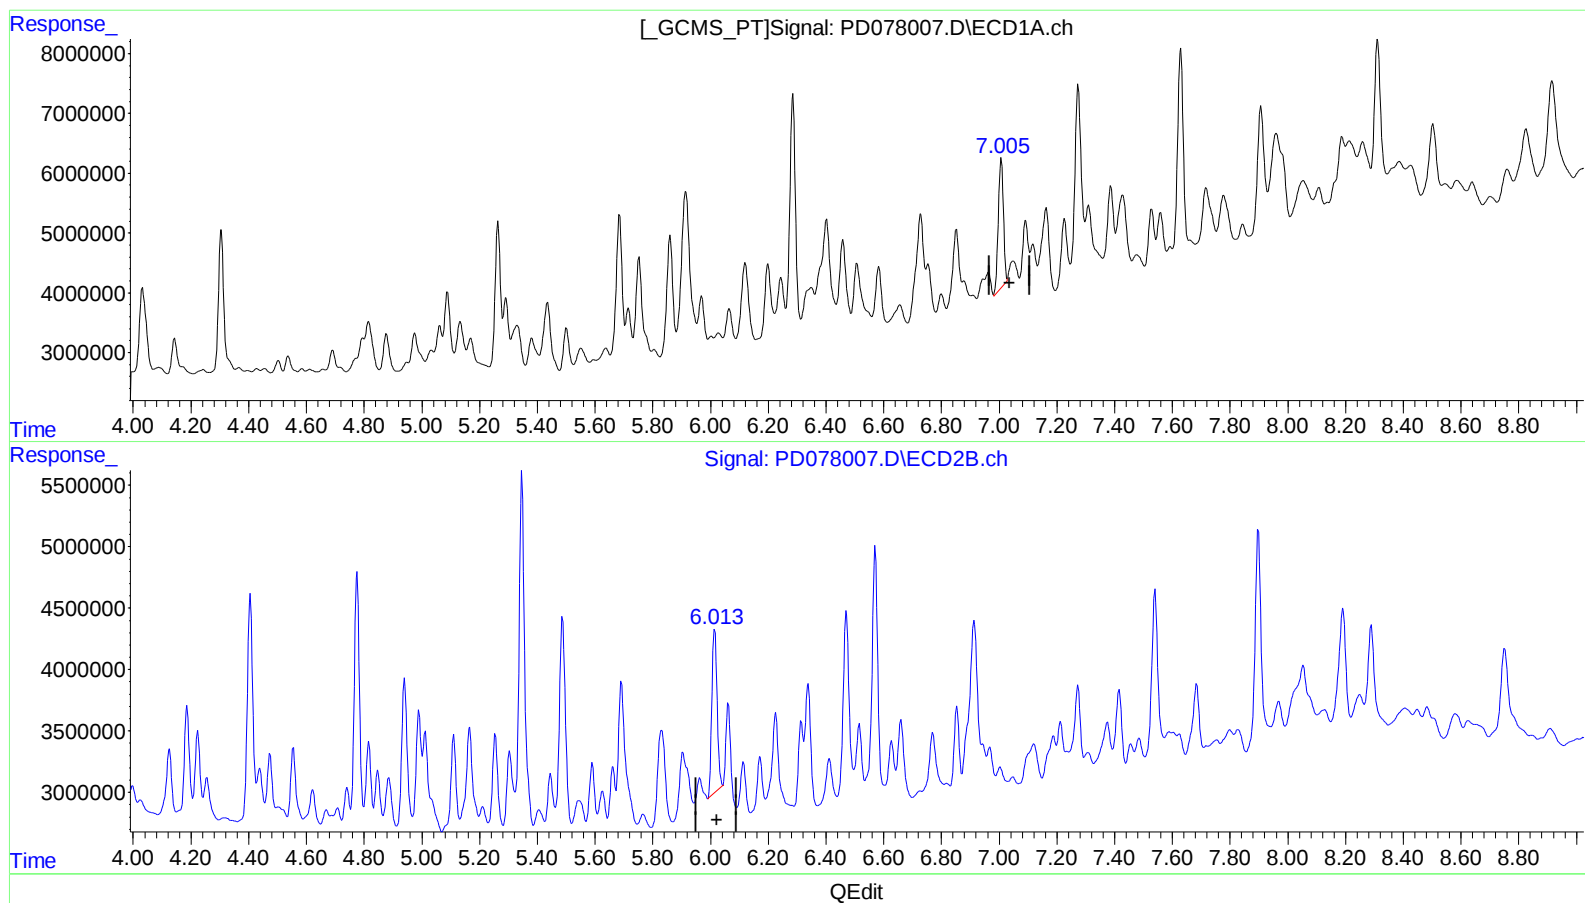

(17) 4,4'-DDT (MA)

7.005min 9.777 ng/ml m

response 26787388

(17) 4,4'-DDT #2 (MA)

6.015min 11.334 ng/ml

response 16019252

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
 Data File : PD078007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 10:18
 Operator : AR\AJ
 Sample : 04330-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:31:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.759	33812577	22385857	13.324	15.147
27) SA Decachlor...	9.078	7.898	56860749	23553542	18.202	14.544
Target Compounds						
5) MB Aldrin	5.264	4.224	26650828	8654225	6.384	3.861 #
10) B trans-Chl...	5.914f	4.939	46745524	14460158	12.555m	7.241m#
14) MA Endrin	6.581	5.625	11163745	2655115	3.618m	1.452m#
17) MA 4,4'-DDT	7.005	6.015	26787388	16019252	9.777m	11.334
19) B Endosulfa...	7.163	6.314	17861419	7503398	5.894	4.541

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

