

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
 Data File : PD078007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 10:18
 Operator : AR\AJ
 Sample : 04330-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYX7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/18/2023
 Supervised By : Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:31:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.759	33812577	22385857	13.324	15.147
2) SA Decachlor...	9.078	7.898	56860749	23553542	18.202	14.544
Target Compounds						
5) MB Aldrin	5.264	4.224	26650828	8654225	6.384	3.861 #
14) MA Endrin	6.581	5.625	11163745	2655115	3.618m	1.452m#
17) MA 4,4'-DDT	7.005	6.015	26787388	16019252	9.777m	11.334
19) B Endosulfa...	7.163	6.314	17861419	7503398	5.894	4.541

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 10:18
Operator : AR\AJ
Sample : 04330-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:31:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

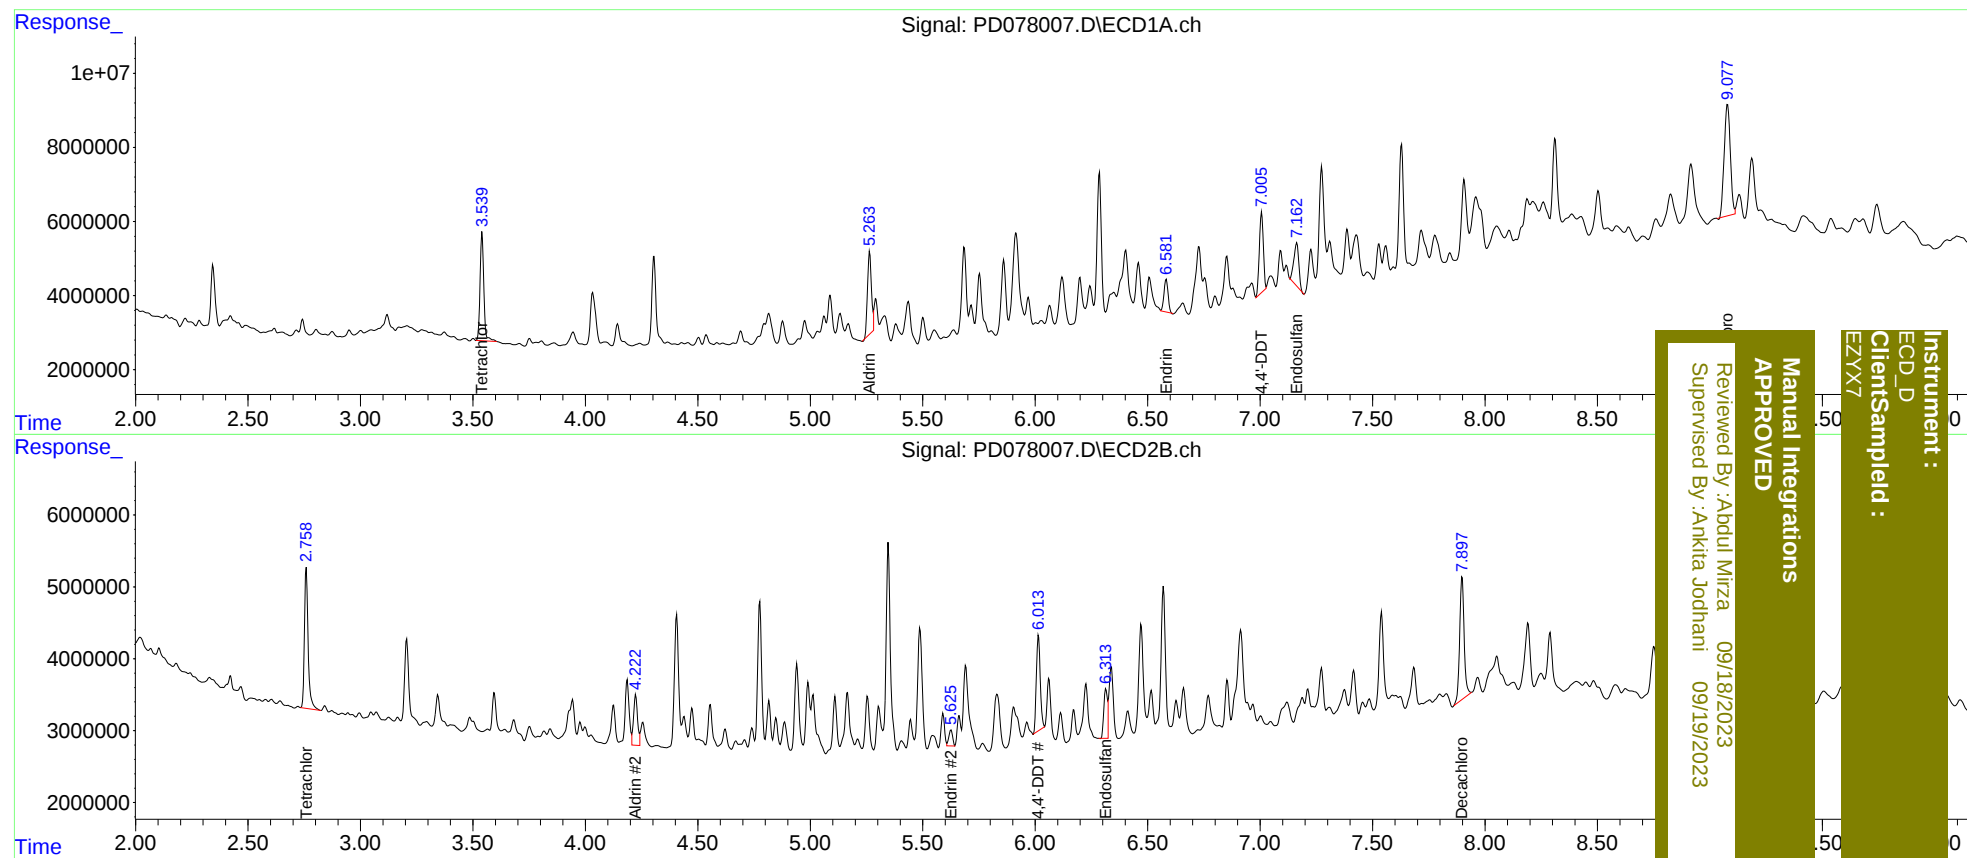

Reviewed By: Abdul Mirza 09/18/2023
Supervised By: Ankita Jodhani 09/19/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EZYX7