

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
 Data File : PD078012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 11:24
 Operator : AR\AJ
 Sample : 04330-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYF9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/18/2023
 Supervised By : Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 05:04:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.759	36481544	23887623	14.376	16.163
2)	SA Decachlor...	9.083	7.899	40922759	20886698	13.100	12.897
Target Compounds							
10)	B trans-Chl...	5.918	4.965	2664574	778861	0.716m	0.390m#
12)	B 4,4'-DDE	6.200	5.213	10284478	7118936	2.901	3.747 #
16)	A 4,4'-DDD	6.720	5.768	4993109	3280432	1.877	2.437 #
17)	MA 4,4'-DDT	7.035	6.017	1271445	1091350	0.464m	0.772 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 11:24
Operator : AR\AJ
Sample : 04330-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 05:04:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

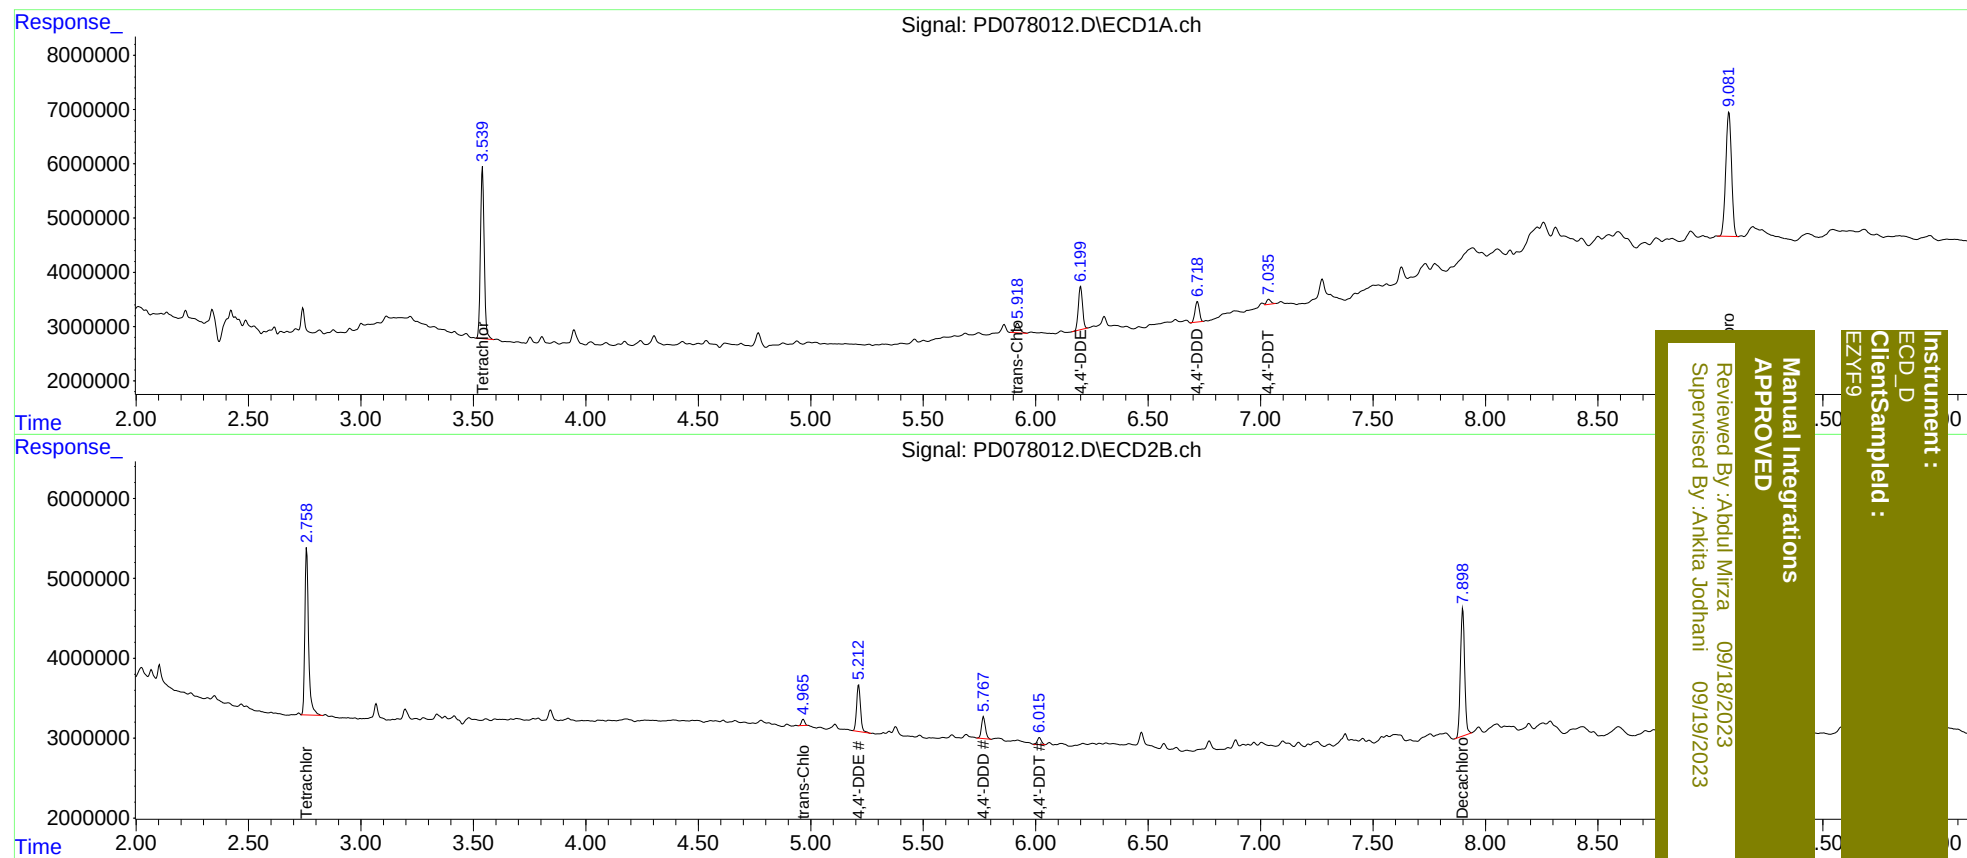

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/18/2023
Supervised By: Ankita Jodhani 09/19/2023

Instrument :
ECD_D
Client Sampled :
EZYF9